
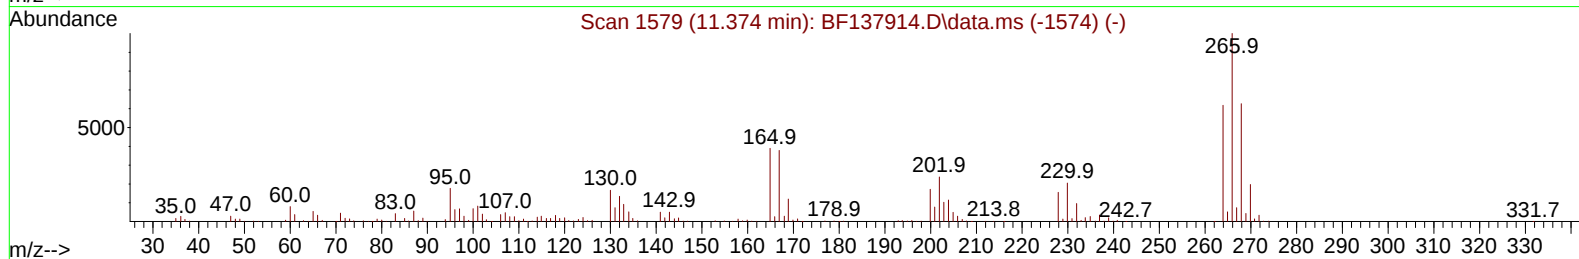
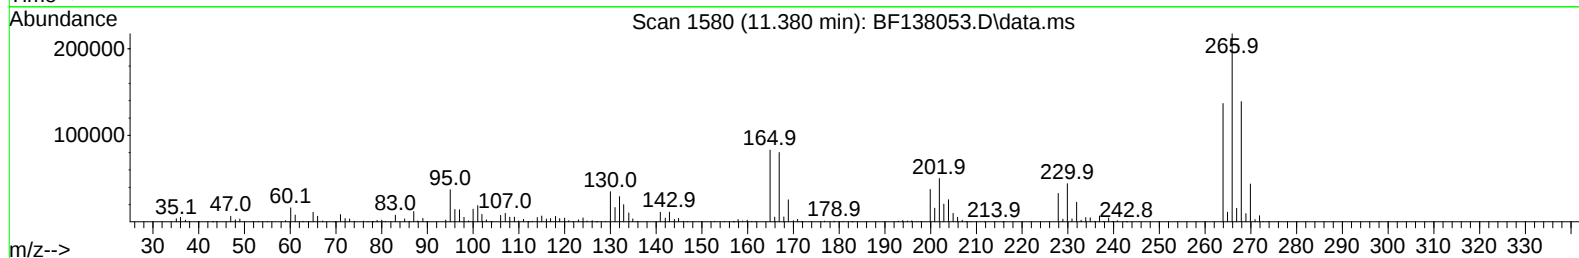


Quant Time: May 29 12:11:44 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF051424.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 15 04:12:16 2024
Response via : Initial Calibration

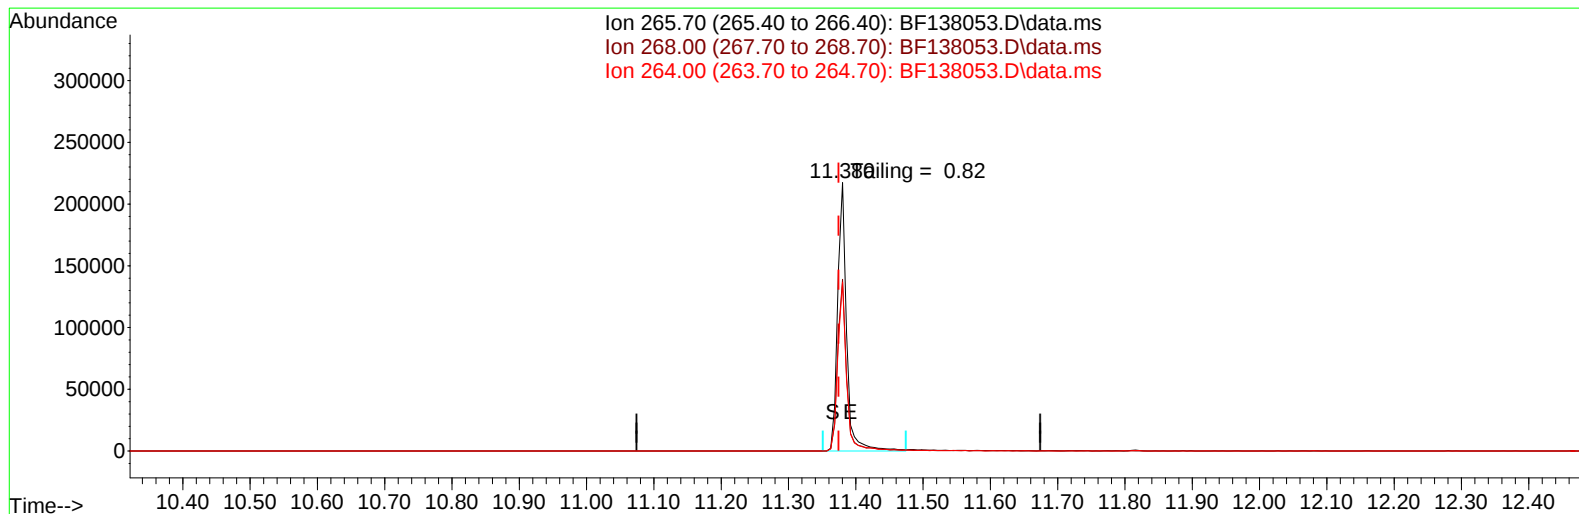

TIC: BF138053.D\data.ms

(70) Pentachlorophenol (C)




11.380min (+ 0.006) 524430.47 ng

response	201022
----------	--------

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.60	63.99
264.00	61.80	62.96
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052924\
Data File : BF138053.D
Acq On : 29 May 2024 11:27
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 29 12:11:44 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF051424.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 15 04:12:16 2024
Response via : Initial Calibration

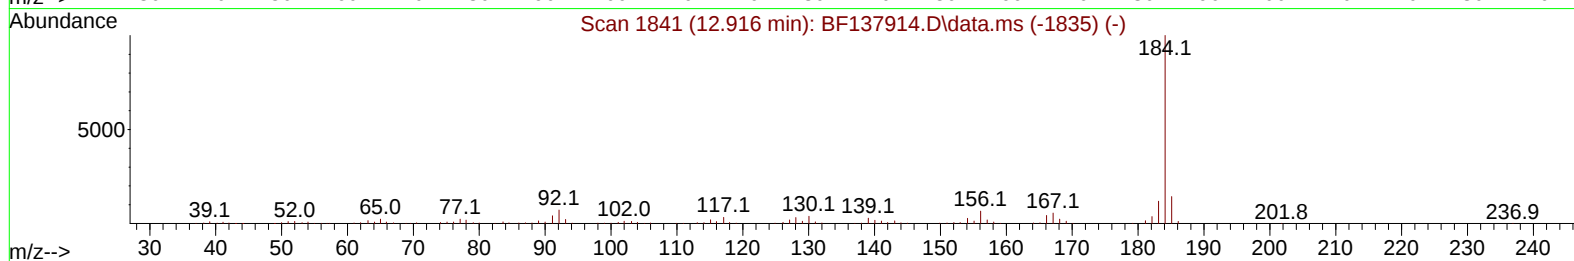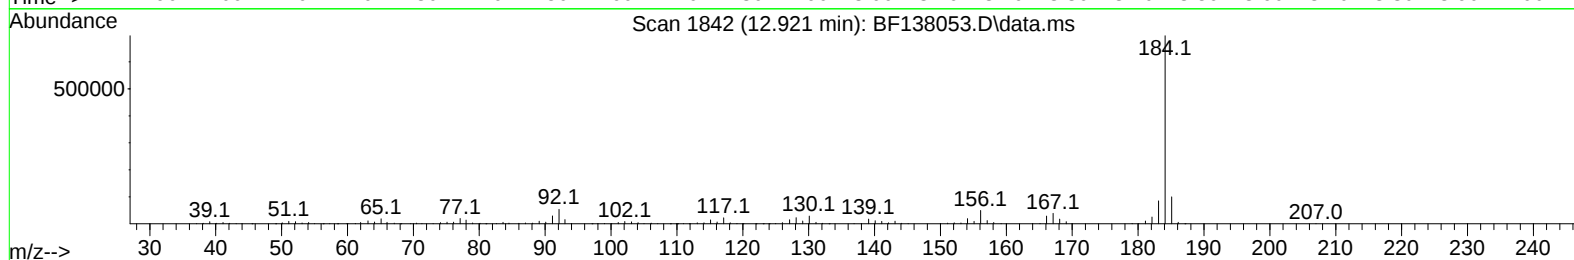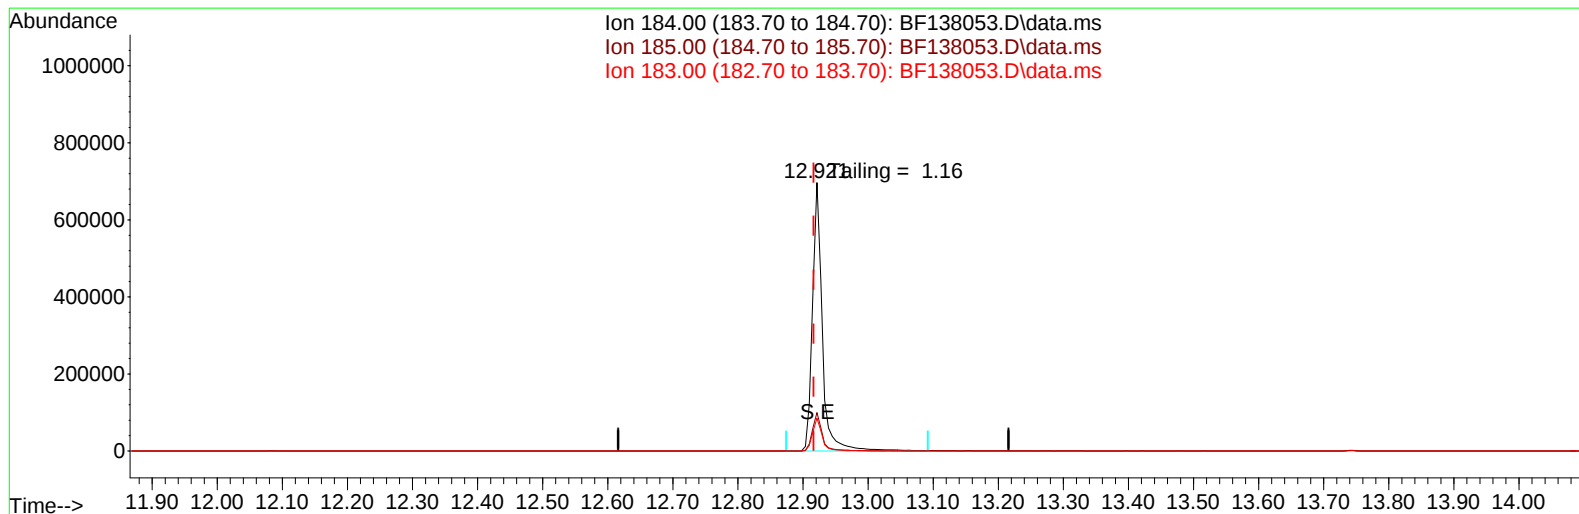

TIC: BF138053.D\data.ms

(77) Benzidine

12.921min (+ 0.005) 365678.65 ng

response 735969

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.30	14.30
183.00	11.90	12.22
0.00	0.00	0.00