


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052924\
Data File : BF138053.D
Acq On : 29 May 2024 11:27
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF051424.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed May 15 04:12:16 2024

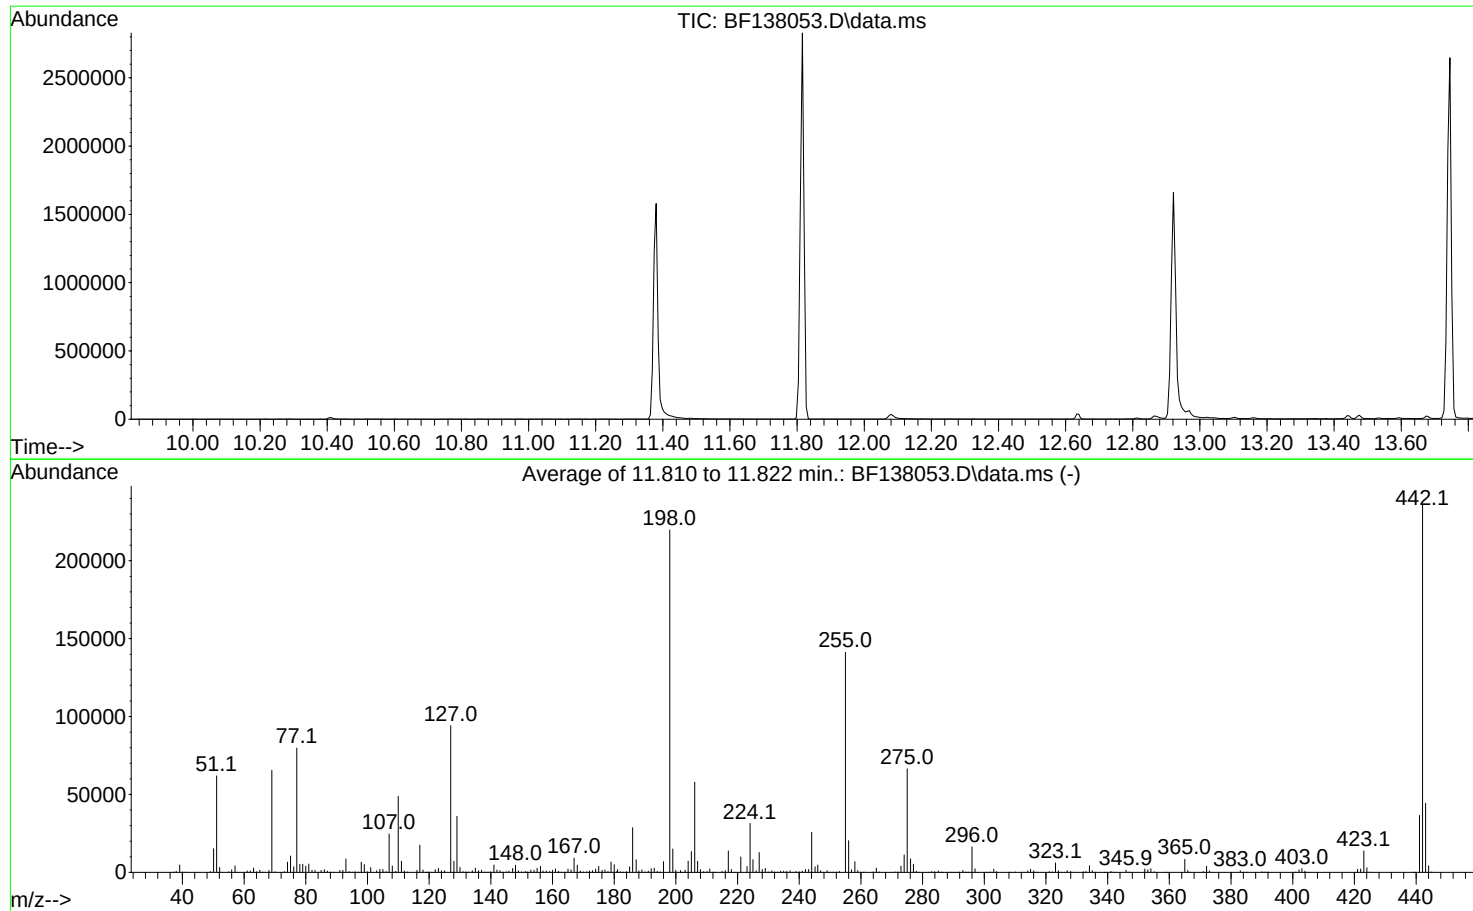

AutoFind: Scans 1653, 1654, 1655; Background Corrected with Scan 1648

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	28.2	61931	PASS
68	69	0.00	2	1.9	1225	PASS
69	198	0.00	100	29.8	65496	PASS
70	69	0.00	2	0.6	402	PASS
127	198	10	80	42.9	94219	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	219712	PASS
199	198	5	9	6.8	14984	PASS
275	198	10	60	30.3	66475	PASS
365	198	1	100	3.8	8358	PASS
441	198	0.01	100	16.6	36515	PASS
442	442	50	100	100.0	236083	PASS
443	442	15	24	18.8	44299	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
5/29/2024	BNA_F	<u>BF138053.D</u>
Compound Name	Response	Retention Time
DDT	465053	13.745
DDD	9996	13.439
DDE	1638	13.104
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
11634	476687	2.44

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052924\
Data File : BF138053.D
Acq On : 29 May 2024 11:27
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: May 29 12:11:44 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF051424.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 15 04:12:16 2024
Response via : Initial Calibration

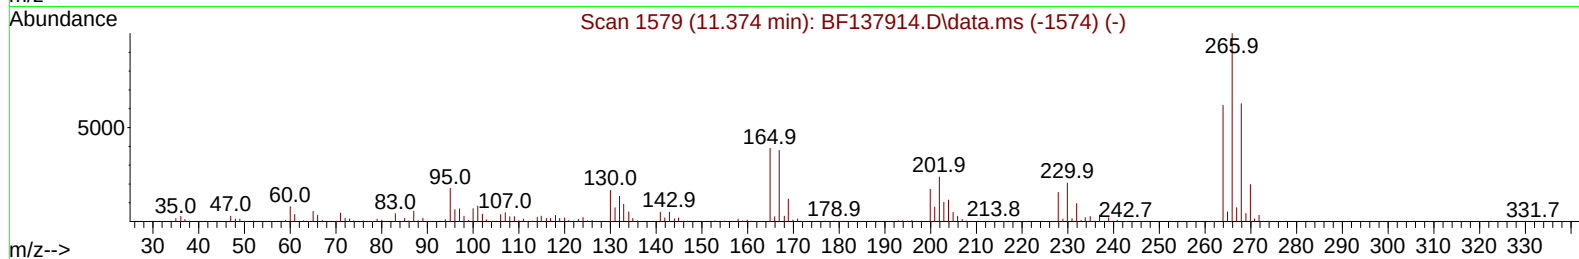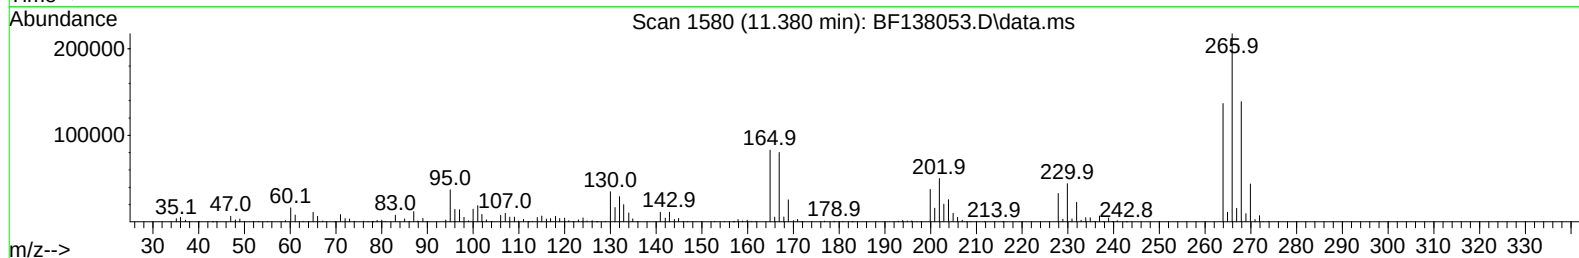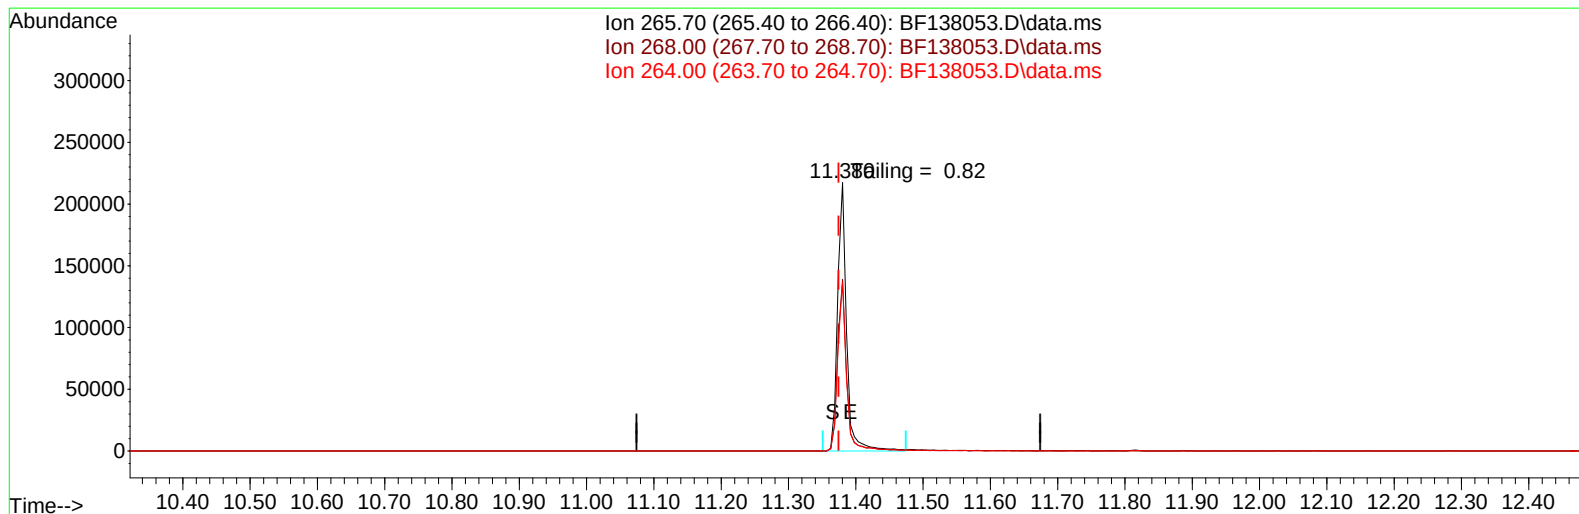

TIC: BF138053.D\data.ms

(70) Pentachlorophenol (C)

11.380min (+ 0.006) 524430.47 ng




response 201022

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.60	63.99
264.00	61.80	62.96
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052924\
Data File : BF138053.D
Acq On : 29 May 2024 11:27
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: May 29 12:11:44 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF051424.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 15 04:12:16 2024
Response via : Initial Calibration

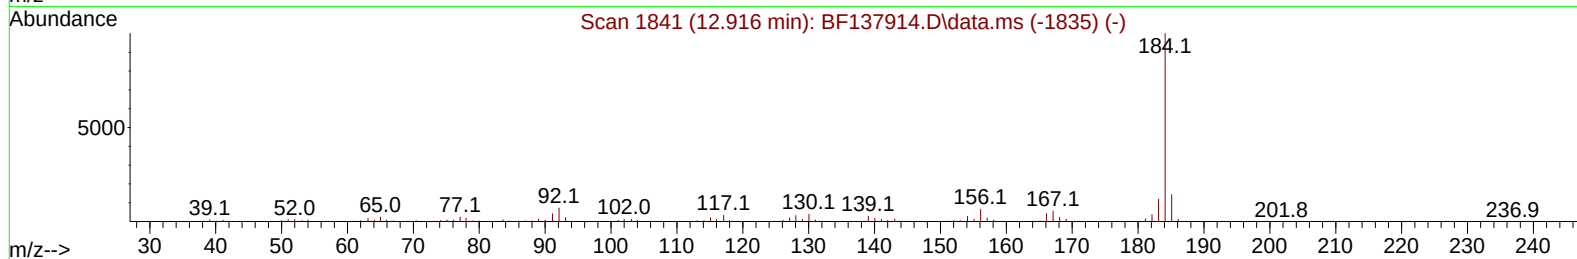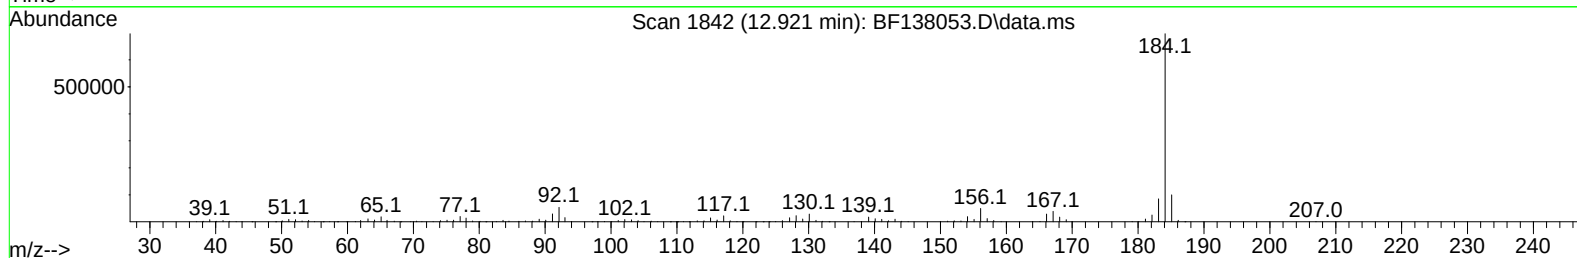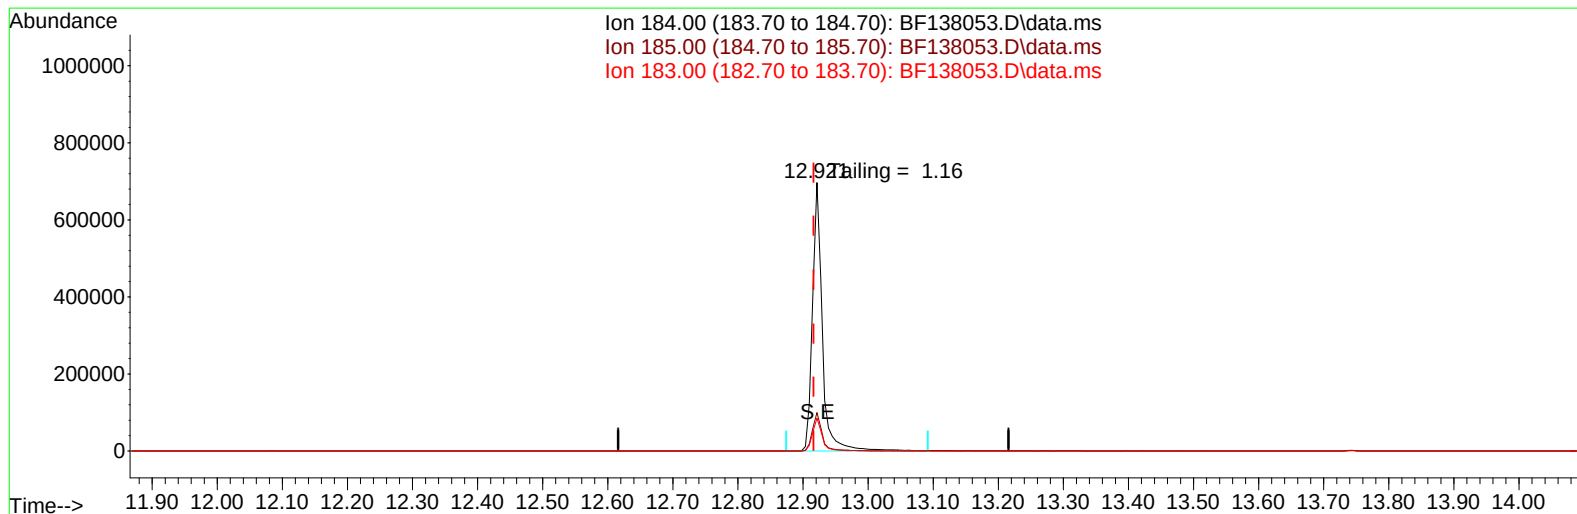

TIC: BF138053.D\data.ms

(77) Benzidine

12.921min (+ 0.005) 365678.65 ng

response 735969

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.30	14.30
183.00	11.90	12.22
0.00	0.00	0.00