

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF053015\
 Data File : BF079607.D
 Acq On : 30 May 2015 17:16
 Operator : TP/IZ
 Sample : G2420-14
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PENRD8.7(5)

Quant Time: May 31 05:46:31 2015
 Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF052615.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri May 29 17:35:14 2015
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.94	152	62702	20.00	ng	-0.02
21) Naphthalene-d8	8.51	136	254118	20.00	ng	-0.02
38) Acenaphthene-d10	10.67	164	119625	20.00	ng	-0.03
63) Phenanthrene-d10	12.50	188	219996	20.00	ng	-0.03
75) Chrysene-d12	15.78	240	237497	20.00	ng	-0.06
86) Perylene-d12	17.51	264	245701	20.00	ng	-0.16
System Monitoring Compounds						
5) 2-Fluorophenol	5.21	112	376037	104.02	ng	-0.02
7) Phenol-d6	6.54	99	509963	110.67	ng	-0.02
23) Nitrobenzene-d5	7.63	82	280579	63.83	ng	-0.03
41) 2,4,6-Tribromophenol	11.66	330	139121	105.88	ng	-0.03
44) 2-Fluorobiphenyl	9.86	172	583943	69.64	ng	-0.02
78) Terphenyl-d14	14.50	244	647138	63.95	ng	-0.03
Target Compounds						
2) 1,4-Dioxane	1.66	88	152097	88.44	ng	# 100
9) Benzaldehyde	6.54	77	702	Below Cal	#	51
49) Dimethylphthalate	10.38	163	48989	5.56	ng	98
73) Di-n-butylphthalate	13.27	149	1313	Below Cal	#	78
89) Benzo(a)pyrene	17.44	252	5446	Below Cal	#	57
90) Dibenzo(a,h)anthracene	18.82	278	4193	Below Cal	#	26
91) Benzo(g,h,i)perylene	19.17	276	5915	Below Cal	#	74

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF053015\
Data File : BF079607.D
Acq On : 30 May 2015 17:16
Operator : TP/IZ
Sample : G2420-14
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PENRD8.7(5)

Quant Time: May 31 05:46:31 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF052615.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri May 29 17:35:14 2015
Response via : Initial Calibration

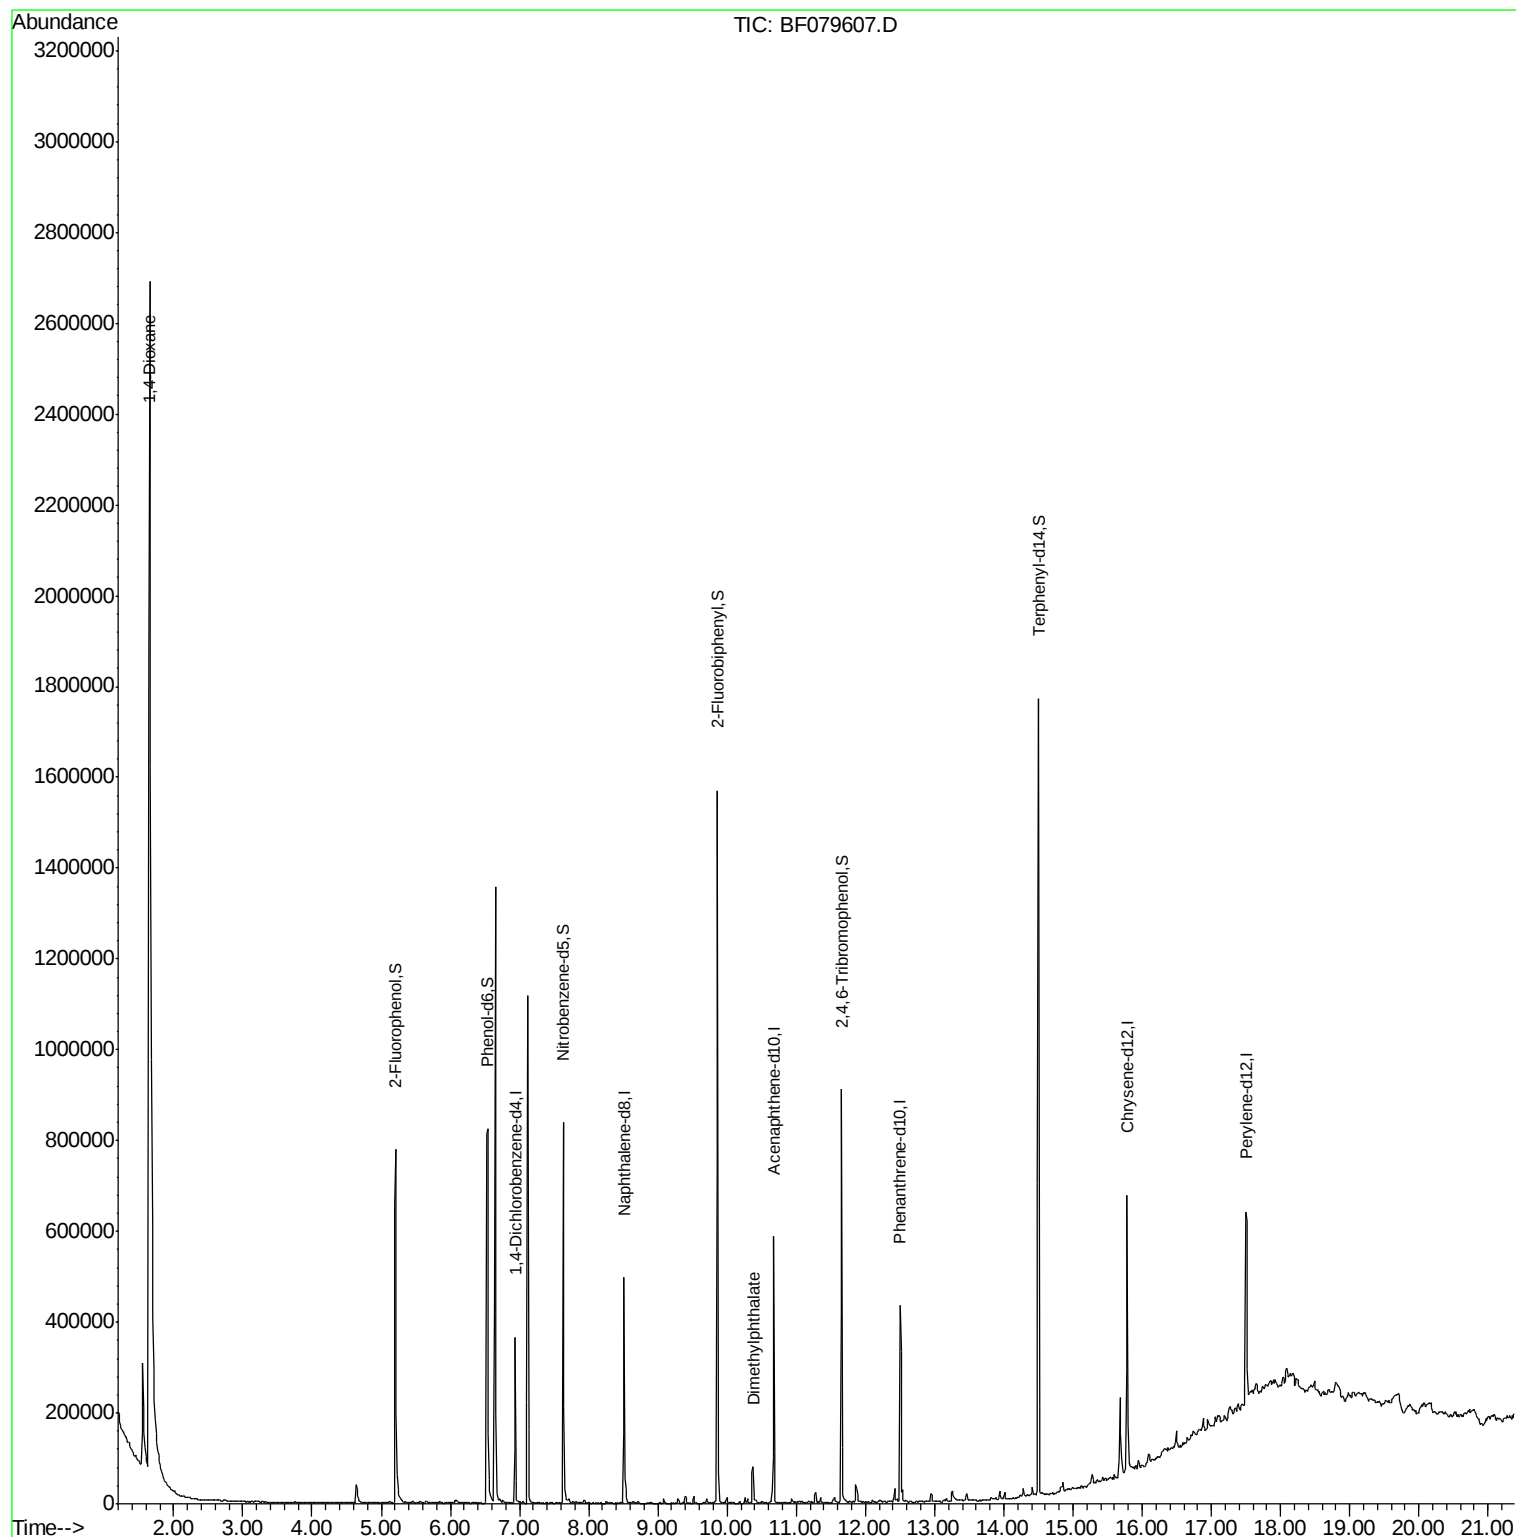



#1

1,4-Dichlorobenzene-d4

Concen: 20.00 ng

RT: 6.94 min Scan# 503

Delta R.T. -0.02 min

Lab File: BF079607.D

Acq: 30 May 2015 17:16

Instrument :

BNA_F

ClientSampleId :

PENRD8.7(5)


Tgt Ion:152 Resp: 62702

Ion Ratio Lower Upper

152 100

150 160.1 124.0 186.0




115 57.6 49.6 74.4

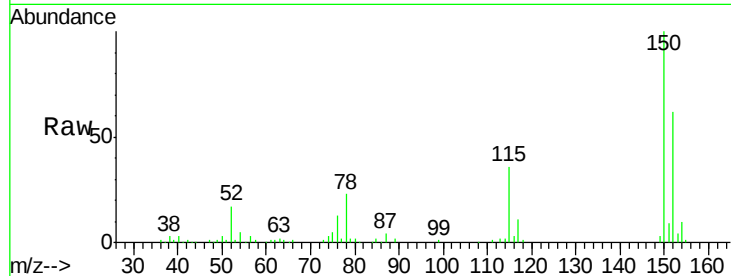

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

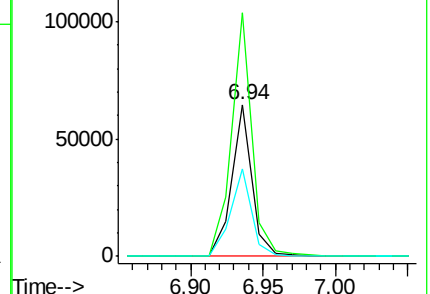

#2

1,4-Dioxane

Concen: 88.44 ng

RT: 1.66 min Scan# 41

Delta R.T. -0.11 min

Lab File: BF079607.D

Acq: 30 May 2015 17:16


Tgt Ion: 88 Resp: 152097

Ion Ratio Lower Upper

88 100

58 0.0 0.0 0.0



43 0.0 0.0 0.0




Abundance Ion 88.00 (87.70 to 88.70): BF0

Ion 58.00 (57.70 to 58.70): BF0

Ion 43.00 (42.70 to 43.70): BF0

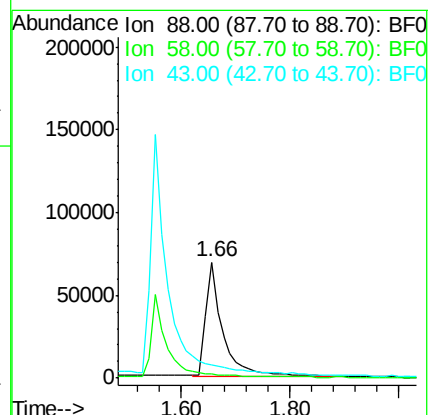



#5

2-Fluorophenol

Concen: 104.02 ng

RT: 5.21 min Scan# 352

Delta R.T. -0.02 min

Lab File: BF079607.D

Acq: 30 May 2015 17:16

Instrument :

BNA_F

ClientSampleId :

PENRD8.7(5)


Tgt Ion: 112 Resp: 376037

Ion Ratio Lower Upper

112 100

64 52.2 43.5 65.3




63 26.1 21.8 32.8



Abundance Ion 112.00 (111.70 to 112.70): B

Ion 64.00 (63.70 to 64.70): BF0

Ion 63.00 (62.70 to 63.70): BF0

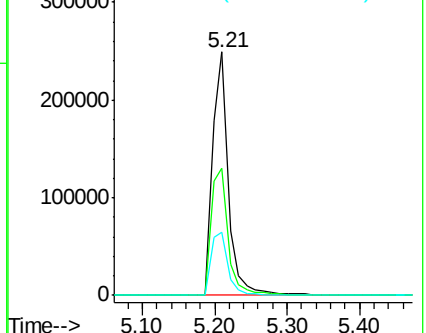

#7

Phenol-d6

Concen: 110.67 ng

RT: 6.54 min Scan# 468

Delta R.T. -0.02 min

Lab File: BF079607.D

Acq: 30 May 2015 17:16


Tgt Ion: 99 Resp: 509963

Ion Ratio Lower Upper

99 100

42 14.3 11.9 17.9



71 27.1 22.1 33.1



Abundance Ion 99.00 (98.70 to 99.70): BF0

Ion 42.00 (41.70 to 42.70): BF0

Ion 71.00 (70.70 to 71.70): BF0

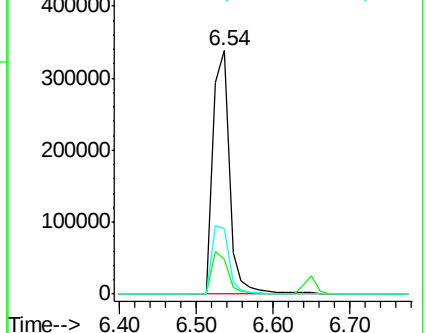







#21
Naphthalene-d8
Concen: 20.00 ng
RT: 8.51 min Scan# 641
Delta R.T. -0.02 min
Lab File: BF079607.D
Acq: 30 May 2015 17:16

Instrument :
BNA_F
ClientSampleId :
PENRD8.7(5)

Tgt Ion:	136	Resp:	254118
Ion	Ratio	Lower	Upper
136	100		
137	10.9	8.5	12.7
54	6.4	6.6	9.8#
68	4.9	4.7	7.1




Abundance Ion 136.00 (135.70 to 136.70): E
Ion 137.00 (136.70 to 137.70): E
Ion 54.00 (53.70 to 54.70): BF0
Ion 68.00 (67.70 to 68.70): BF0

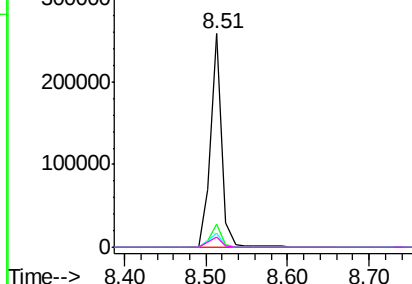




#23
Nitrobenzene-d5
Concen: 63.83 ng
RT: 7.63 min Scan# 564
Delta R.T. -0.03 min
Lab File: BF079607.D
Acq: 30 May 2015 17:16

Tgt Ion:	82	Resp:	280579
Ion	Ratio	Lower	Upper
82	100		
128	42.4	30.8	46.2
54	51.5	42.8	64.2



Abundance Ion 82.00 (81.70 to 82.70): BF0
Ion 128.00 (127.70 to 128.70): E
Ion 54.00 (53.70 to 54.70): BF0

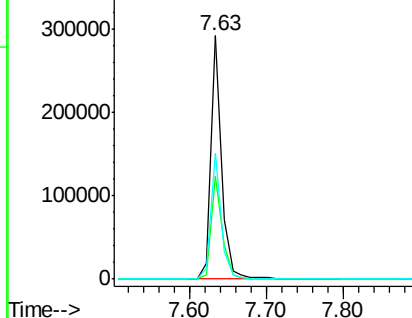

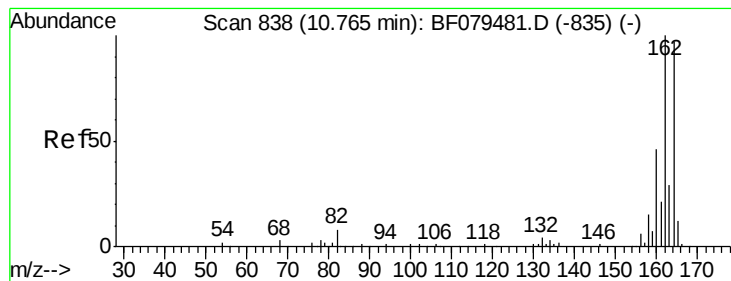

#38

Acenaphthene-d10

Concen: 20.00 ng

RT: 10.67 min Scan# 830

Delta R.T. -0.03 min

Lab File: BF079607.D

Acq: 30 May 2015 17:16

Instrument :

BNA_F

ClientSampleId :

PENRD8.7(5)


Tgt Ion:164 Resp: 119625

Ion Ratio Lower Upper

164 100

162 102.7 82.6 124.0




160 46.6 37.7 56.5



Abundance Ion 164.00 (163.70 to 164.70): E

Ion 162.00 (161.70 to 162.70): E

Ion 160.00 (159.70 to 160.70): E

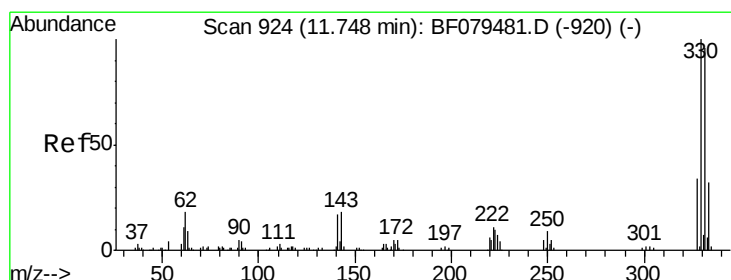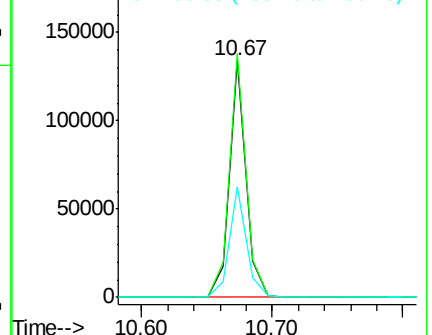

#41

2,4,6-Tribromophenol

Concen: 105.88 ng

RT: 11.66 min Scan# 916

Delta R.T. -0.03 min

Lab File: BF079607.D

Acq: 30 May 2015 17:16


Tgt Ion:330 Resp: 139121

Ion Ratio Lower Upper

330 100

332 96.6 0.0 0.0#



141 31.6 0.0 0.0#




Abundance Ion 329.80 (329.50 to 330.50): E

Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E




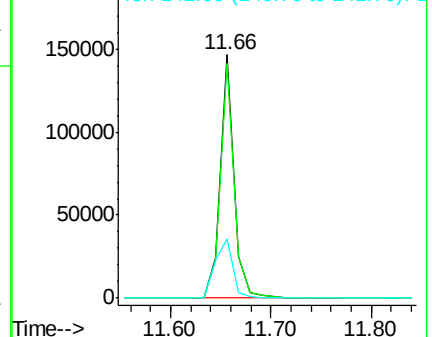


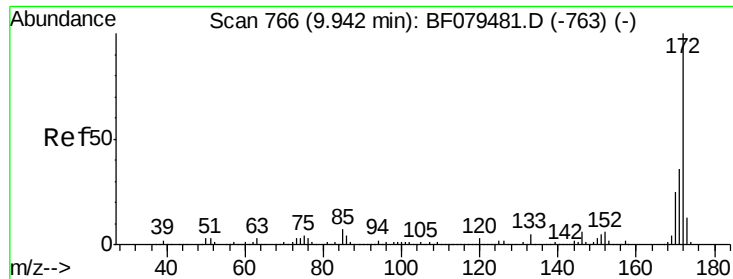

#44
 2-Fluorobiphenyl
 Concen: 69.64 ng
 RT: 9.86 min Scan# 759
 Delta R.T. -0.02 min
 Lab File: BF079607.D
 Acq: 30 May 2015 17:16




Instrument :
 BNA_F
 ClientSampleId :
 PENRD8.7(5)


Tgt Ion:172 Resp: 583943
 Ion Ratio Lower Upper
 172 100
 171 35.1 28.5 42.7
 170 24.1 19.7 29.5

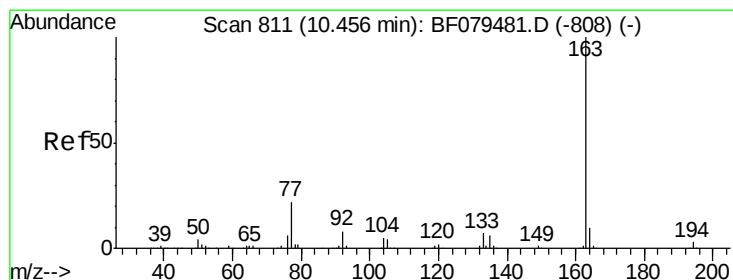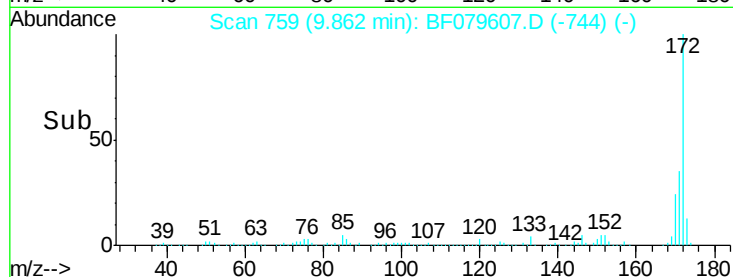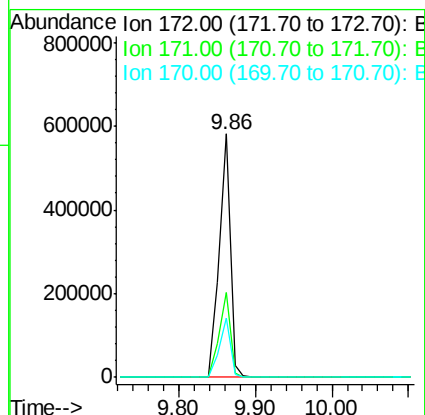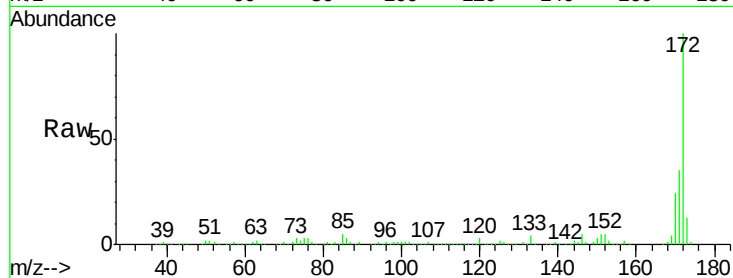

#49
 Dimethylphthalate
 Concen: 5.56 ng
 RT: 10.38 min Scan# 804
 Delta R.T. -0.03 min
 Lab File: BF079607.D
 Acq: 30 May 2015 17:16

Tgt Ion:163 Resp: 48989
 Ion Ratio Lower Upper
 163 100
 194 3.2 2.4 3.6
 164 9.5 8.2 12.4


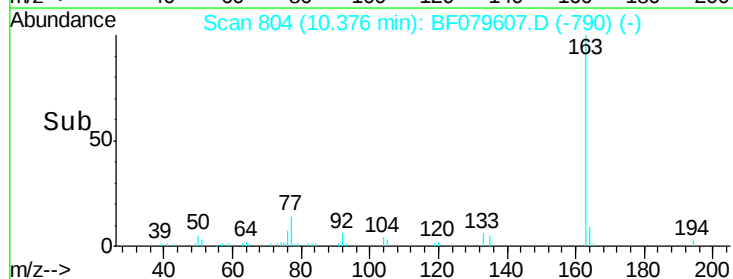
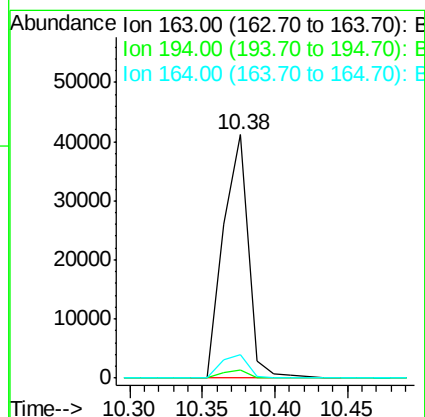
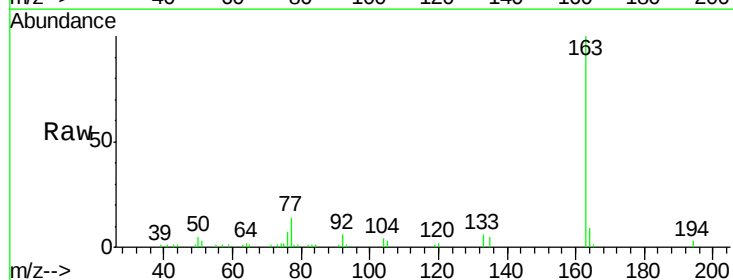




#63
Phenanthrene-d10
Concen: 20.00 ng
RT: 12.50 min Scan# 990
Delta R.T. -0.03 min
Lab File: BF079607.D
Acq: 30 May 2015 17:16




Instrument :
BNA_F
ClientSampleId :
PENRD8.7(5)


Tgt Ion:188 Resp: 219996
Ion Ratio Lower Upper
188 100
94 13.3 9.8 14.6
80 13.5 10.5 15.7

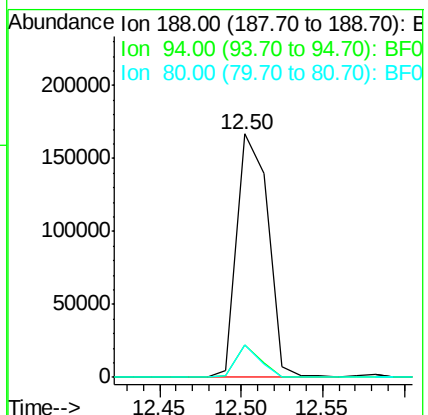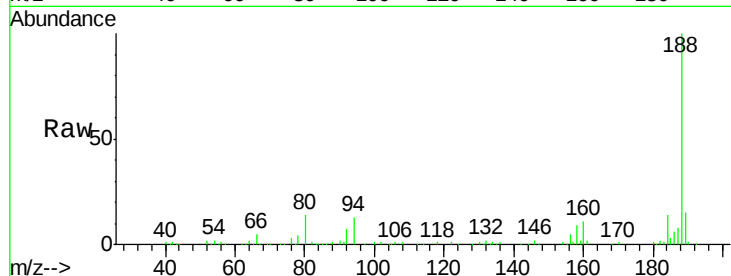

#75
Chrysene-d12
Concen: 20.00 ng
RT: 15.78 min Scan# 1277
Delta R.T. -0.06 min
Lab File: BF079607.D
Acq: 30 May 2015 17:16

Tgt Ion:240 Resp: 237497
Ion Ratio Lower Upper
240 100
120 10.9 10.8 16.2
236 26.4 21.0 31.6



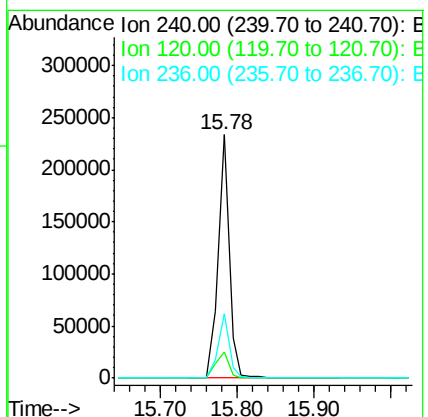



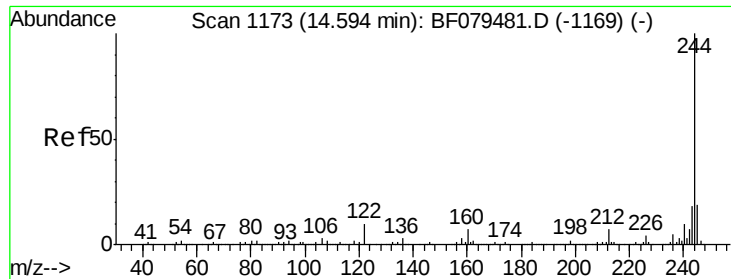

#78
 Terphenyl-d14
 Concen: 63.95 ng
 RT: 14.50 min Scan# 1165
 Delta R.T. -0.03 min
 Lab File: BF079607.D
 Acq: 30 May 2015 17:16

Instrument :
 BNA_F
 ClientSampleId :
 PENRD8.7(5)

Tgt Ion:244 Resp: 647138
 Ion Ratio Lower Upper
 244 100
 212 6.5 5.2 7.8
 122 10.8 8.0 12.0

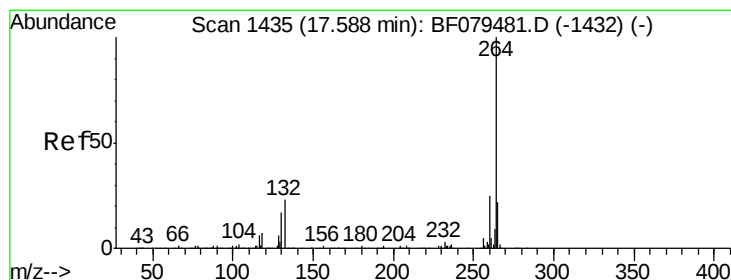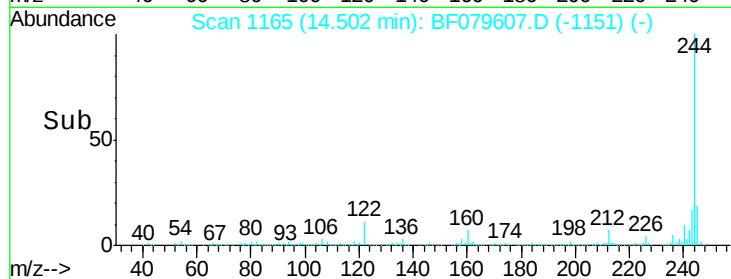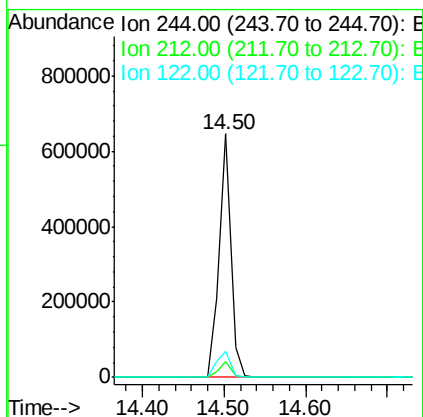

#86
 Perylene-d12
 Concen: 20.00 ng
 RT: 17.51 min Scan# 1428
 Delta R.T. -0.16 min
 Lab File: BF079607.D
 Acq: 30 May 2015 17:16

Tgt Ion:264 Resp: 245701
 Ion Ratio Lower Upper
 264 100
 260 24.4 19.8 29.8
 265 22.0 17.8 26.6

