
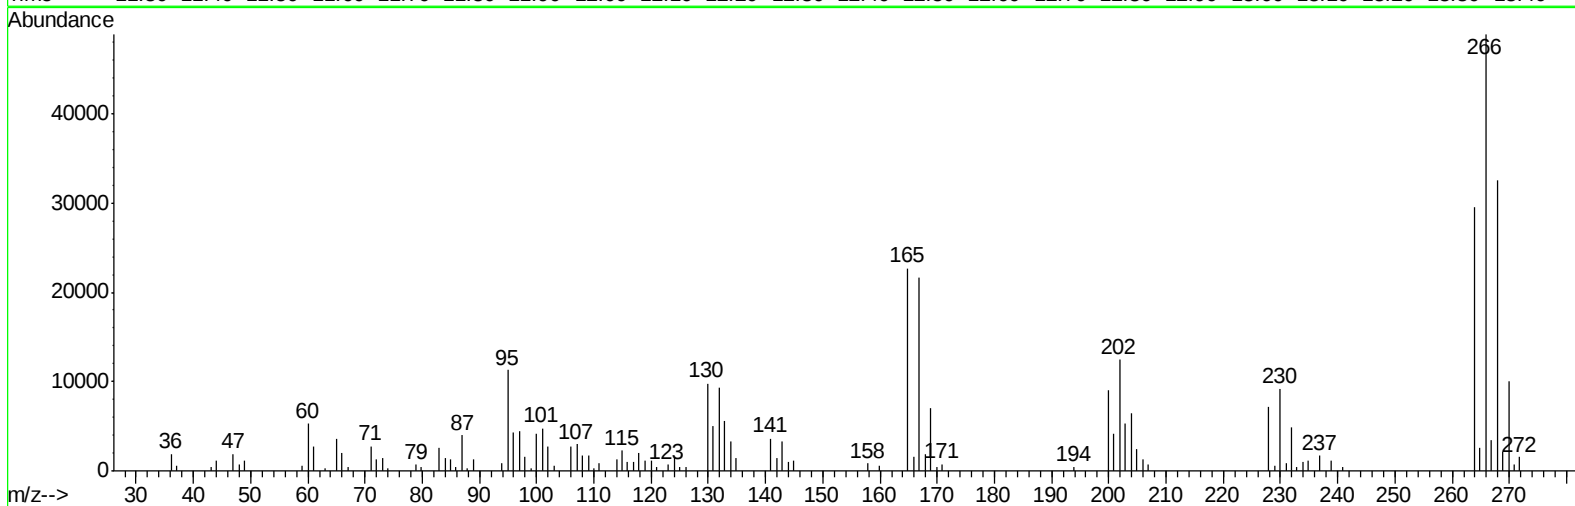


Data Path : Z:\HPCHEM1\BNA_F\Data\BF053015\
Data File : BF079598.D
Acq On : 30 May 2015 12:44
Operator : TP/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 01 08:04:40 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF052615.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun May 31 14:01:50 2015
Response via : Initial Calibration

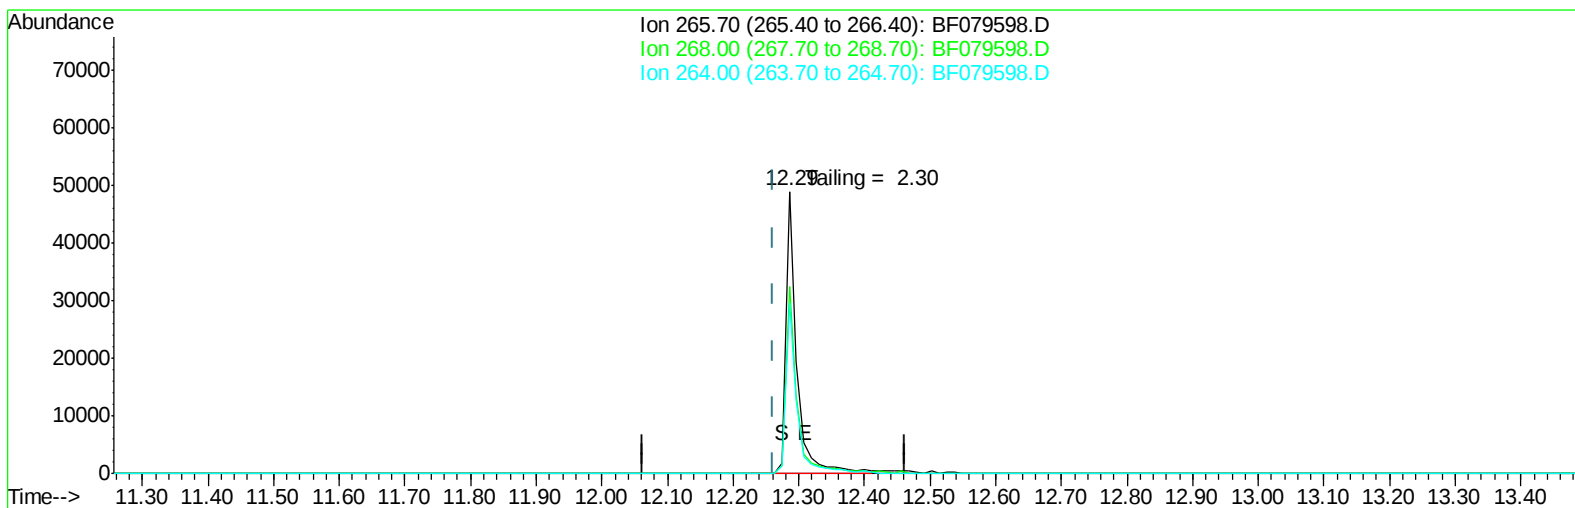

TIC: BF079598.D

(69) Pentachlorophenol (C)



12.285min (+0.023) 3068.95ng

response 60084

Ion	Exp%	Act%
265.70	100	100
268.00	70.10	66.54
264.00	62.50	60.38
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\Data\BF053015\
Data File : BF079598.D
Acq On : 30 May 2015 12:44
Operator : TP/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 01 08:04:40 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF052615.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun May 31 14:01:50 2015
Response via : Initial Calibration

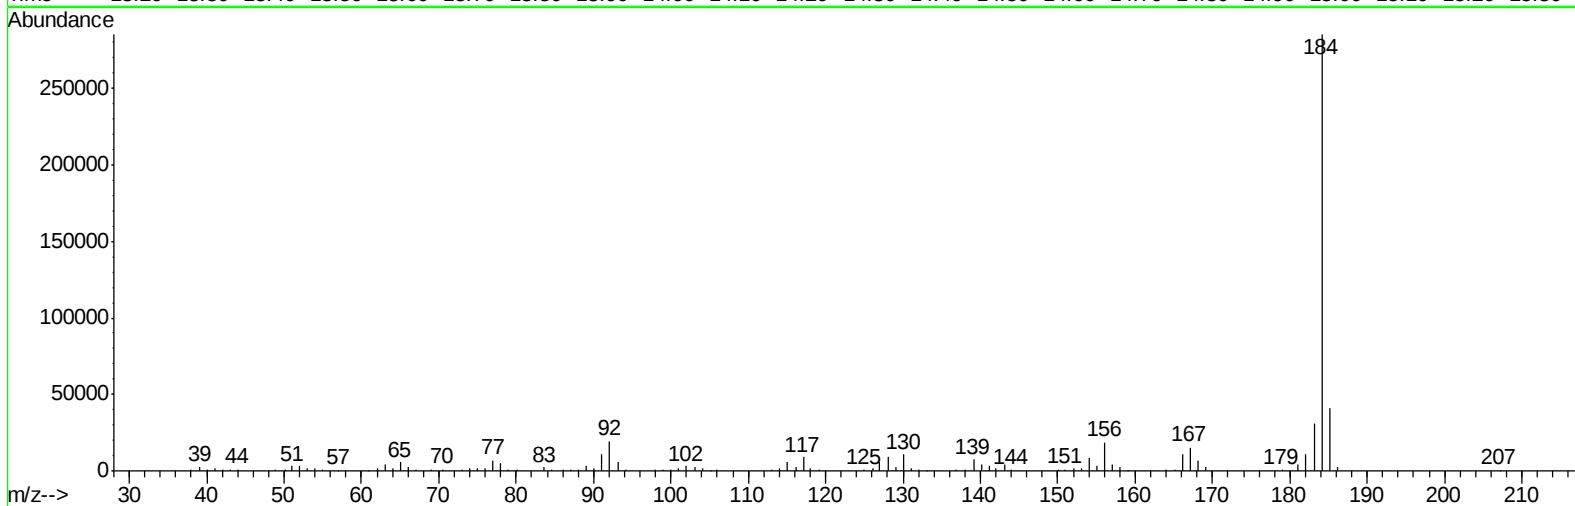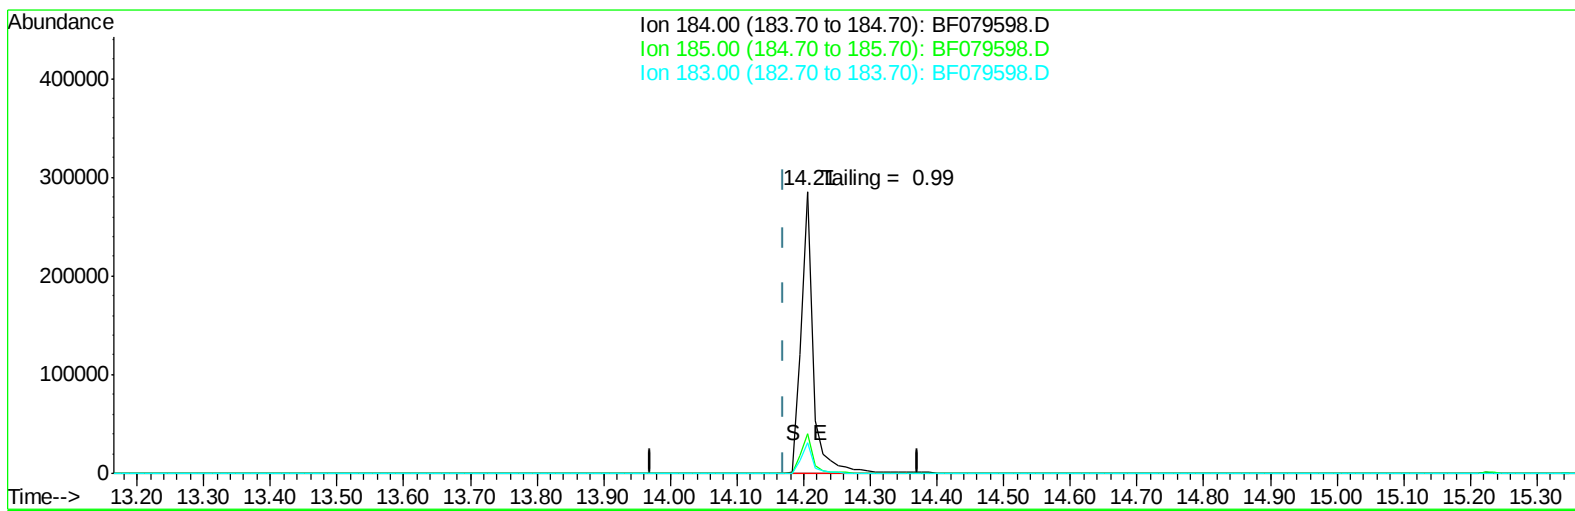

TIC: BF079598.D

(76) Benzidine

14.205min (+0.034) 62549.17ng

response 360387

Ion	Exp%	Act%
184.00	100	100
185.00	15.10	14.30
183.00	10.70	10.75
0.00	0.00	0.00