


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF053015\
 Data File : BF079598.D
 Acq On : 30 May 2015 12:44
 Operator : TP/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF052615.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Sun May 31 14:01:50 2015

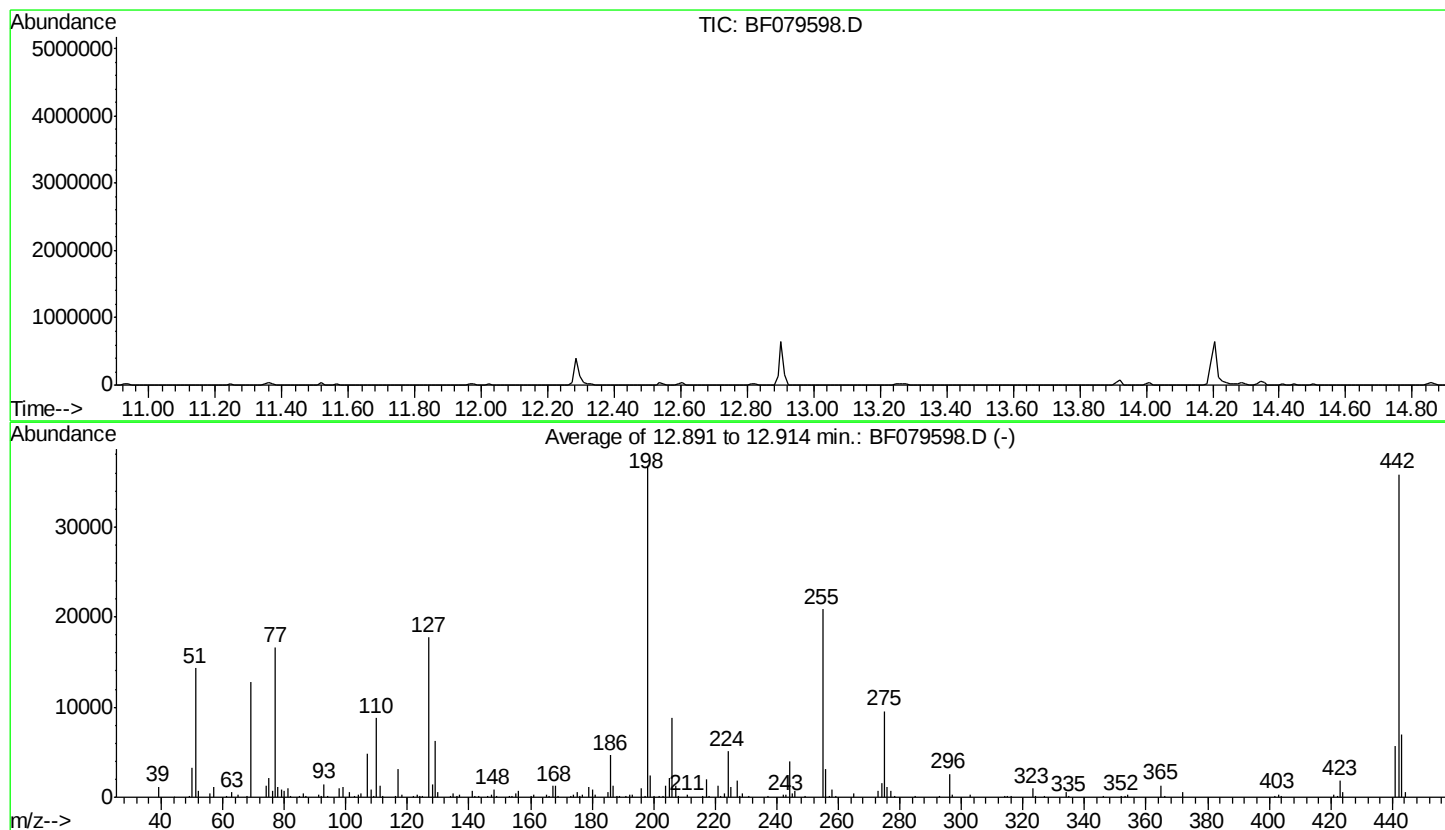

AutoFind: Scans 1024, 1025, 1026; Background Corrected with Scan 1021

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.8	14287	PASS
68	69	0.00	2	1.2	153	PASS
69	198	0.00	100	34.7	12768	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	48.2	17724	PASS
197	198	0.00	2	0.4	137	PASS
198	198	100	100	100.0	36788	PASS
199	198	5	9	6.6	2418	PASS
275	198	10	60	26.0	9564	PASS
365	198	1	100	3.5	1305	PASS
441	442	0.01	24	15.8	5647	PASS
442	198	50	100	97.4	35847	PASS
443	442	15	24	19.5	6976	PASS