


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF053015\
Data File : BF079622.D
Acq On : 31 May 2015 1:28
Operator : TP/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF052615.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Sun May 31 14:01:50 2015

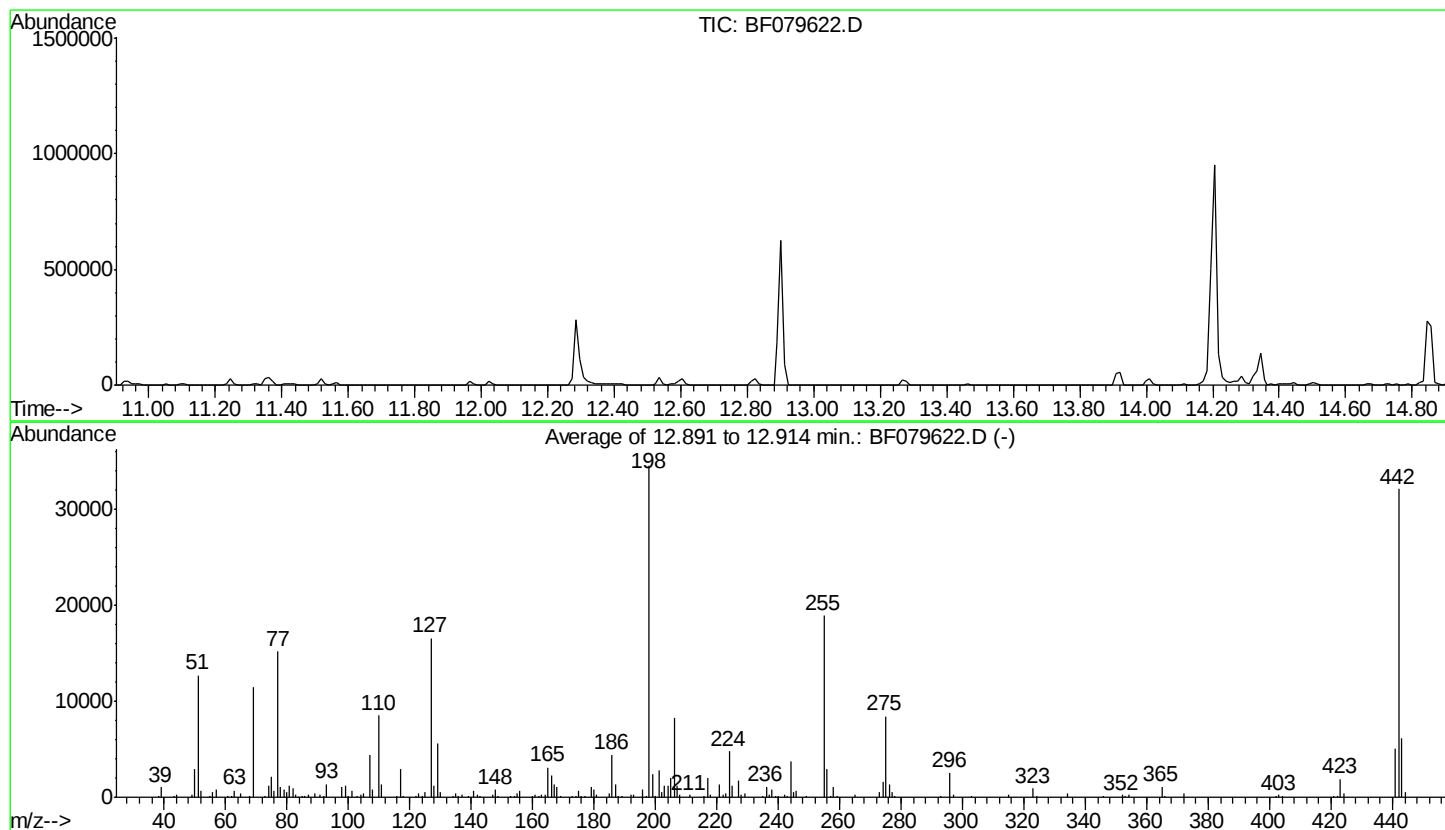

AutoFind: Scans 1024, 1025, 1026; Background Corrected with Scan 1021

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.8	12693	PASS
68	69	0.00	2	1.3	146	PASS
69	198	0.00	100	33.3	11488	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	47.9	16519	PASS
197	198	0.00	2	0.5	171	PASS
198	198	100	100	100.0	34480	PASS
199	198	5	9	7.1	2446	PASS
275	198	10	60	24.4	8419	PASS
365	198	1	100	3.1	1073	PASS
441	442	0.01	24	15.9	5084	PASS
442	198	50	100	92.9	32033	PASS
443	442	15	24	19.2	6143	PASS