

Data Path : Z:\HPCHEM1\BNA F\DATA\BF053017\
 Data File : BF095532.D
 Acq On : 30 May 2017 13:27
 Operator : SJ/MA
 Sample : I3281-09
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :

Quant Time: May 31 01:38:34 2017
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF050217.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri May 26 16:50:16 2017
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.74	152	96089	20.00	ng	0.00
21) Naphthalene-d8	9.76	136	402809	20.00	ng	0.00
38) Acenaphthene-d10	12.59	164	188912	20.00	ng	0.00
63) Phenanthrene-d10	14.99	188	343771	20.00	ng	0.00
75) Chrysene-d12	18.67	240	253431	20.00	ng	0.00
86) Perylene-d12	20.35	264	183671	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.70	112	850898	147.64	ng	0.00
7) Phenol-d6	7.28	99	1054368	152.47	ng	-0.01
23) Nitrobenzene-d5	8.64	82	608581	95.27	ng	-0.01
41) 2,4,6-Tribromophenol	13.89	330	224244	144.94	ng	-0.01
44) 2-Fluorobiphenyl	11.53	172	1149753	87.60	ng	0.00
78) Terphenyl-d14	17.31	244	874083	75.97	ng	-0.01
Target Compounds						Qvalue
15) Benzyl Alcohol	7.97	79	10129	2.28	ng	# 42
19) n-Nitroso-di-n-propylamine	8.64	70	73911	15.80	ng	# 79
49) Dimethylphthalate	12.23	163	291675	18.81	ng	100
70) Phenanthrene	15.04	178	52046	2.63	ng	98
71) Anthracene	15.04	178	52046	2.58	ng	97
74) Fluoranthene	16.78	202	103975	5.13	ng	99
77) Pyrene	17.09	202	92922	4.90	ng	98
80) Benzo(a)anthracene	18.66	228	38375	2.60	ng	96
82) Chrysene	18.66	228	38375	2.69	ng	95
87) Benzo(b)fluoranthene	19.95	252	54060	4.76	ng	# 96
88) Benzo(k)fluoranthene	19.95	252	54060	4.94	ng	100
89) Benzo(a)pyrene	20.30	252	27854	2.66	ng	96
91) Benzo(a,h,i)perylene	22.11	276	18378	2.17	ng	92


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA F\DATA\BF053017\
Data File : BF095532.D
Acq On : 30 May 2017 13:27
Operator : SJ/MA
Sample : I3281-09
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :

Quant Time: May 31 01:38:34 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF050217.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri May 26 16:50:16 2017
Response via : Initial Calibration

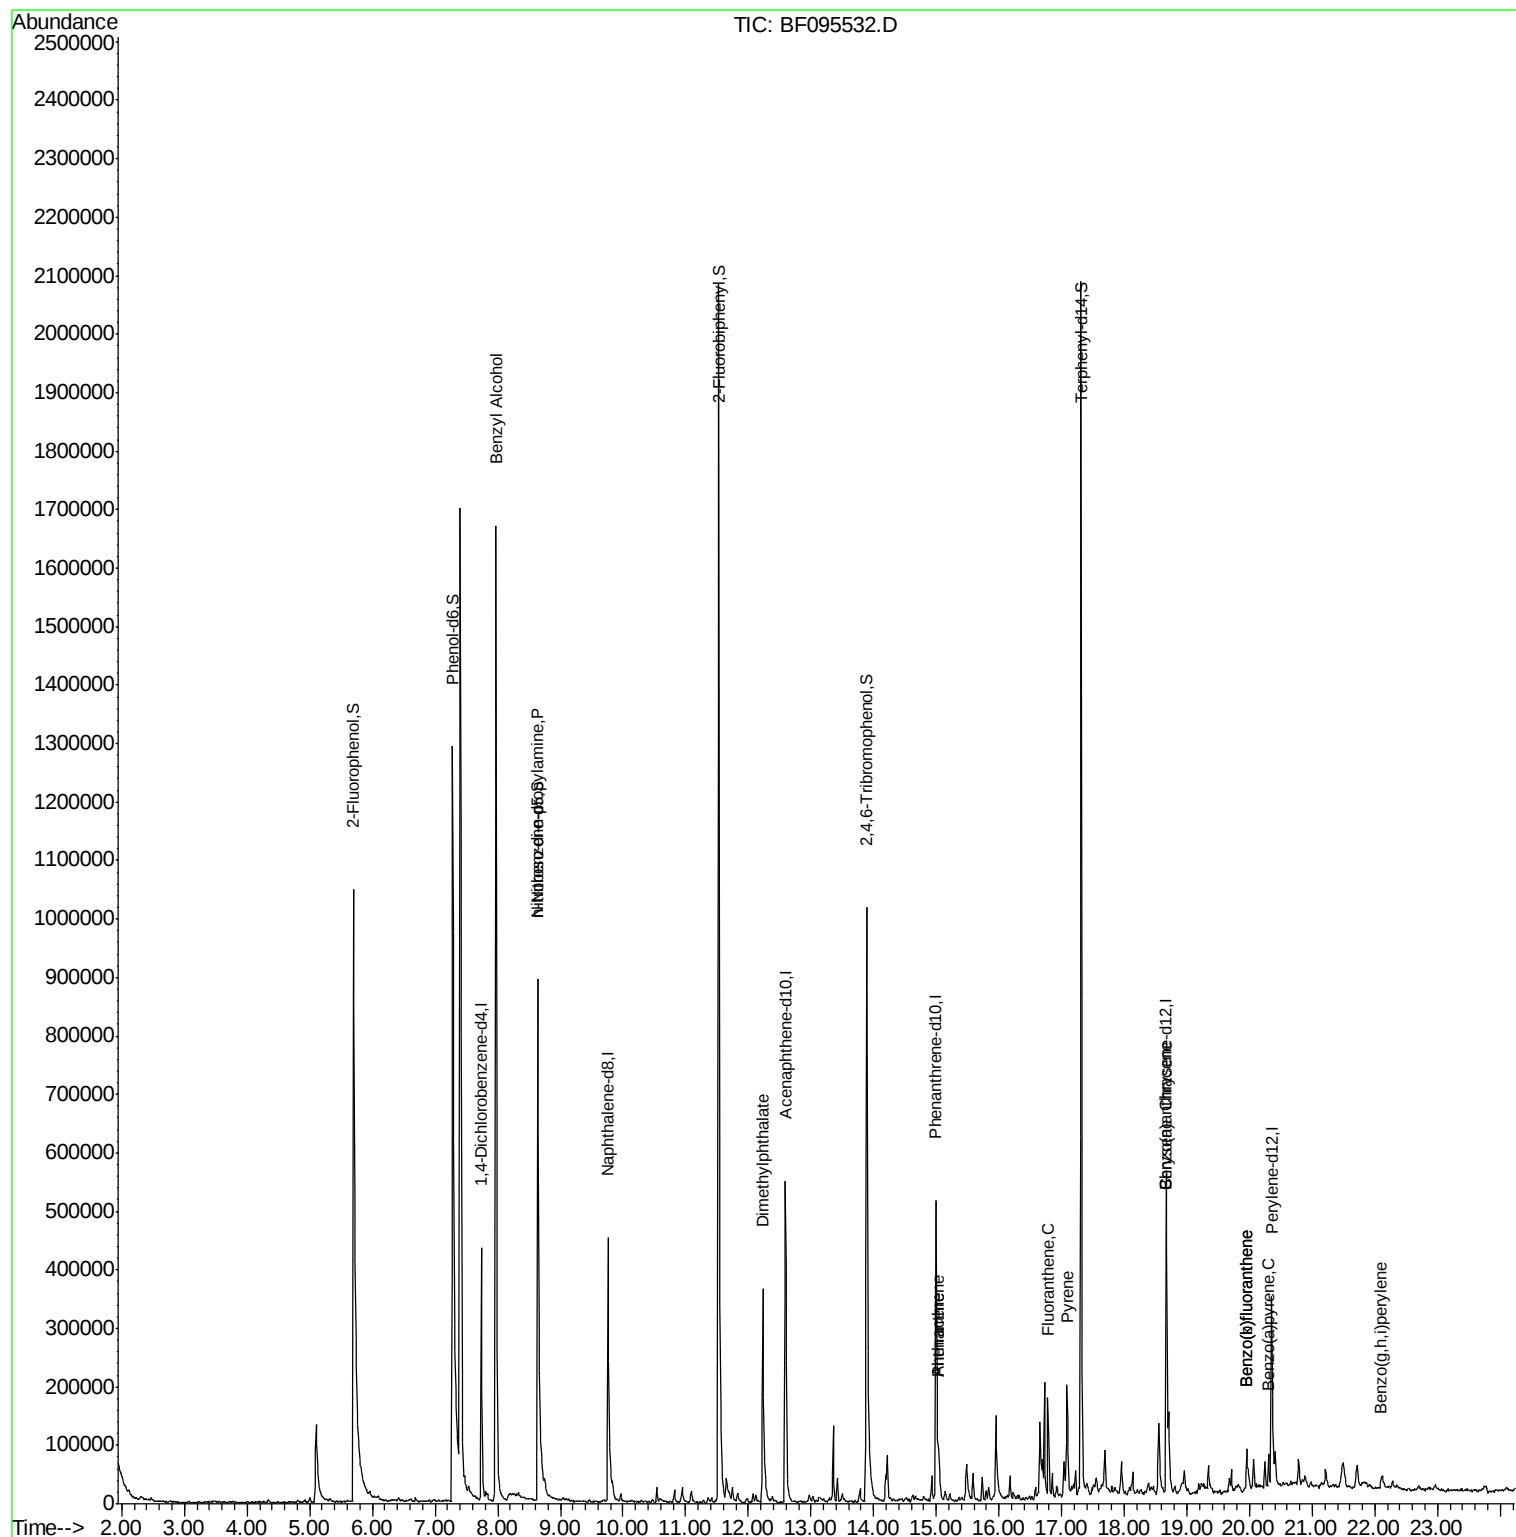

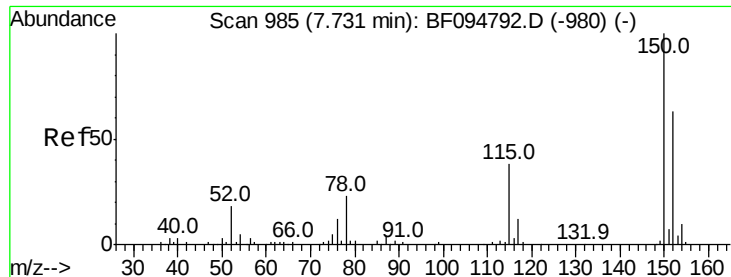


#1




1,4-Dichlorobenzene-d4
Concen: 20.00 ng
RT: 7.74 min Scan# 986
Delta R.T. -0.01 min
Lab File: BF095532.D
Acq: 30 May 2017 13:27

Instrument :
BNA_F
ClientSampleId :

Tot Ion:152 Resp: 96089
Ion Ratio Lower Upper
152 100
150 151.3 126.2 189.2
115 58.4 52.2 78.2




Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

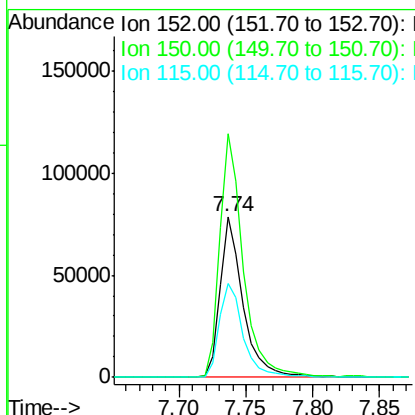



#5


2-Fluorophenol
Concen: 147.64 ng
RT: 5.70 min Scan# 640
Delta R.T. -0.01 min
Lab File: BF095532.D
Acq: 30 May 2017 13:27

Tgt Ion:112 Resp: 850898
Ion Ratio Lower Upper
112 100
64 54.7 46.0 69.0
63 26.1 23.4 35.0



Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BF0
Ion 63.00 (62.70 to 63.70): BF0

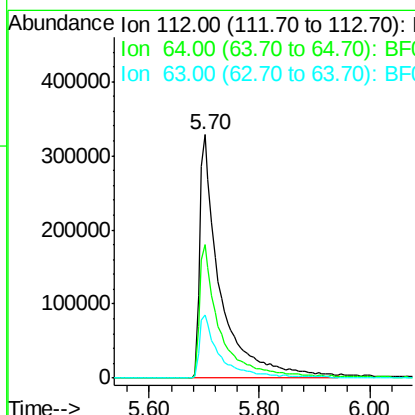

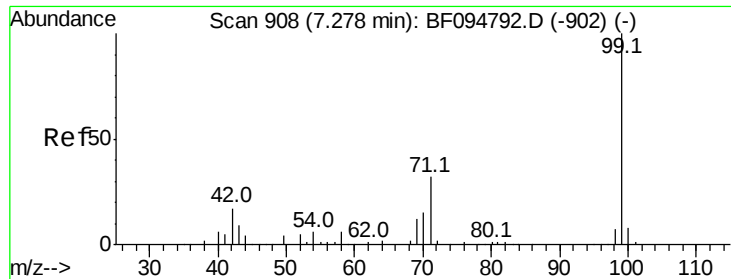

#7

Phenol-d6

Concen: 152.47 ng

RT: 7.28 min Scan# 909

Delta R.T. -0.01 min

Lab File: BF095532.D

Acq: 30 May 2017 13:27

Instrument :

BNA_F

ClientSampleId :


Tot Ion: 99 Resp: 1054368

Ion Ratio Lower Upper

99 100

42 16.1 13.5 20.3




71 31.4 24.5 36.7

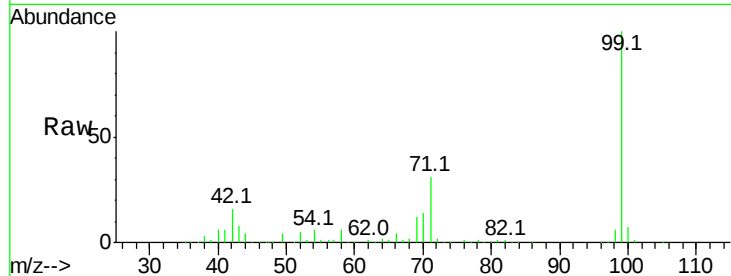

Abundance Ion 99.00 (98.70 to 99.70): BF0

Ion 42.00 (41.70 to 42.70): BF0

Ion 71.00 (70.70 to 71.70): BF0

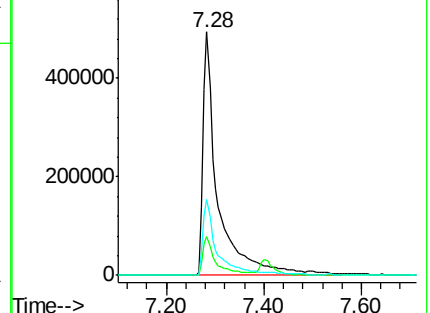

#15

Benzyl Alcohol

Concen: 2.28 ng

RT: 7.97 min Scan# 1026

Delta R.T. -0.06 min

Lab File: BF095532.D

Acq: 30 May 2017 13:27


Tgt Ion: 79 Resp: 10129

Ion Ratio Lower Upper

79 100

108 29.3 63.4 95.0#



77 107.1 49.2 73.8#




Abundance Ion 79.00 (78.70 to 79.70): BF0

Ion 108.00 (107.70 to 108.70): BF0

Ion 77.00 (76.70 to 77.70): BF0

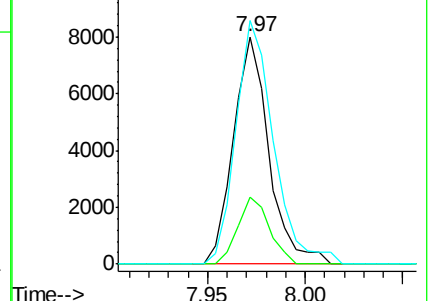

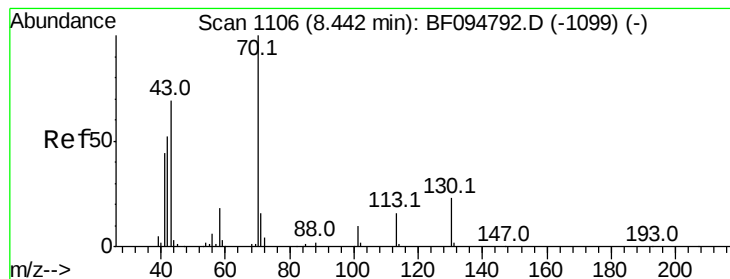

#19

n-Nitroso-di-n-propylamine

Concen: 15.80 ng

RT: 8.64 min Scan# 1140

Delta R.T. 0.18 min

Lab File: BF095532.D

Acq: 30 May 2017 13:27

Instrument :





BNA_F

ClientSampleId :

Tot Ion: 70 Resp: 73911

Ion Ratio Lower Upper

70	100		
42	47.5	47.2	70.8
101	0.0	7.2	10.8#
130	2.6	15.9	23.9#

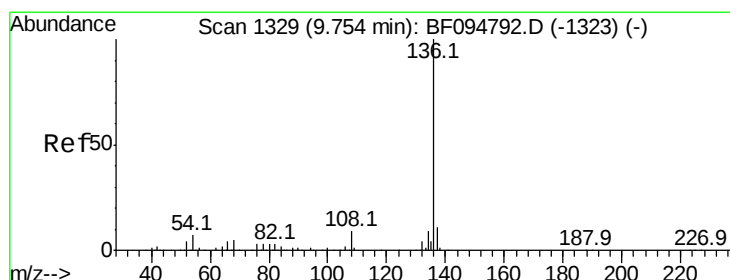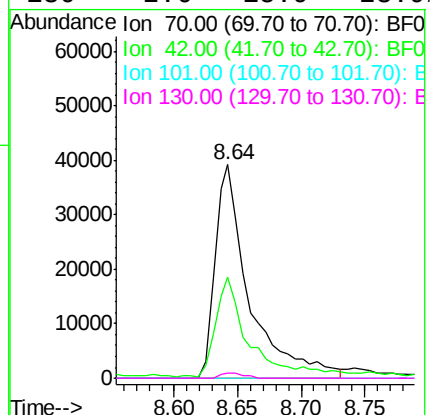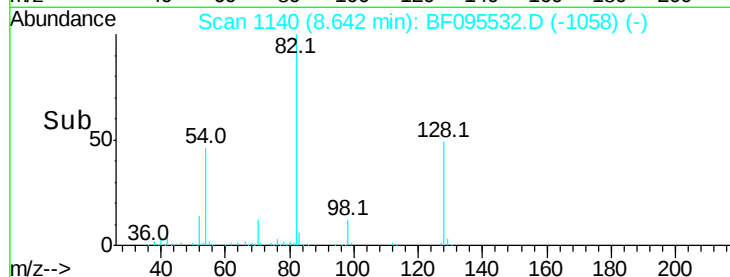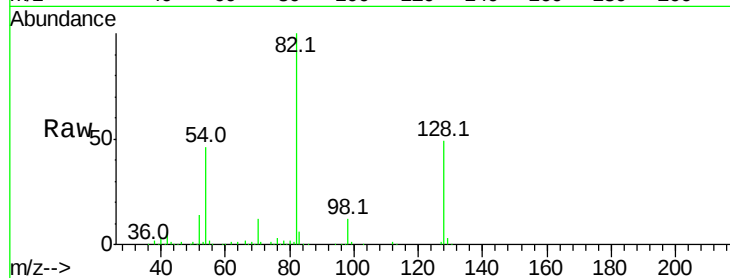

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 9.76 min Scan# 1330

Delta R.T. 0.00 min




Lab File: BF095532.D


Acq: 30 May 2017 13:27

Tgt Ion: 136 Resp: 402809

Ion Ratio Lower Upper

136	100		
137	10.5	8.5	12.7
54	7.4	4.9	7.3#
68	5.7	4.1	6.1


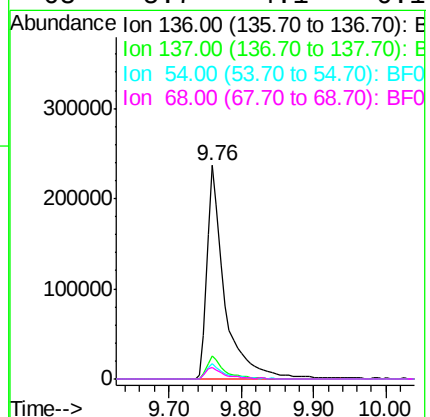
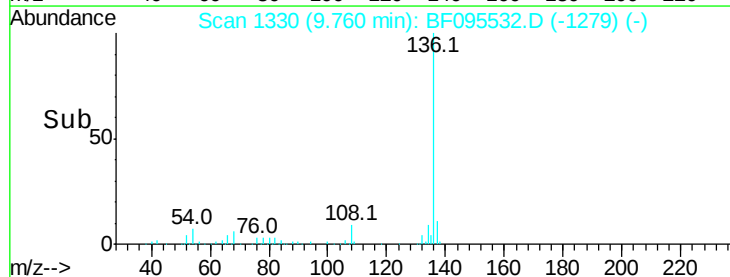
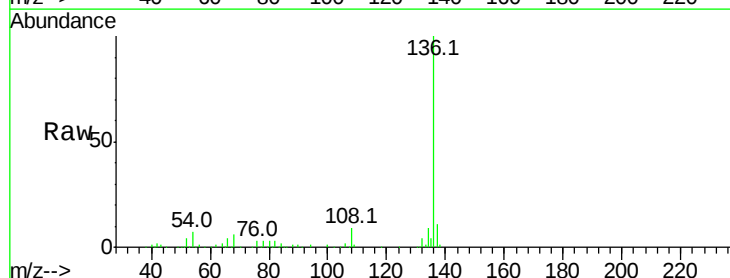


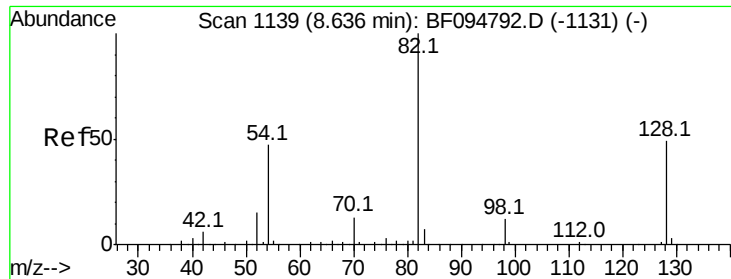

#23
 Nitrobenzene-d5
 Concen: 95.27 ng
 RT: 8.64 min Scan# 1140
 Delta R.T. -0.01 min
 Lab File: BF095532.D
 Acq: 30 May 2017 13:27




Instrument :
 BNA_F
 ClientSampleId :


Tot Ion: 82 Resp: 608581
 Ion Ratio Lower Upper
 82 100
 128 48.8 34.0 51.0
 54 45.8 42.2 63.2

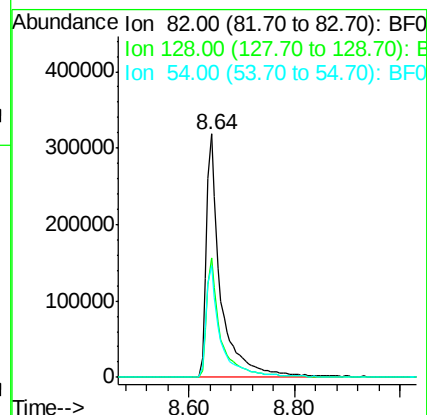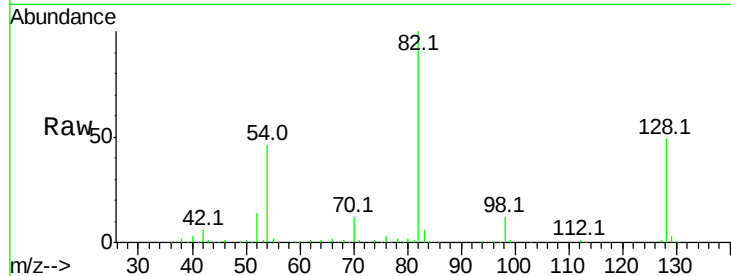

#38
 Acenaphthene-d10
 Concen: 20.00 ng
 RT: 12.59 min Scan# 1811
 Delta R.T. -0.01 min
 Lab File: BF095532.D
 Acq: 30 May 2017 13:27

Tgt Ion:164 Resp: 188912
 Ion Ratio Lower Upper
 164 100
 162 103.3 82.6 123.8
 160 44.8 36.2 54.2

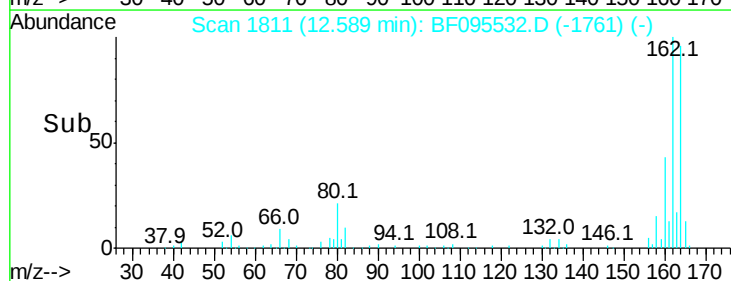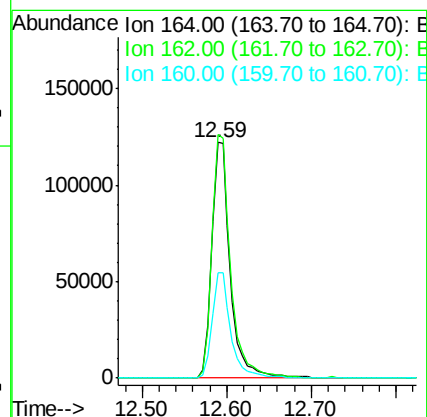


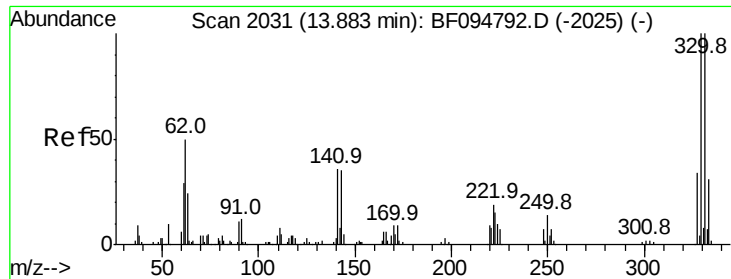




#41
 2,4,6-Tribromophenol
 Concen: 144.94 ng
 RT: 13.89 min Scan# 2032
 Delta R.T. -0.01 min
 Lab File: BF095532.D
 Acq: 30 May 2017 13:27

Instrument :
 BNA_F
 ClientSampleId :

Tot Ion:330 Resp: 224244
 Ion Ratio Lower Upper
 330 100
 332 95.7 76.6 115.0
 141 40.6 31.4 47.2




Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

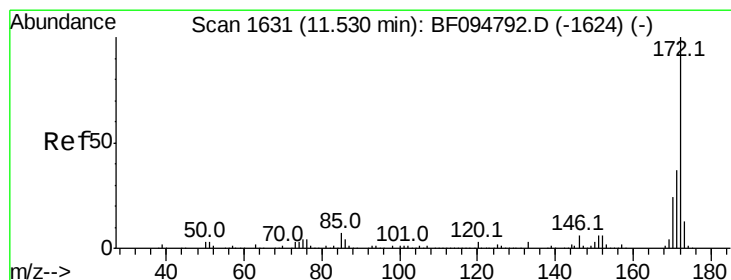
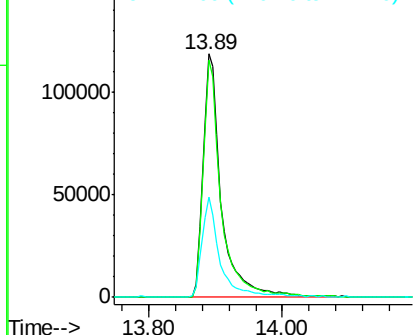



#44
 2-Fluorobiphenyl
 Concen: 87.60 ng
 RT: 11.53 min Scan# 1631
 Delta R.T. -0.01 min
 Lab File: BF095532.D
 Acq: 30 May 2017 13:27

Tgt Ion:172 Resp: 1149753
 Ion Ratio Lower Upper
 172 100
 171 35.5 29.6 44.4
 170 23.3 19.8 29.8

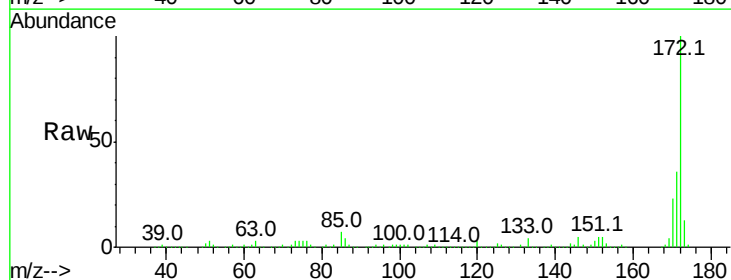

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

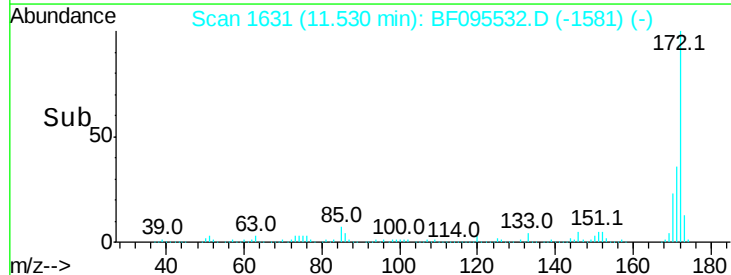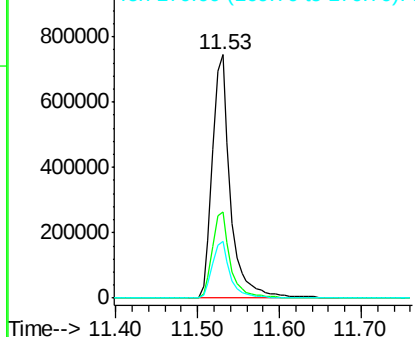

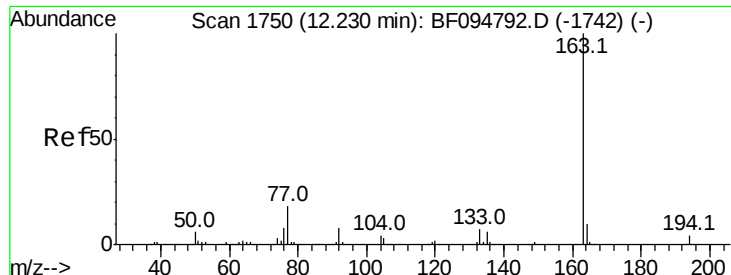

#49

Dimethylphthalate

Concen: 18.81 ng

RT: 12.23 min Scan# 1750

Delta R.T. -0.01 min

Lab File: BF095532.D

Acq: 30 May 2017 13:27

Instrument :

BNA_F

ClientSampled :


Tot Ion:163 Resp: 291675

Ion Ratio Lower Upper

163 100

194 3.5 2.6 4.0




164 10.6 8.4 12.6

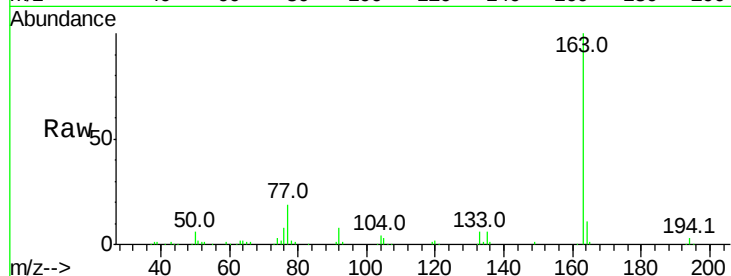

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

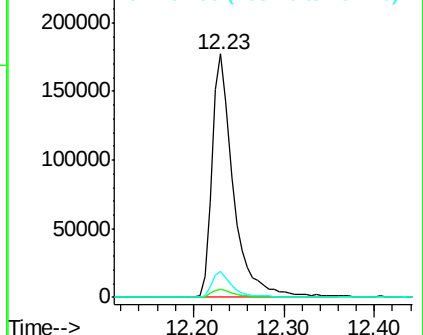

#63

Phenanthrene-d10

Concen: 20.00 ng

RT: 14.99 min Scan# 2220

Delta R.T. -0.01 min

Lab File: BF095532.D

Acq: 30 May 2017 13:27


Tgt Ion:188 Resp: 343771

Ion Ratio Lower Upper

188 100

94 10.5 9.4 14.2



80 12.0 10.2 15.2

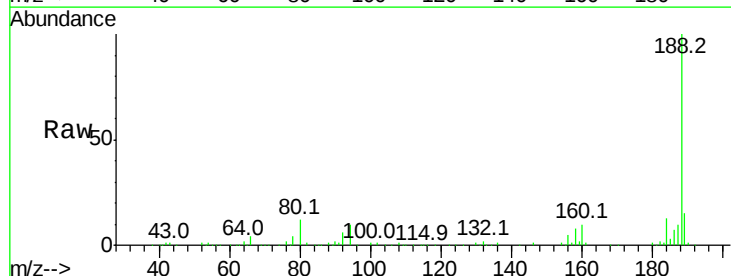


Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BF0

Ion 80.00 (79.70 to 80.70): BF0




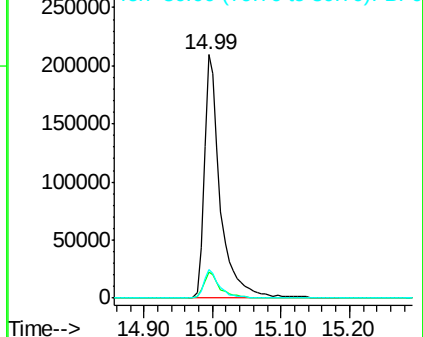


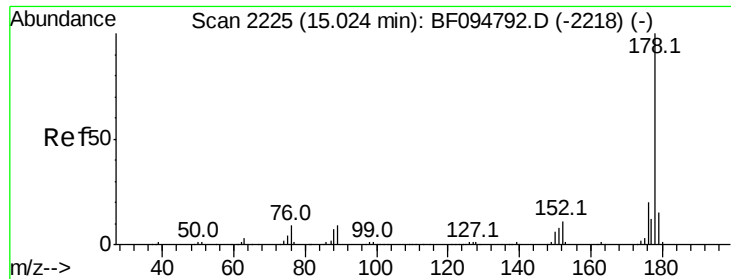

#70
Phenanthrene
Concen: 2.63 ng
RT: 15.04 min Scan# 2227
Delta R.T. -0.01 min
Lab File: BF095532.D
Acq: 30 May 2017 13:27




Instrument :
BNA_F
ClientSampleId :


Tot Ion:178 Resp: 52046
Ion Ratio Lower Upper
178 100
176 21.8 16.2 24.4
179 15.6 12.6 19.0

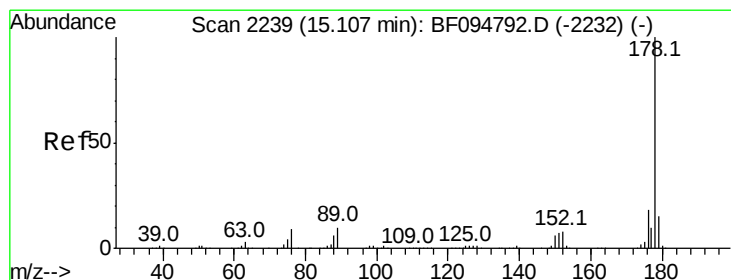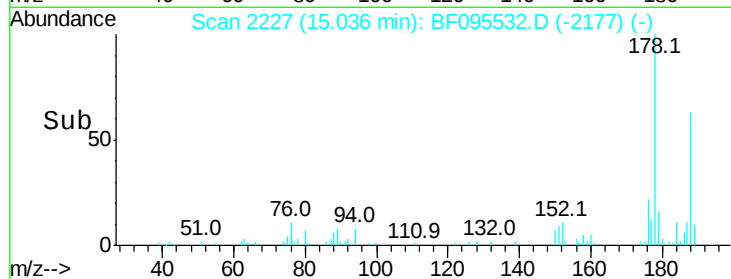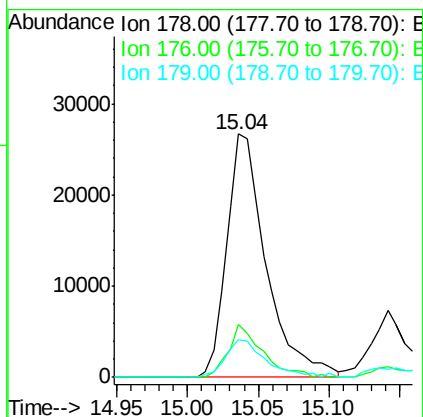

#71
Anthracene
Concen: 2.58 ng
RT: 15.04 min Scan# 2227
Delta R.T. -0.09 min
Lab File: BF095532.D
Acq: 30 May 2017 13:27

Tgt Ion:178 Resp: 52046
Ion Ratio Lower Upper
178 100
176 21.8 15.8 23.8
179 15.6 12.7 19.1


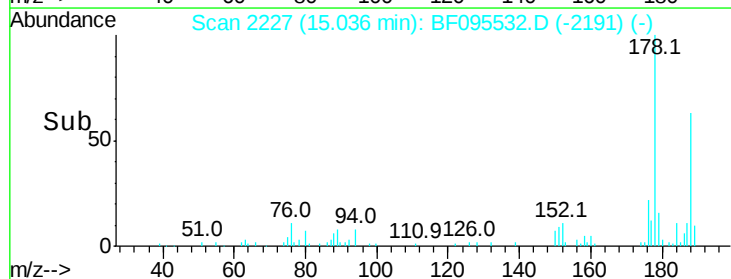
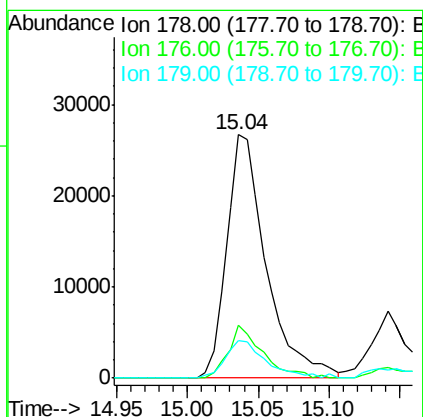
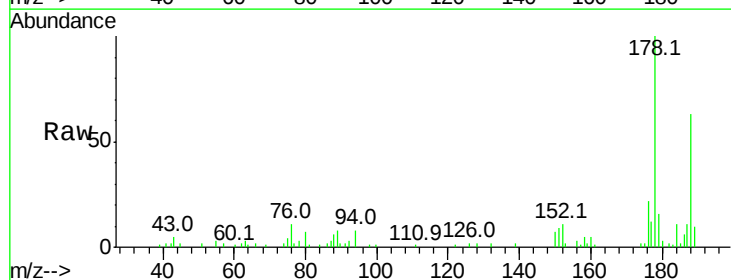




#74
 Fluoranthene
 Concen: 5.13 ng
 RT: 16.78 min Scan# 2524
 Delta R.T. 0.00 min
 Lab File: BF095532.D
 Acq: 30 May 2017 13:27




Instrument :
 BNA_F
 ClientSampled :


Tot Ion:	202	Resp:	103975
Ion Ratio	Lower	Upper	
202	100		
101	13.7	0.0	33.2
203	18.2	0.0	38.1

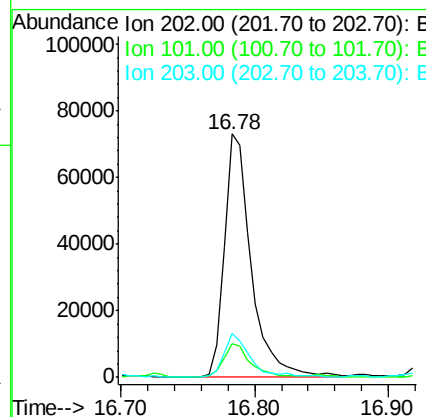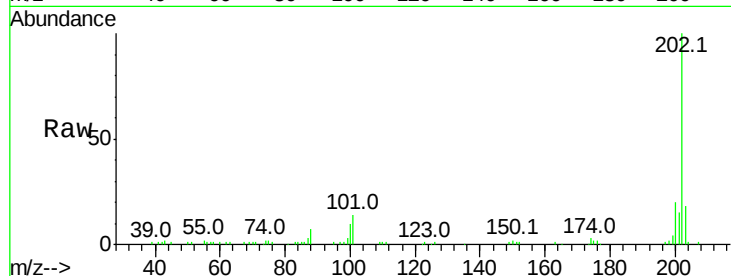

#75
 Chrysene-d12
 Concen: 20.00 ng
 RT: 18.67 min Scan# 2845
 Delta R.T. -0.01 min
 Lab File: BF095532.D
 Acq: 30 May 2017 13:27

Tgt Ion:	240	Resp:	253431
Ion Ratio	Lower	Upper	
240	100		
120	14.7	5.8	8.8#
236	24.5	20.5	30.7

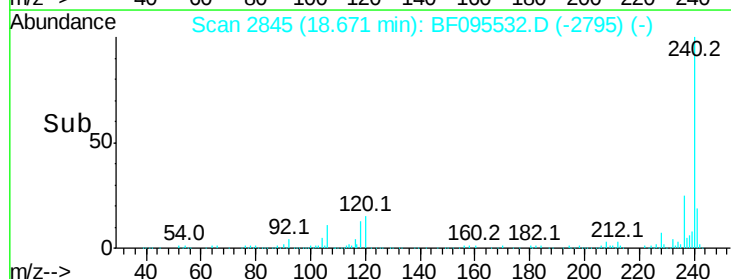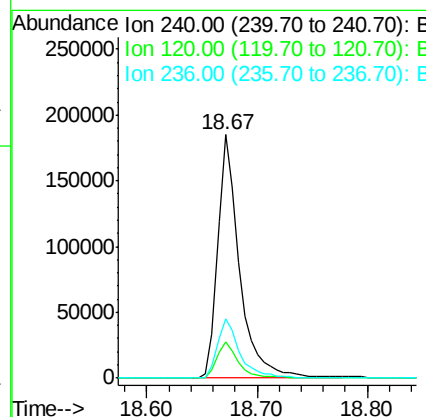



#77

Pvrene

Concen: 4.90 ng

RT: 17.09 min Scan# 2576

Delta R.T. 0.00 min

Lab File: BF095532.D

Acq: 30 May 2017 13:27

Instrument :

BNA_F

ClientSampleId :


Tot Ion:202 Resp: 92922

Ion Ratio Lower Upper

202 100

200 21.2 17.6 26.4




203 18.6 14.4 21.6

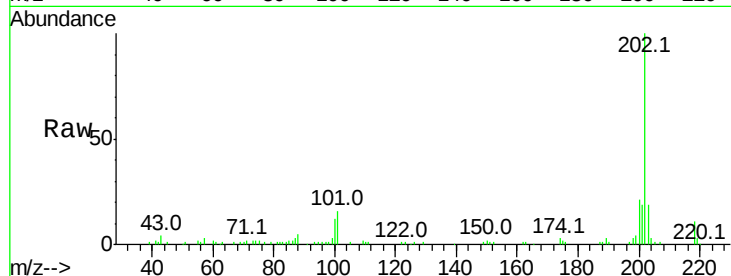

Abundance Ion 202.00 (201.70 to 202.70): E

Ion 200.00 (199.70 to 200.70): E

Ion 203.00 (202.70 to 203.70): E

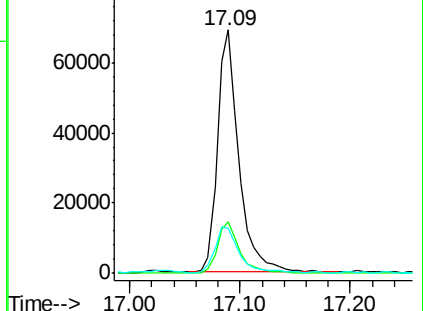

#78

Terphenyl-d14

Concen: 75.97 ng

RT: 17.31 min Scan# 2614

Delta R.T. -0.01 min

Lab File: BF095532.D

Acq: 30 May 2017 13:27


Tgt Ion:244 Resp: 874083

Ion Ratio Lower Upper

244 100

212 6.9 6.0 9.0



122 14.8 10.3 15.5




Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

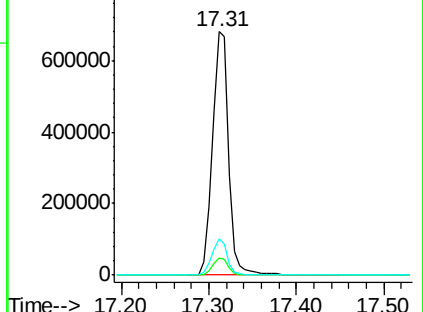



#80

Benzo(a)anthracene

Concen: 2.60 ng

RT: 18.66 min Scan# 2843

Delta R.T. -0.01 min

Lab File: BF095532.D

Acq: 30 May 2017 13:27

Instrument :

BNA_F

ClientSampleId :


Tot Ion:228 Resp: 38375

Ion Ratio Lower Upper

228 100

226 29.2 22.6 33.8




229 23.3 16.3 24.5



Abundance Ion 228.00 (227.70 to 228.70): E

Ion 226.00 (225.70 to 226.70): E

Ion 229.00 (228.70 to 229.70): E

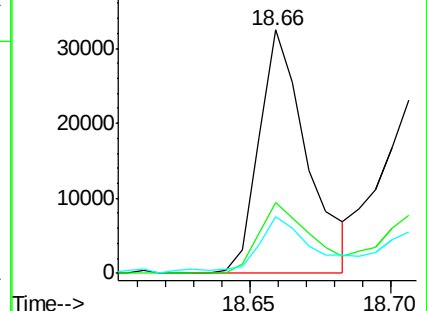

#82

Chrysene

Concen: 2.69 ng

RT: 18.66 min Scan# 2843

Delta R.T. -0.05 min

Lab File: BF095532.D

Acq: 30 May 2017 13:27


Tgt Ion:228 Resp: 38375

Ion Ratio Lower Upper

228 100

226 29.2 24.9 37.3



229 23.3 15.8 23.6




Abundance Ion 228.00 (227.70 to 228.70): E

Ion 226.00 (225.70 to 226.70): E

Ion 229.00 (228.70 to 229.70): E



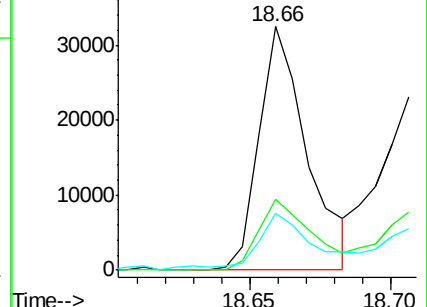



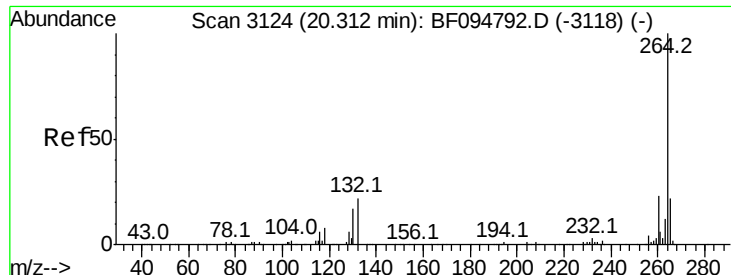

#86
Pervlene-d12
Concen: 20.00 ng
RT: 20.35 min Scan# 3131
Delta R.T. 0.00 min
Lab File: BF095532.D
Acq: 30 May 2017 13:27




Instrument :
BNA_F
ClientSampled :


Tot Ion:264 Resp: 183671
Ion Ratio Lower Upper
264 100
260 23.9 19.5 29.3
265 21.9 17.2 25.8

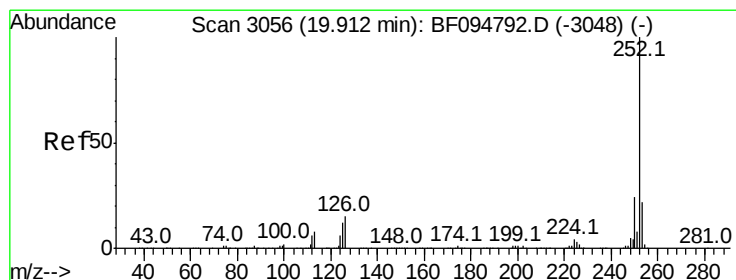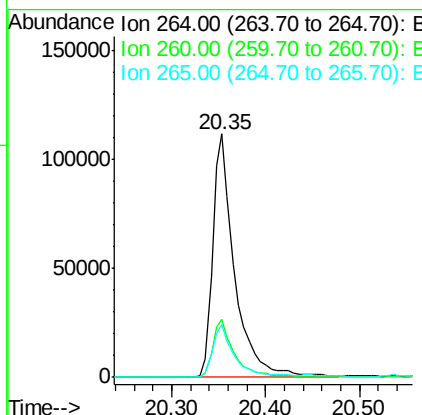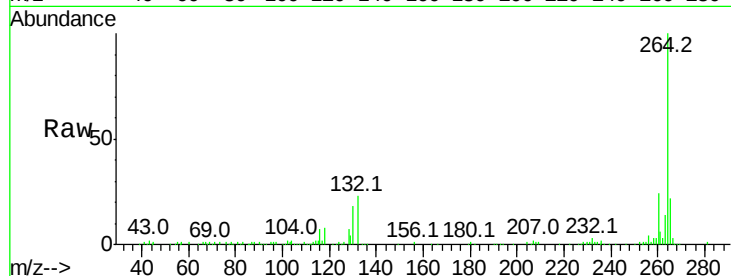

#87
Benzo(b)fluoranthene
Concen: 4.76 ng
RT: 19.95 min Scan# 3063
Delta R.T. 0.01 min
Lab File: BF095532.D
Acq: 30 May 2017 13:27

Tgt Ion:252 Resp: 54060
Ion Ratio Lower Upper
252 100
253 22.8 18.1 27.1
125 16.5 9.8 14.8#


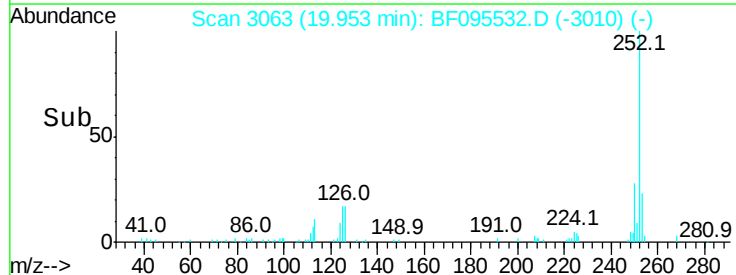
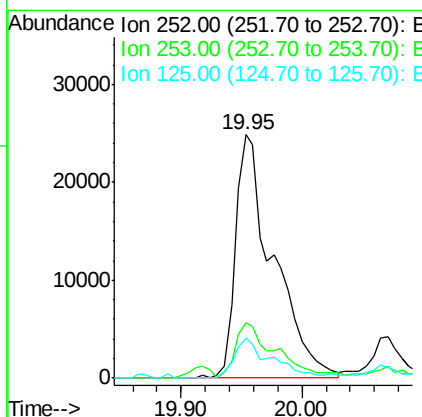
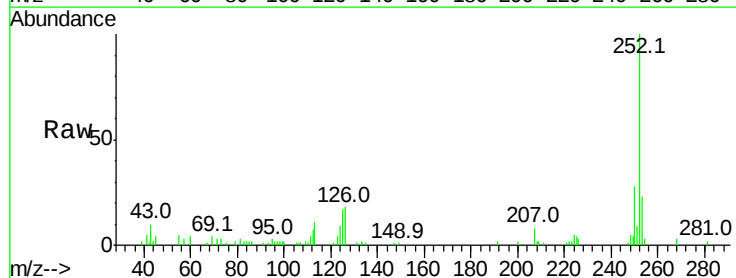


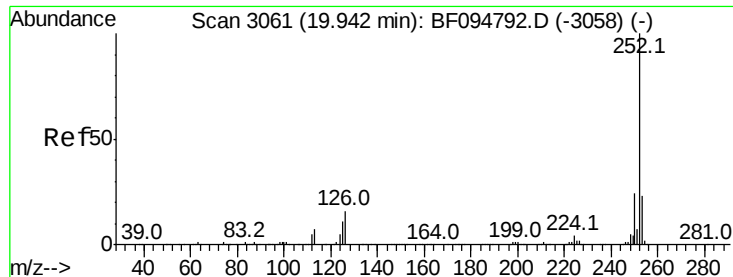

#88
Benzo(k)fluoranthene
Concen: 4.94 ng
RT: 19.95 min Scan# 3063
Delta R.T. -0.02 min
Lab File: BF095532.D
Acq: 30 May 2017 13:27




Instrument :
BNA_F
ClientSampleId :


Tot Ion:252 Resp: 54060
Ion Ratio Lower Upper
252 100
253 22.8 18.4 27.6
125 16.5 13.1 19.7

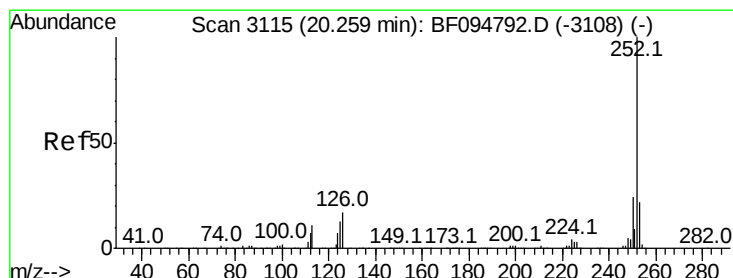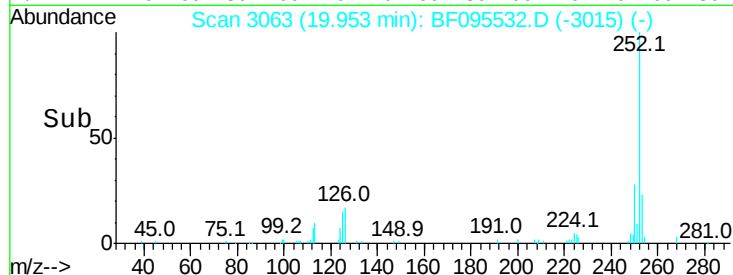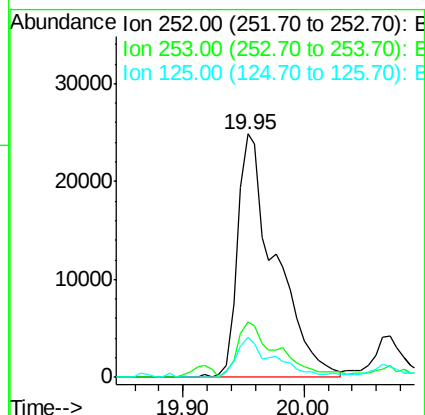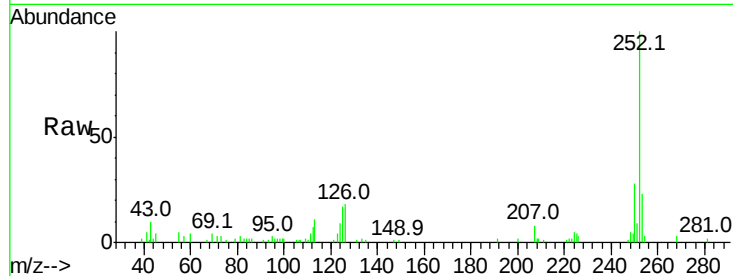

#89
Benzo(a)pyrene
Concen: 2.66 ng
RT: 20.30 min Scan# 3122
Delta R.T. 0.00 min
Lab File: BF095532.D
Acq: 30 May 2017 13:27

Tgt Ion:252 Resp: 27854
Ion Ratio Lower Upper
252 100
253 23.7 17.5 26.3
125 15.7 11.0 16.4

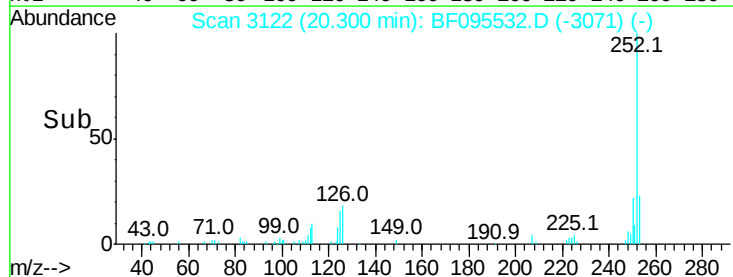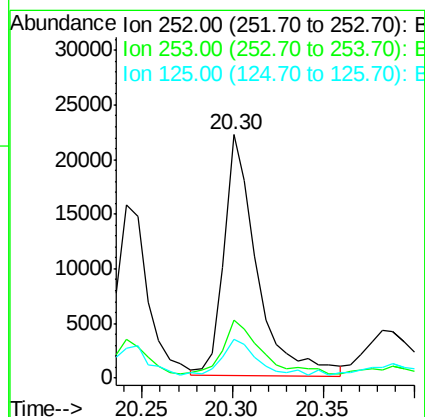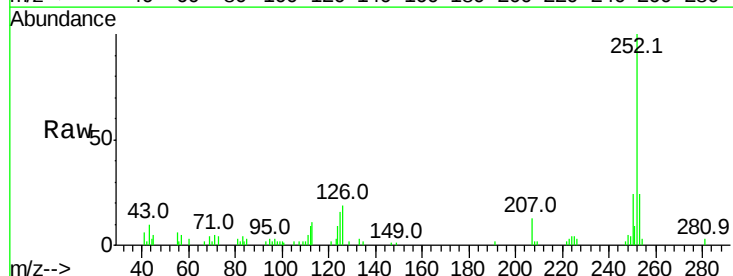

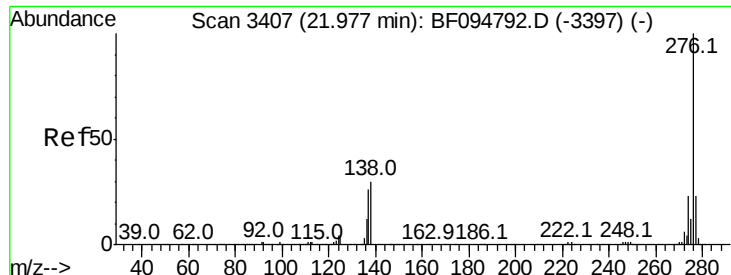

#91

Benzo(a,h,i)perylene

Concen: 2.17 ng

RT: 22.11 min Scan# 3429

Delta R.T. 0.04 min

Lab File: BF095532.D

Acq: 30 May 2017 13:27

Instrument :

BNA_F

ClientSampleId :


Tot Ion: 276 Resp: 18378

Ion Ratio Lower Upper

276 100

277 26.7 18.6 28.0

138 36.2 25.4 38.0



Abundance Ion 276.00 (275.70 to 276.70): E

Ion 277.00 (276.70 to 277.70): E

Ion 138.00 (137.70 to 138.70): E

