
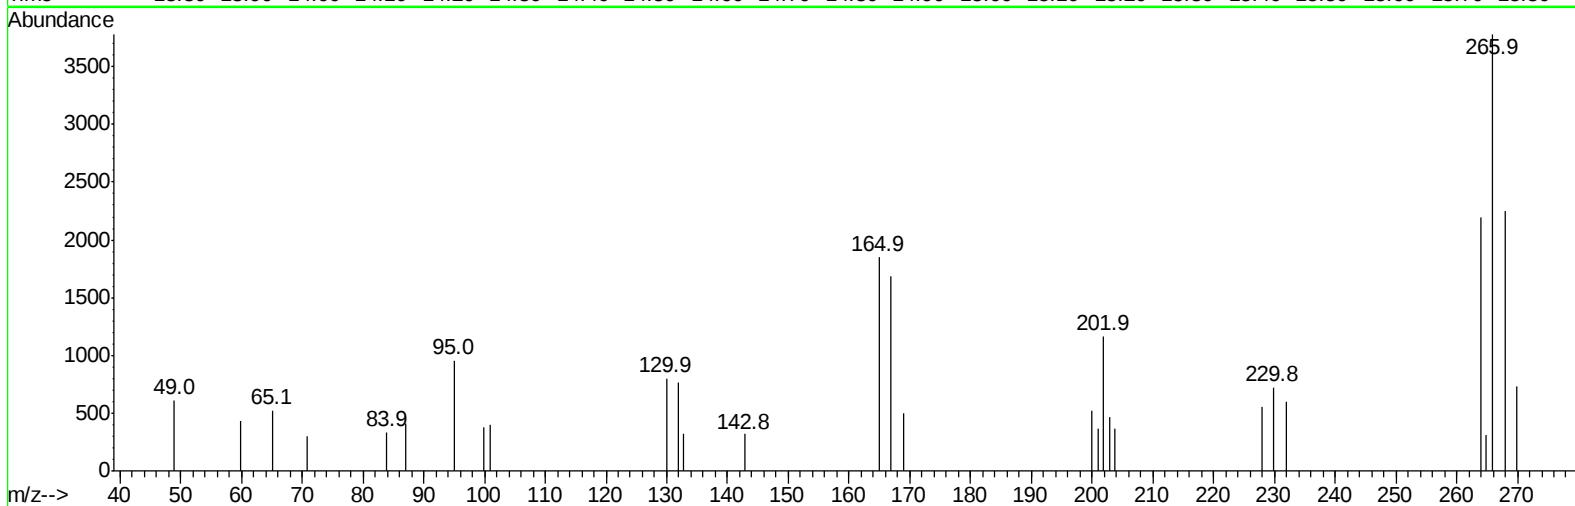


Data Path : Z:\HPCHEM1\BNA F\DATA\BF053017\  
Data File : BF095553.D  
Acq On : 31 May 2017 1:46  
Operator : SJ/MA  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 31 09:33:10 2017  
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF050217.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Fri May 26 16:50:16 2017  
Response via : Initial Calibration

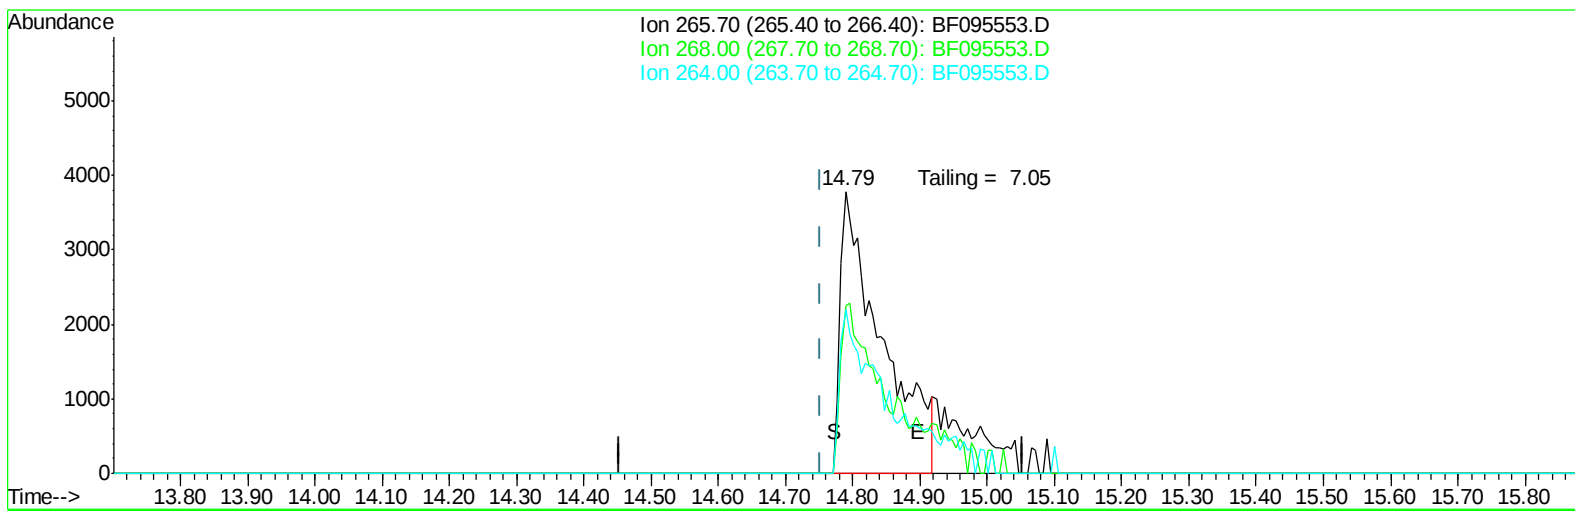

TIC: BF095553.D

(69) Pentachlorophenol (C)



14.789min (+0.035) 0.00ng

response 13429

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 265.70 | 100   | 100   |
| 268.00 | 63.90 | 59.41 |
| 264.00 | 64.60 | 58.03 |
| 0.00   | 0.00  | 0.00  |

Data Path : Z:\HPCHEM1\BNA F\DATA\BF053017\  
Data File : BF095553.D  
Acq On : 31 May 2017 1:46  
Operator : SJ/MA  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 31 09:33:10 2017  
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF050217.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Fri May 26 16:50:16 2017  
Response via : Initial Calibration

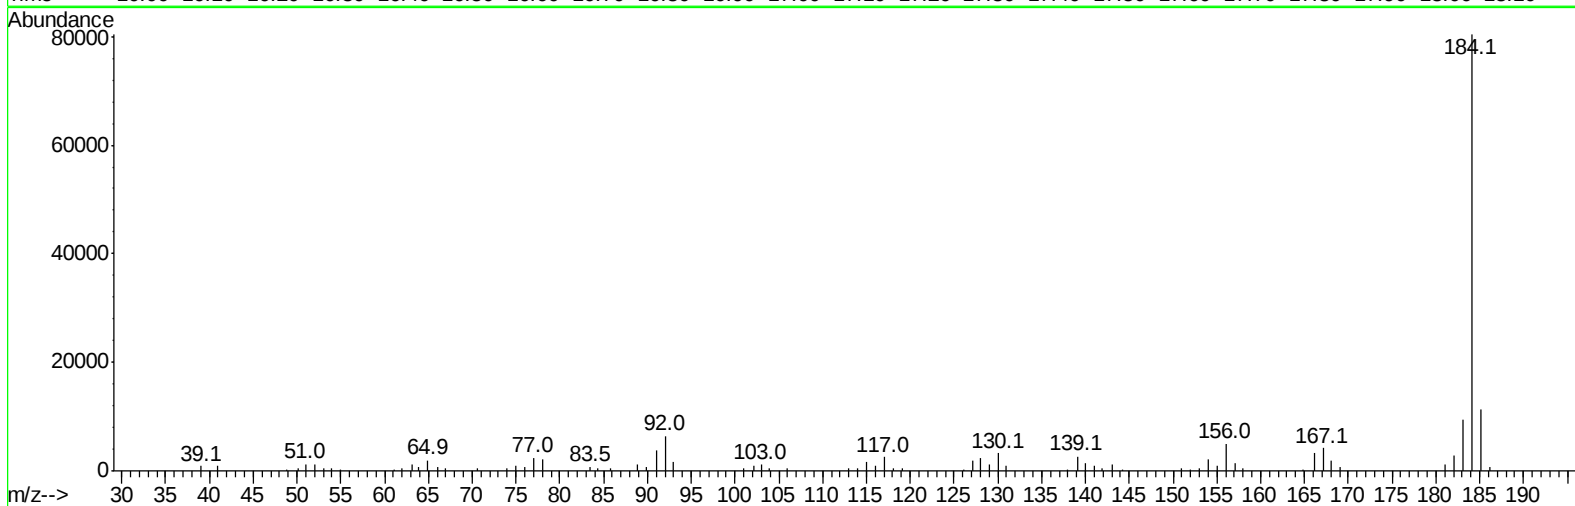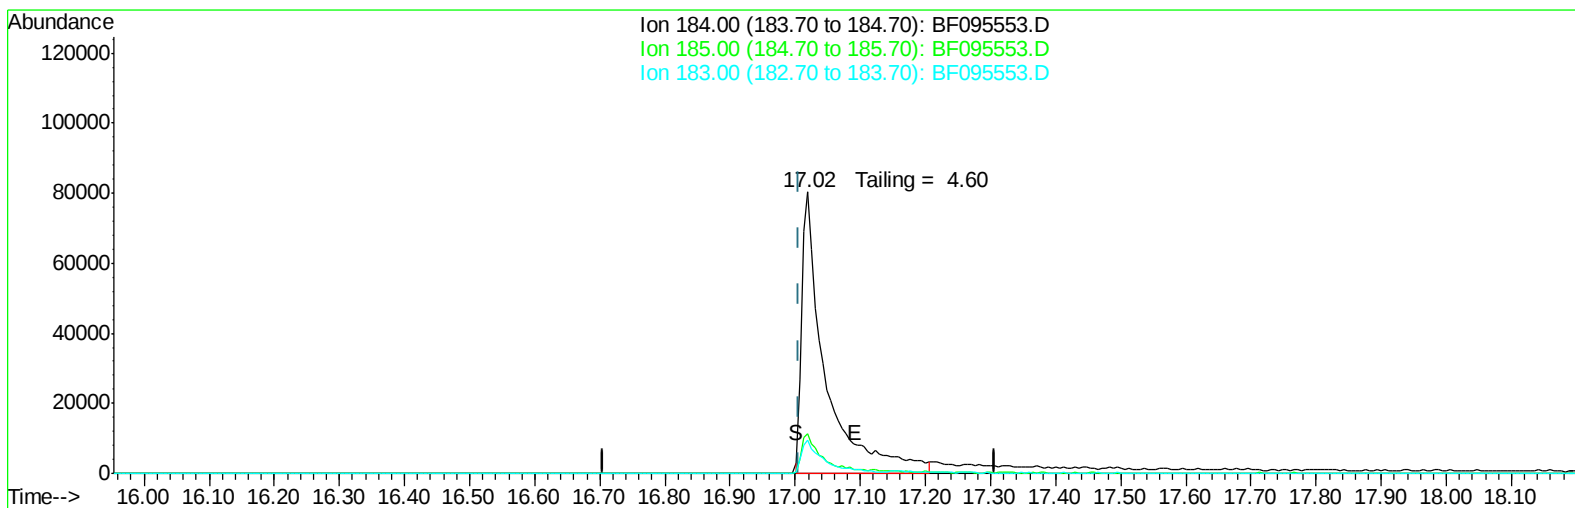

TIC: BF095553.D

(76) Benzidine

17.018min (+0.012) 0.00ng

response 203728

| Ion    | Exp%  | Act%   |
|--------|-------|--------|
| 184.00 | 100   | 100    |
| 185.00 | 19.40 | 13.97# |
| 183.00 | 12.20 | 11.74  |
| 0.00   | 0.00  | 0.00   |