


Data Path : Z:\HPCHEM1\BNA_F\Data\BF053017\
 Data File : BF095529.D
 Acq On : 30 May 2017 11:18
 Operator : SJ/MA
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF050217.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri May 26 16:50:16 2017

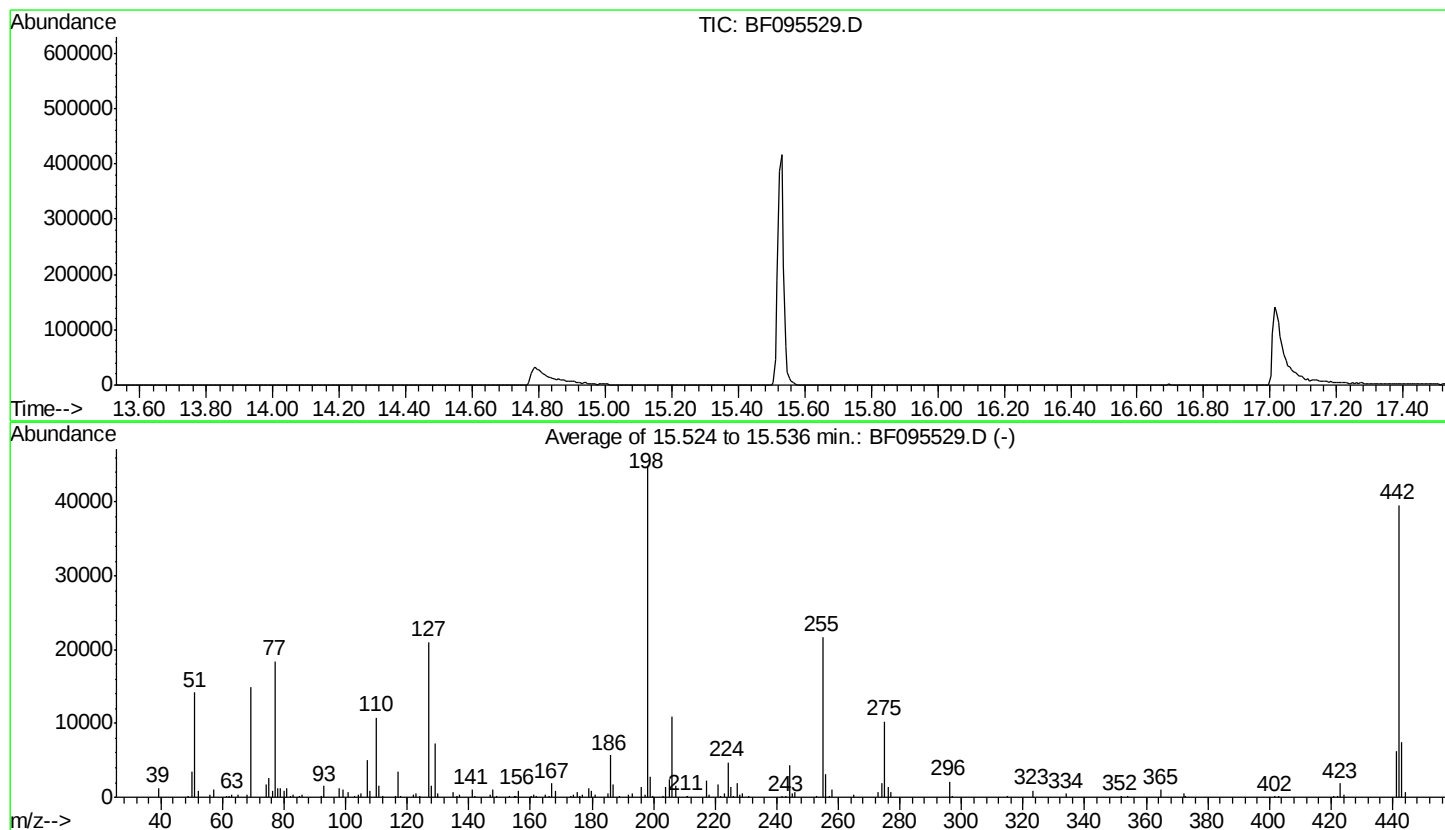

AutoFind: Scans 2310, 2311, 2312; Background Corrected with Scan 2304

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	31.6	14183	PASS
68	69	0.00	2	2.2	327	FAIL*
69	198	0.00	100	33.1	14872	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	46.9	21063	PASS
197	198	0.00	2	0.7	300	PASS
198	198	100	100	100.0	44946	PASS
199	198	5	9	6.2	2768	PASS
275	198	10	60	22.8	10239	PASS
365	198	1	100	2.3	1038	PASS
441	442	0.01	24	15.7	6243	PASS
442	198	50	100	88.2	39645	PASS
443	442	15	24	19.0	7547	PASS