


Data Path : Z:\HPCHEM1\BNA_F\Data\BF053017\
 Data File : BF095530.D
 Acq On : 30 May 2017 12:17
 Operator : SJ/MA
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF050217.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri May 26 16:50:16 2017

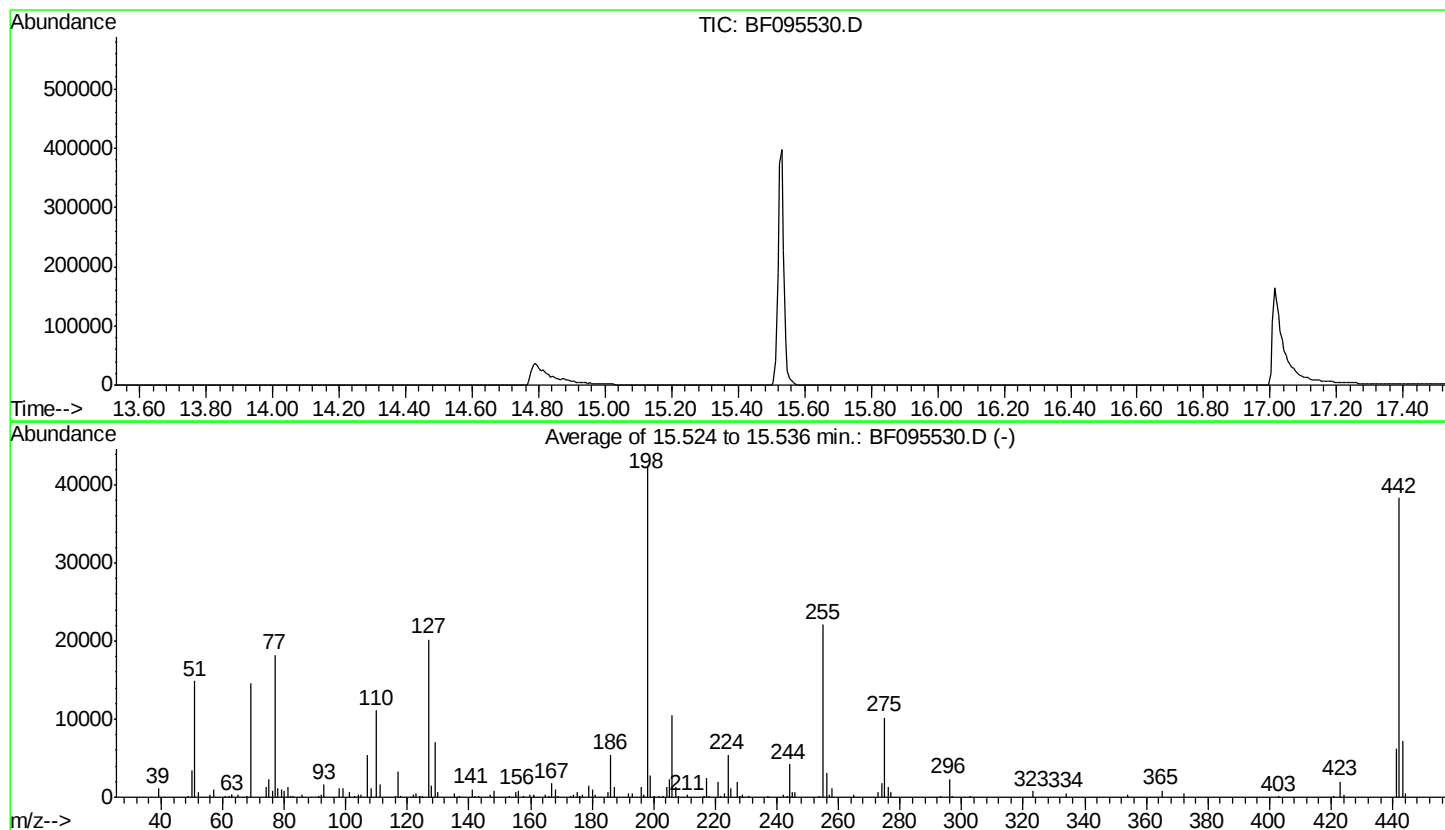

AutoFind: Scans 2310, 2311, 2312; Background Corrected with Scan 2304

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.0	14883	PASS
68	69	0.00	2	0.9	125	PASS
69	198	0.00	100	34.3	14580	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	47.5	20175	PASS
197	198	0.00	2	0.6	276	PASS
198	198	100	100	100.0	42466	PASS
199	198	5	9	6.5	2760	PASS
275	198	10	60	24.0	10176	PASS
365	198	1	100	2.0	851	PASS
441	442	0.01	24	16.2	6222	PASS
442	198	50	100	90.3	38354	PASS
443	442	15	24	19.0	7294	PASS