


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF053017\
 Data File : BF095553.D
 Acq On : 31 May 2017 1:46
 Operator : SJ/MA
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF050217.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri May 26 16:50:16 2017

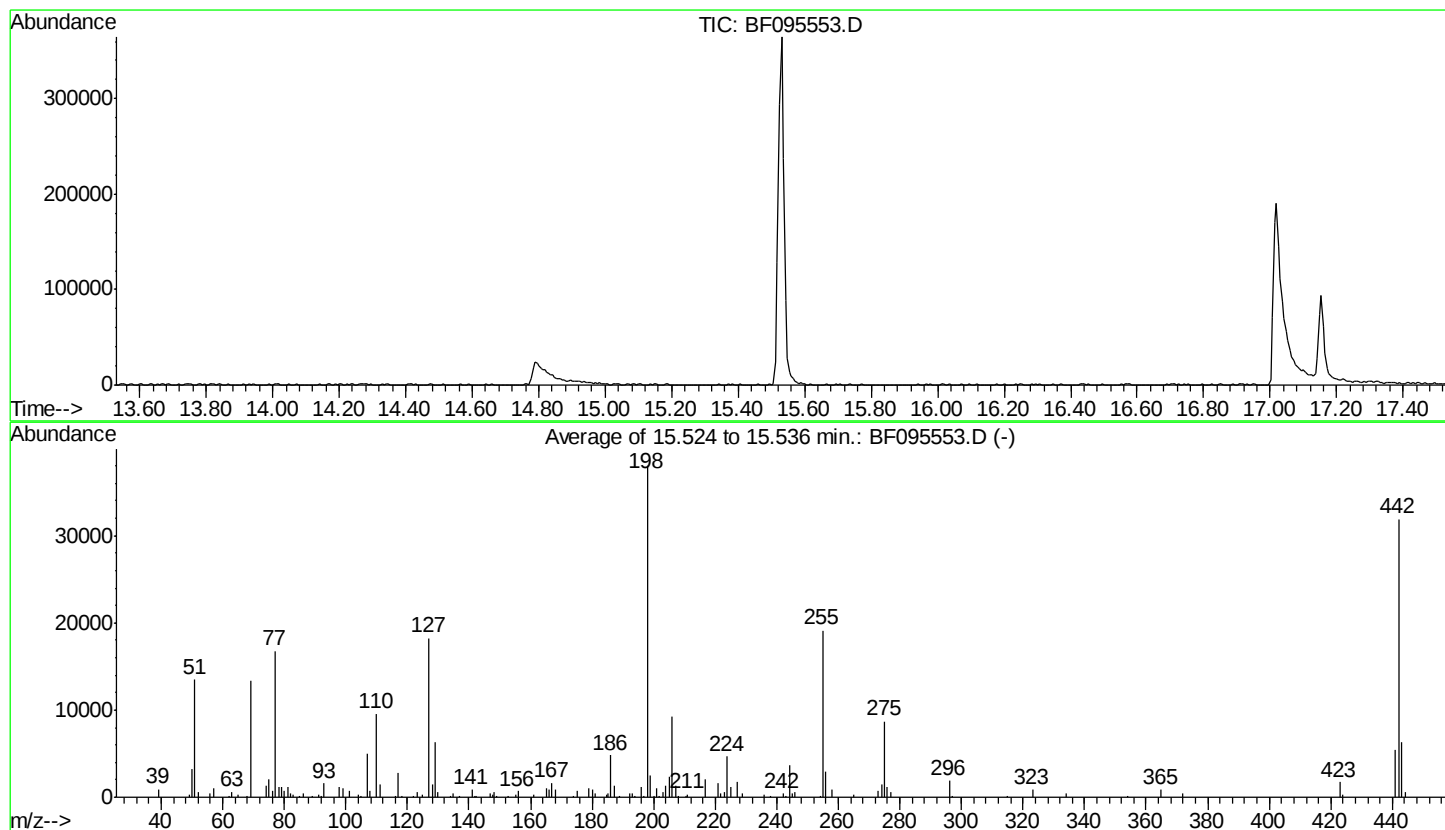

AutoFind: Scans 2310, 2311, 2312; Background Corrected with Scan 2304

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.5	13499	PASS
68	69	0.00	2	0.9	124	PASS
69	198	0.00	100	35.0	13300	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	48.0	18252	PASS
197	198	0.00	2	0.4	136	PASS
198	198	100	100	100.0	38029	PASS
199	198	5	9	6.5	2487	PASS
275	198	10	60	22.9	8700	PASS
365	198	1	100	2.3	864	PASS
441	442	0.01	24	16.9	5401	PASS
442	198	50	100	83.9	31901	PASS
443	442	15	24	19.9	6336	PASS