
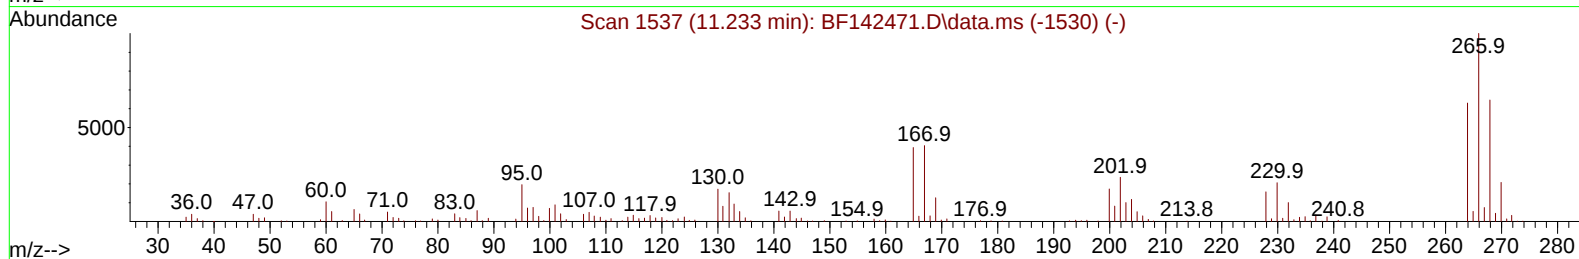
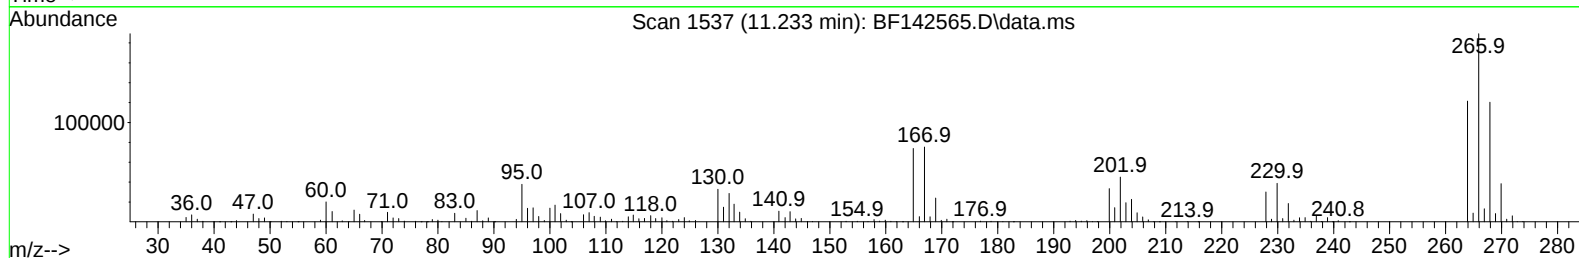


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF053025\
Data File : BF142565.D
Acq On : 30 May 2025 12:23
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 30 13:07:01 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052025.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 20 16:26:47 2025
Response via : Initial Calibration

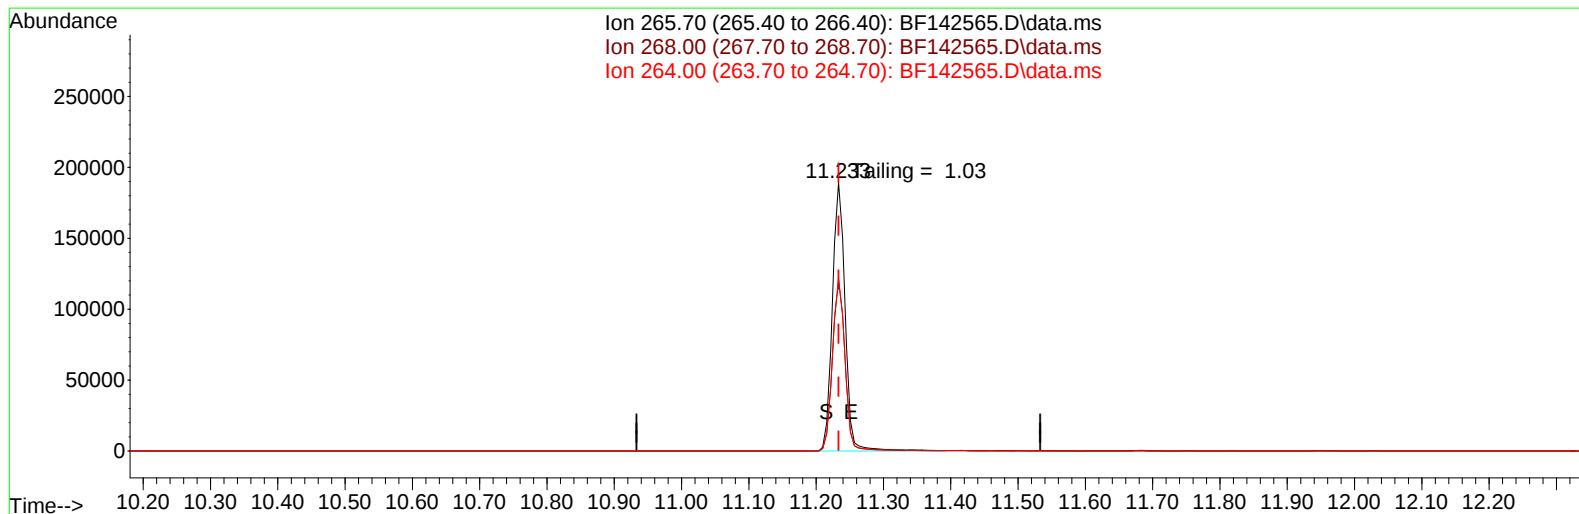

TIC: BF142565.D\data.ms

(70) Pentachlorophenol (C)




11.233min (+ 0.000) 56283.72 ng

response 248099

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.60	63.62
264.00	63.00	64.21
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF053025\
Data File : BF142565.D
Acq On : 30 May 2025 12:23
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 30 13:07:01 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052025.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 20 16:26:47 2025
Response via : Initial Calibration

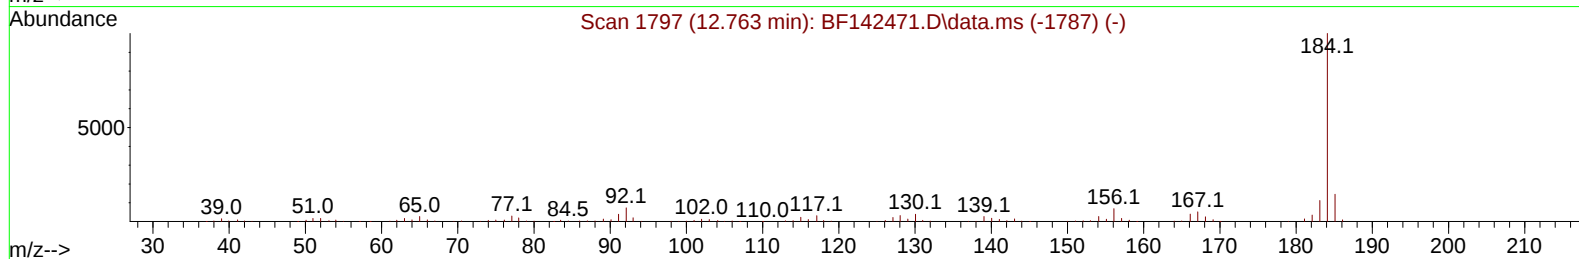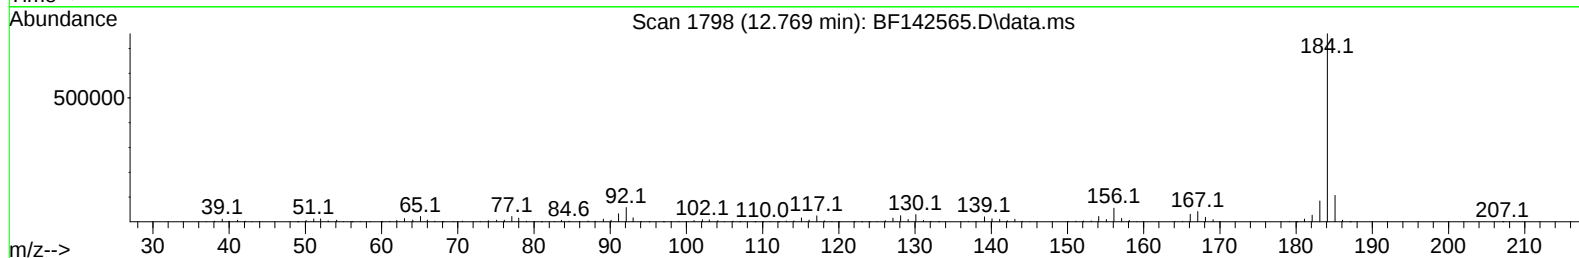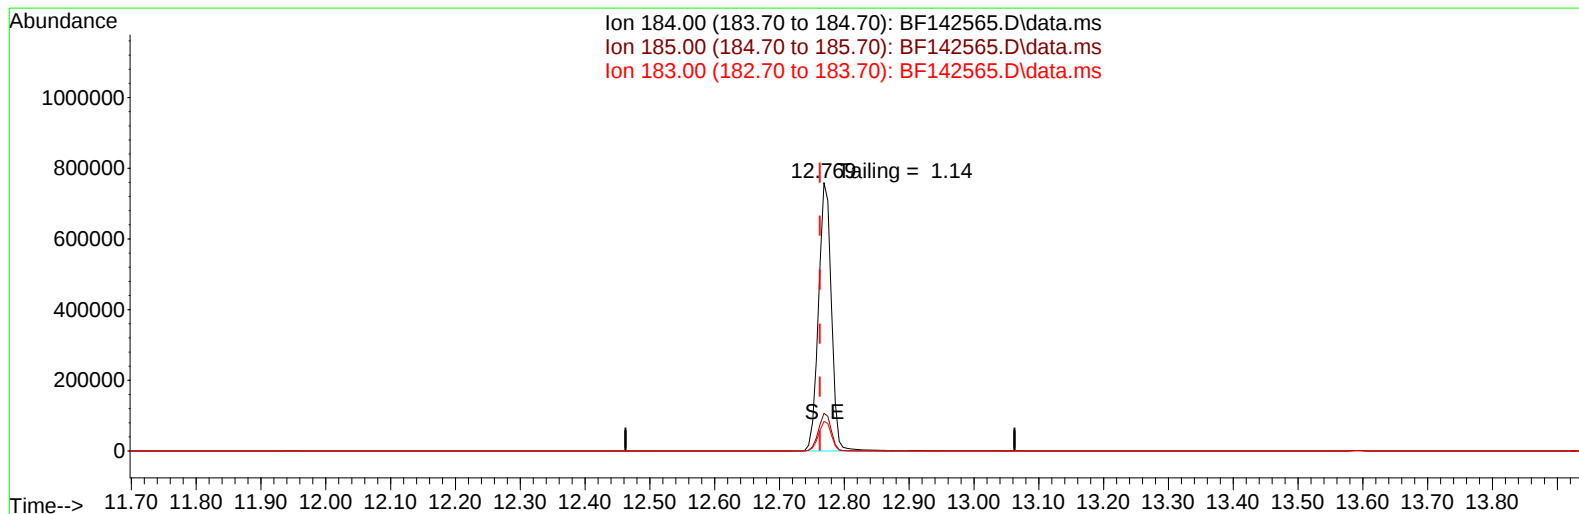

TIC: BF142565.D\data.ms

(77) Benzidine

12.769min (+ 0.006) 59056.94 ng

response 1057087

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.50	14.09
183.00	11.20	11.08
0.00	0.00	0.00