

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF053025\
 Data File : BF142570.D
 Acq On : 30 May 2025 15:21
 Operator : RC/JU
 Sample : Q2150-09
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 TP-54

Quant Time: May 30 15:43:17 2025
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052025.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue May 20 16:26:47 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	6.898	152	118247	20.000	ng	0.00
21) Naphthalene-d8	8.181	136	441924	20.000	ng	0.00
39) Acenaphthene-d10	9.933	164	231484	20.000	ng	-0.01
64) Phenanthrene-d10	11.422	188	379392	20.000	ng	-0.01
76) Chrysene-d12	14.068	240	216438	20.000	ng	0.00
86) Perylene-d12	15.562	264	226398	20.000	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.516	112	756406	107.771	ng	0.00
7) Phenol-d6	6.522	99	949761	112.414	ng	-0.01
23) Nitrobenzene-d5	7.457	82	557041	68.733	ng	-0.02
42) 2,4,6-Tribromophenol	10.727	330	303025	117.946	ng	-0.01
45) 2-Fluorobiphenyl	9.257	172	1081028	62.665	ng	-0.01
79) Terphenyl-d14	13.010	244	985998	62.254	ng	0.00


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF053025\
Data File : BF142570.D
Acq On : 30 May 2025 15:21
Operator : RC/JU
Sample : Q2150-09
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
TP-54

Quant Time: May 30 15:43:17 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052025.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 20 16:26:47 2025
Response via : Initial Calibration




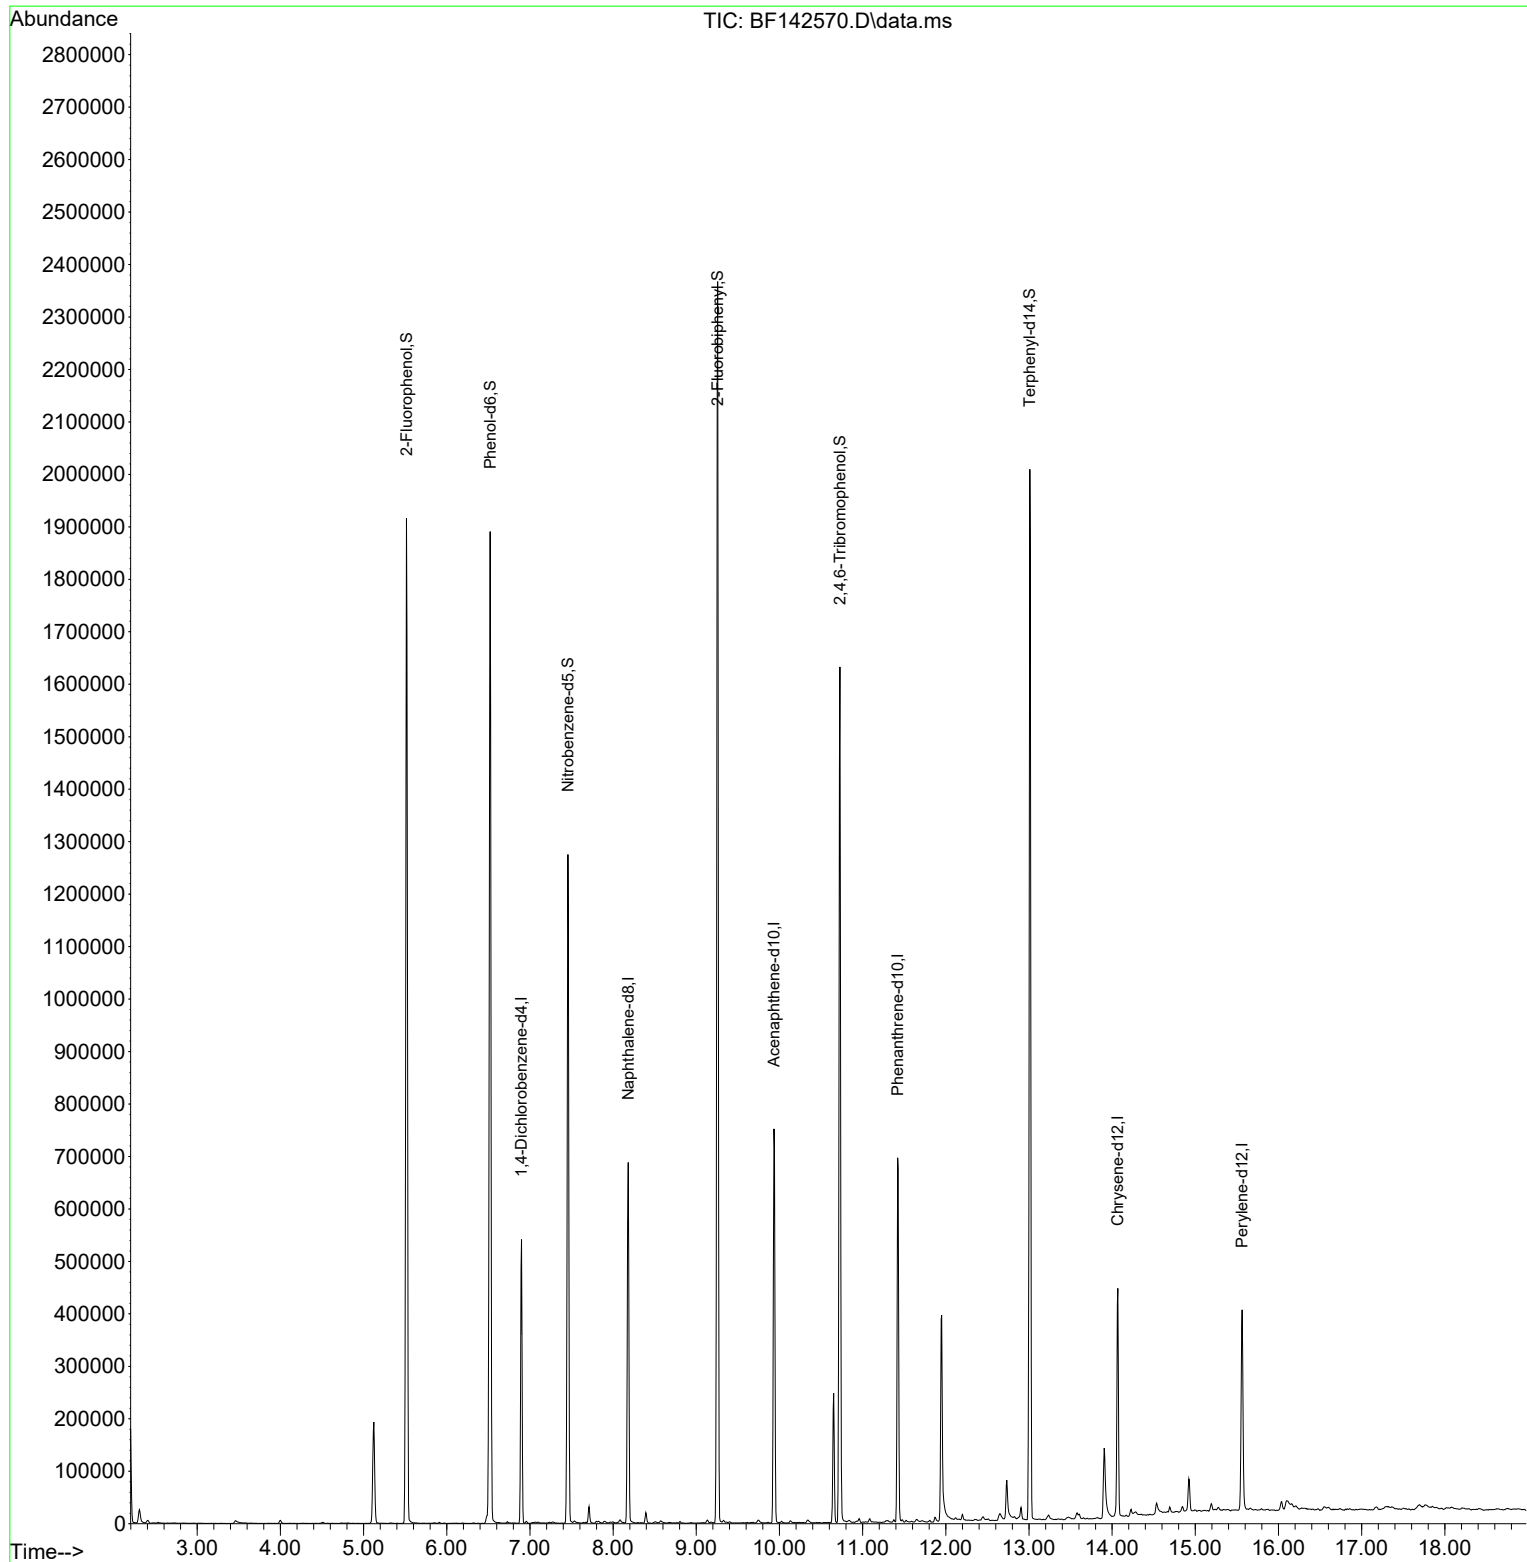




#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.898 min Scan# 800
Delta R.T. -0.006 min
Lab File: BF142570.D
Acq: 30 May 2025 15:21




Instrument :
BNA_F
ClientSampleId :
TP-54


Tgt Ion:152 Resp: 118247
Ion Ratio Lower Upper
152 100
150 153.9 128.2 192.4
115 56.6 48.3 72.5

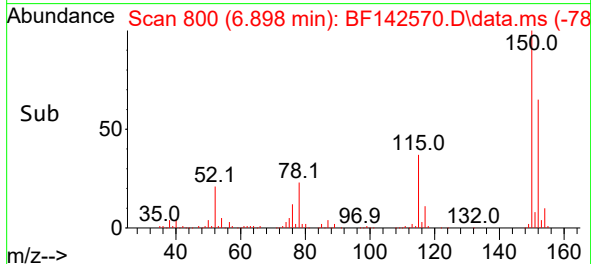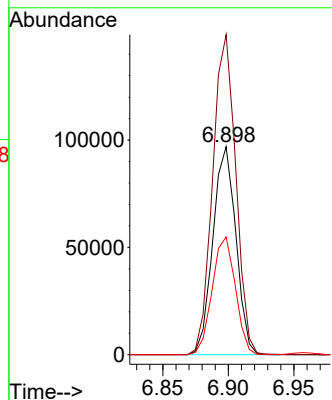

#5
2-Fluorophenol
Concen: 107.771 ng
RT: 5.516 min Scan# 565
Delta R.T. 0.000 min
Lab File: BF142570.D
Acq: 30 May 2025 15:21

Tgt Ion:112 Resp: 756406
Ion Ratio Lower Upper
112 100
64 58.8 47.5 71.3
63 30.7 24.9 37.3


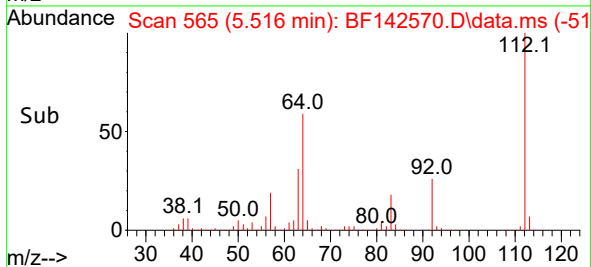
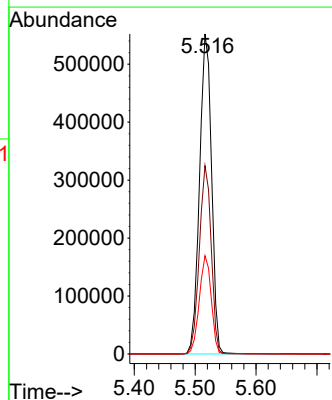
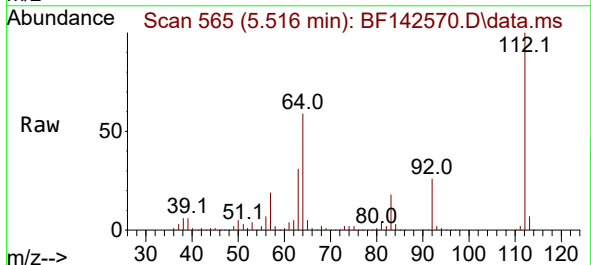


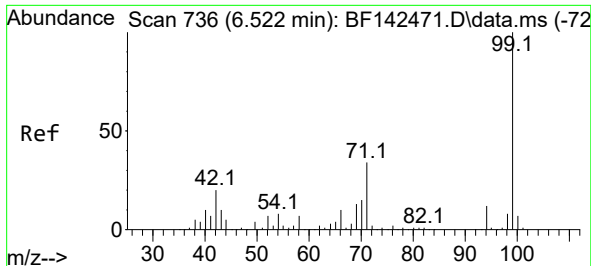

#7
Phenol-d6
Concen: 112.414 ng
RT: 6.522 min Scan# 71
Delta R.T. -0.012 min
Lab File: BF142570.D
Acq: 30 May 2025 15:21




Instrument :
BNA_F
ClientSampleId :
TP-54


Tgt Ion: 99 Resp: 949761
Ion Ratio Lower Upper
99 100
42 19.4 16.2 24.2
71 33.1 27.3 40.9

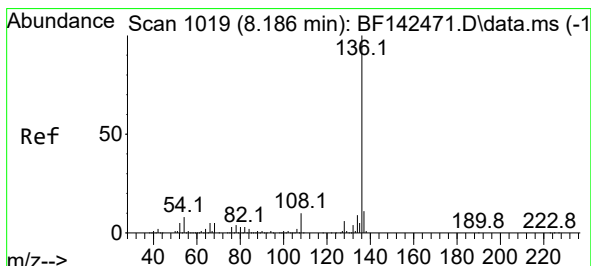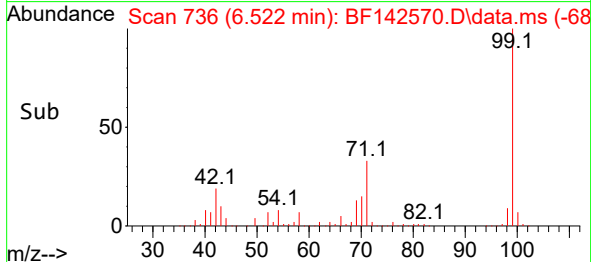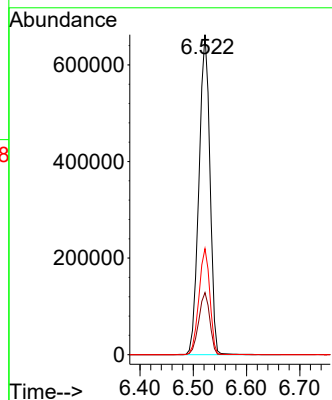

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 8.181 min Scan# 1018
Delta R.T. -0.006 min
Lab File: BF142570.D
Acq: 30 May 2025 15:21

Tgt Ion:136 Resp: 441924
Ion Ratio Lower Upper
136 100
137 10.9 8.6 13.0
54 8.4 6.6 10.0
68 5.5 4.1 6.1

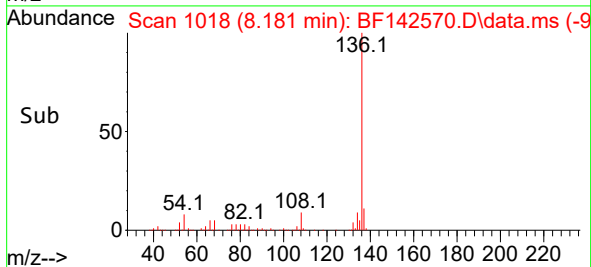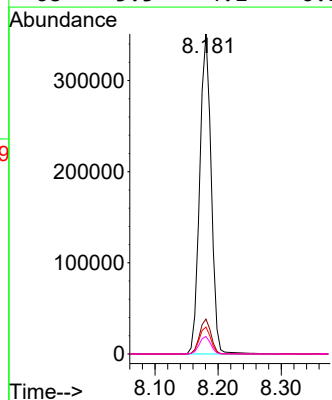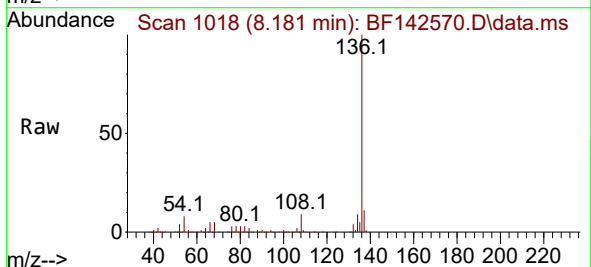

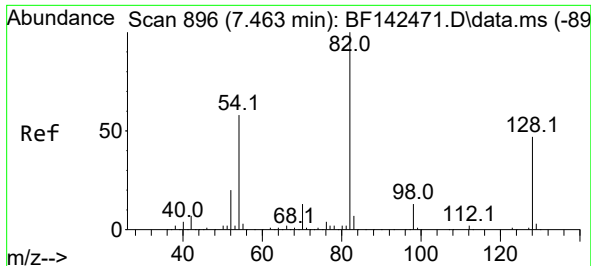

#23

Nitrobenzene-d5

Concen: 68.733 ng

RT: 7.457 min Scan# 895

Delta R.T. -0.018 min

Lab File: BF142570.D

Acq: 30 May 2025 15:21

Instrument :

BNA_F

ClientSampleId :

TP-54





Tgt Ion: 82 Resp: 557041

Ion Ratio Lower Upper

82 100

128 48.3 37.4 56.2

54 57.4 46.6 70.0

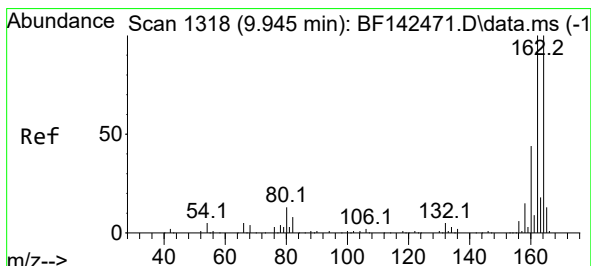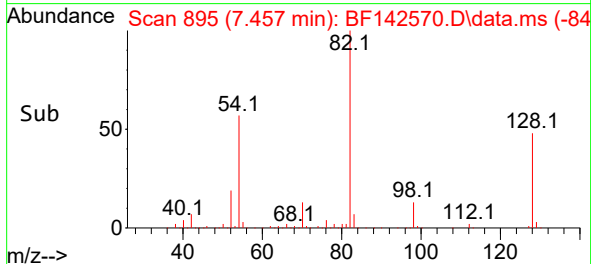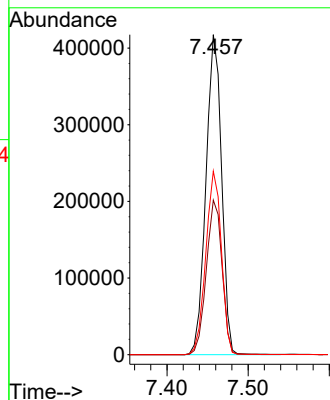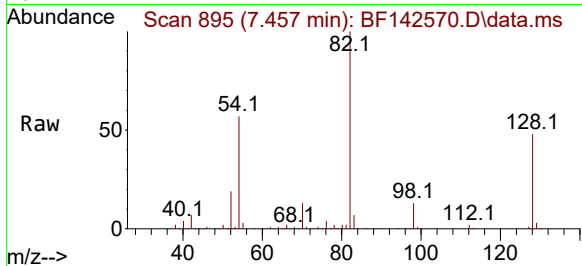

#39

Acenaphthene-d10

Concen: 20.000 ng

RT: 9.933 min Scan# 1316

Delta R.T. -0.012 min

Lab File: BF142570.D

Acq: 30 May 2025 15:21




Tgt Ion:164 Resp: 231484


Ion Ratio Lower Upper

164 100

162 100.4 80.2 120.4

160 44.1 35.6 53.4



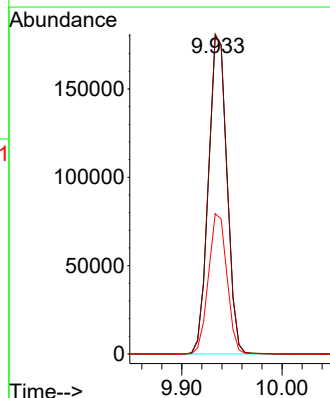
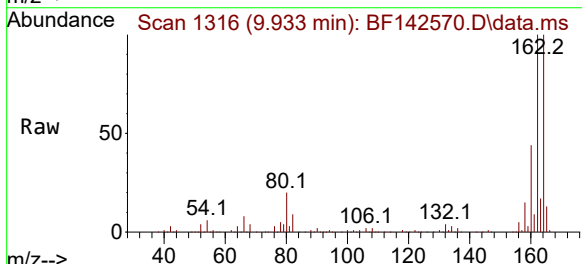


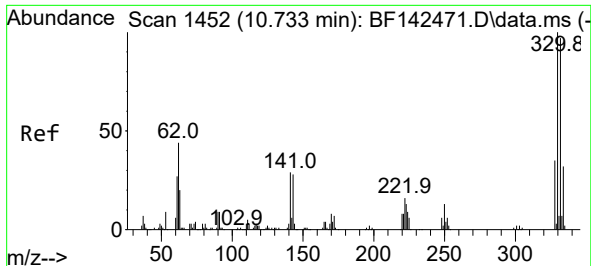

#42
 2,4,6-Tribromophenol
 Concen: 117.946 ng
 RT: 10.727 min Scan# 1451
 Delta R.T. -0.012 min
 Lab File: BF142570.D
 Acq: 30 May 2025 15:21




Instrument :
 BNA_F
 ClientSampleId :
 TP-54


Tgt Ion: 330 Resp: 303025
 Ion Ratio Lower Upper
 330 100
 332 94.8 77.6 116.4
 141 28.5 24.6 36.8

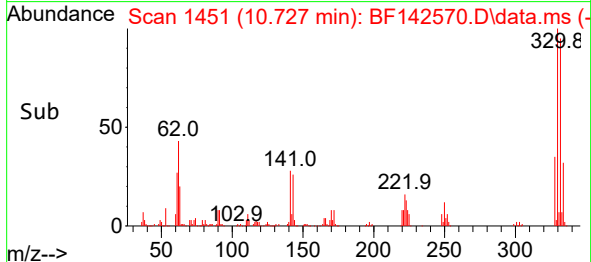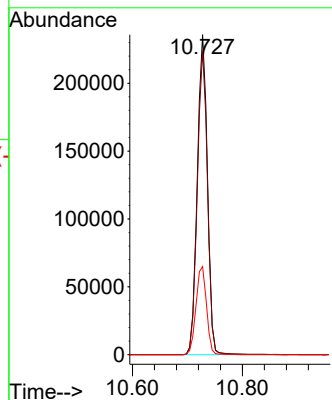

#45
 2-Fluorobiphenyl
 Concen: 62.665 ng
 RT: 9.257 min Scan# 1201
 Delta R.T. -0.012 min
 Lab File: BF142570.D
 Acq: 30 May 2025 15:21

Tgt Ion: 172 Resp: 1081028
 Ion Ratio Lower Upper
 172 100
 171 35.5 28.6 42.8
 170 23.2 18.9 28.3

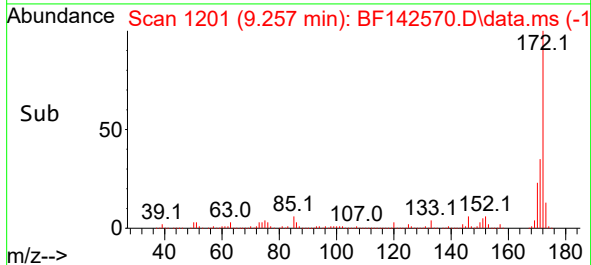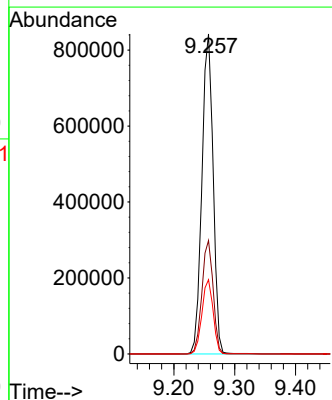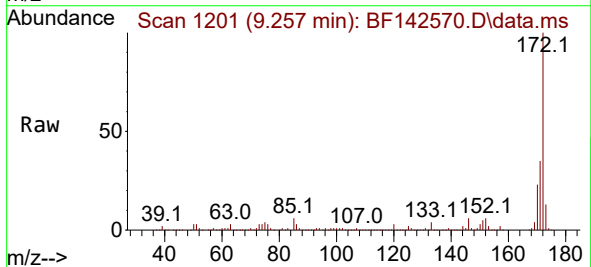



#64

Phenanthrene-d10

Concen: 20.000 ng

RT: 11.422 min Scan# 1

Delta R.T. -0.012 min

Lab File: BF142570.D

Acq: 30 May 2025 15:21

Instrument :

BNA_F

ClientSampleId :

TP-54





Tgt Ion:188 Resp: 379392

Ion Ratio Lower Upper

188 100

94 9.5 6.6 10.0

80 9.7 7.4 11.0

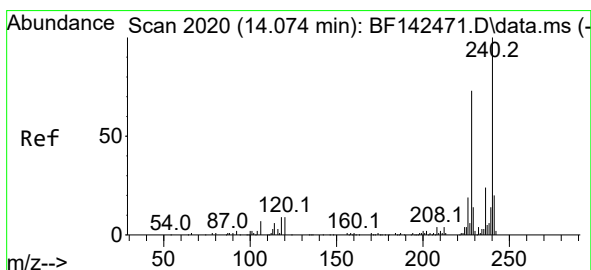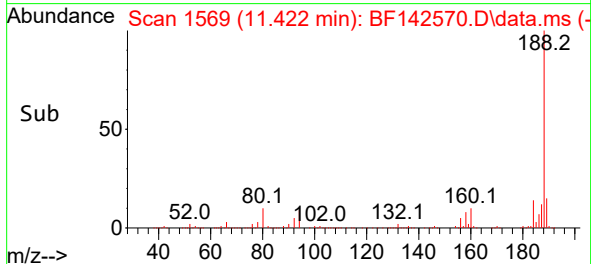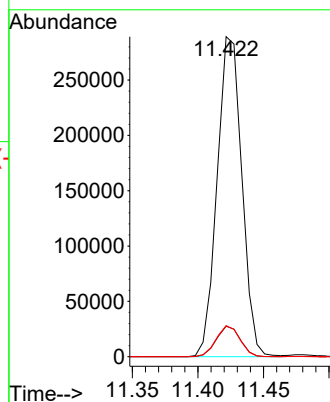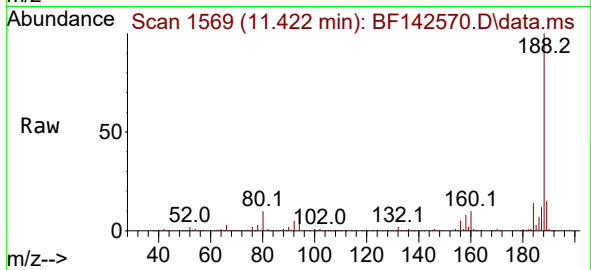

#76

Chrysene-d12

Concen: 20.000 ng

RT: 14.068 min Scan# 2019

Delta R.T. -0.006 min

Lab File: BF142570.D

Acq: 30 May 2025 15:21




Tgt Ion:240 Resp: 216438


Ion Ratio Lower Upper

240 100

120 10.3 7.5 11.3

236 25.1 19.6 29.4


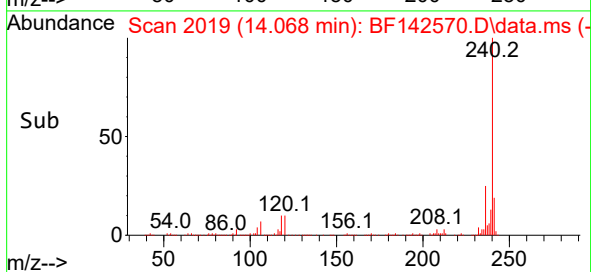
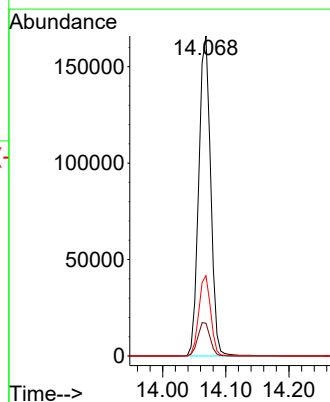
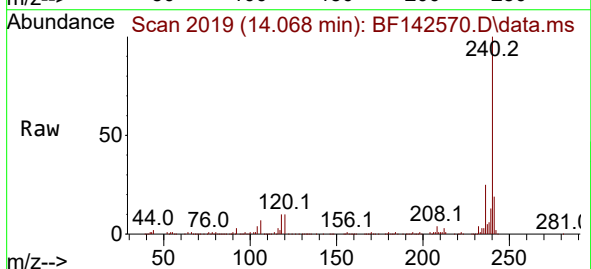


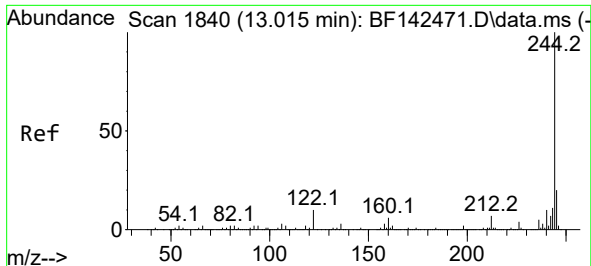

#79
 Terphenyl-d14
 Concen: 62.254 ng
 RT: 13.010 min Scan# 1839
 Delta R.T. -0.006 min
 Lab File: BF142570.D
 Acq: 30 May 2025 15:21

Instrument :
 BNA_F
 ClientSampleId :
 TP-54

Tgt Ion:244 Resp: 985998
 Ion Ratio Lower Upper
 244 100
 212 6.7 5.3 7.9
 122 11.0 8.2 12.2

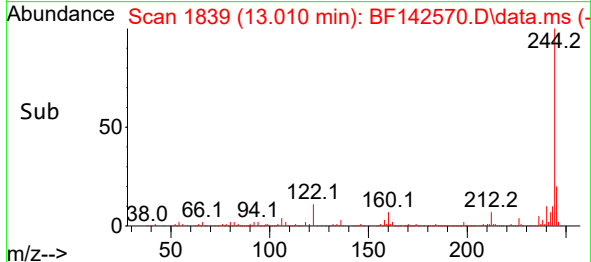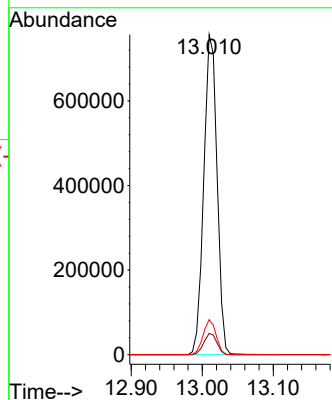

#86
 Perylene-d12
 Concen: 20.000 ng
 RT: 15.562 min Scan# 2273
 Delta R.T. -0.006 min
 Lab File: BF142570.D
 Acq: 30 May 2025 15:21

Tgt Ion:264 Resp: 226398
 Ion Ratio Lower Upper
 264 100
 260 23.4 18.6 28.0
 265 21.1 17.7 26.5

