


Data Path : Z:\HPCHEM1\BNA_F\Data\BF053115\
 Data File : BF079629.D
 Acq On : 31 May 2015 11:04
 Operator : TP/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF052615.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Jun 01 03:28:53 2015

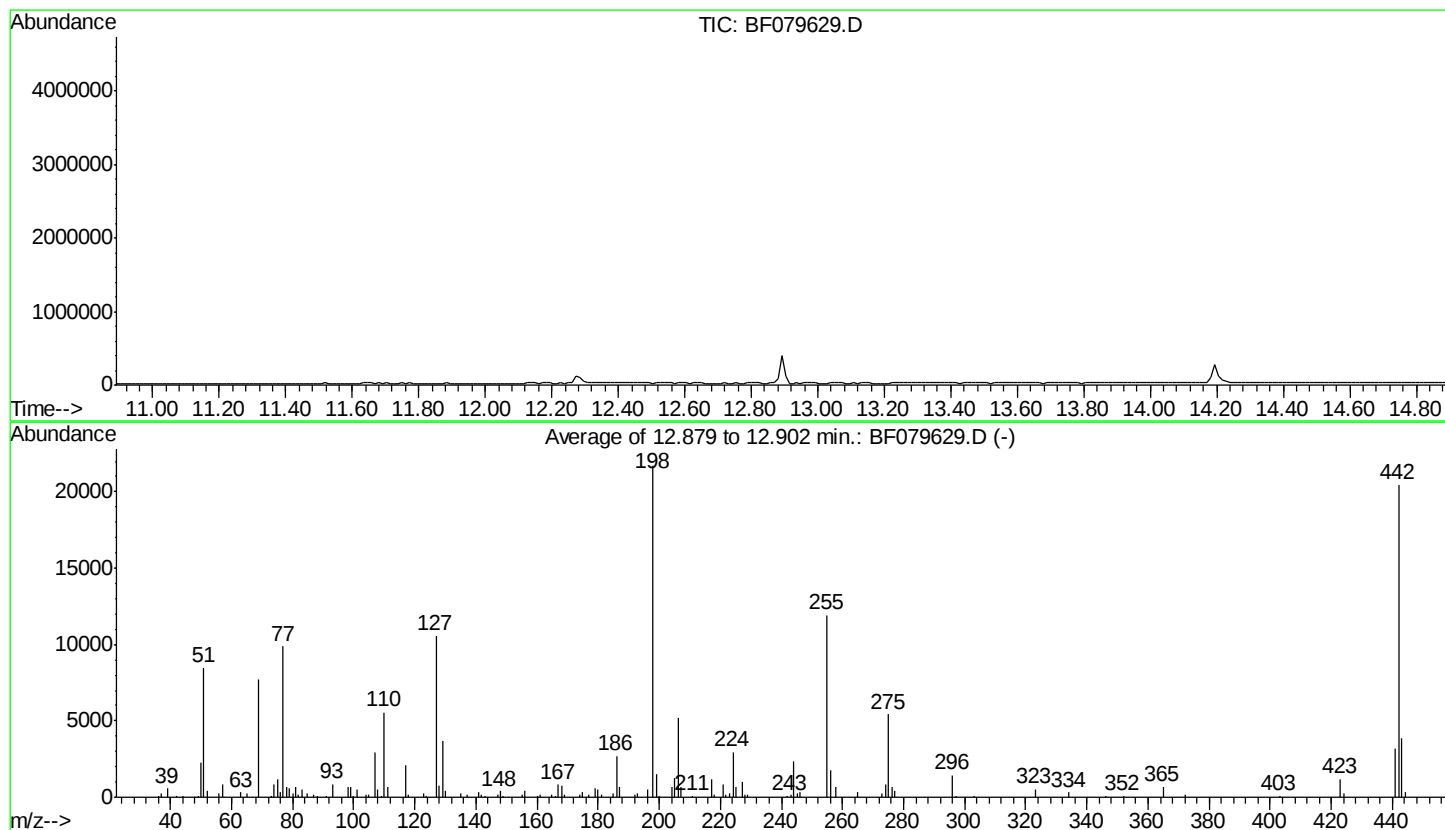

AutoFind: Scans 1023, 1024, 1025; Background Corrected with Scan 1020

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	39.1	8480	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	35.6	7733	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	48.8	10598	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	21711	PASS
199	198	5	9	6.8	1481	PASS
275	198	10	60	25.0	5421	PASS
365	198	1	100	3.3	708	PASS
441	442	0.01	24	15.5	3168	PASS
442	198	50	100	94.2	20459	PASS
443	442	15	24	19.0	3884	PASS