

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF053115\
Data File : BF079639.D
Acq On : 31 May 2015 18:10
Operator : TP/IZ
Sample : G2416-26 5X
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
RAMP440NB-TP5.4(6)

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF052615.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.633	38	39	81	rVB	3694967	8697006	100.00%	64.687%
2	6.902	498	500	503	rBV	320569	341943	3.93%	2.543%
3	8.479	636	638	641	rBV	443286	494441	5.69%	3.678%
4	10.651	825	828	830	rVB	503595	563675	6.48%	4.193%
5	12.479	986	988	991	rBV	645822	615437	7.08%	4.577%
6	15.005	1204	1209	1211	rBV4	29486	97625	1.12%	0.726%
7	15.748	1271	1274	1276	rBV	612515	715077	8.22%	5.319%
8	15.874	1276	1285	1291	rVV	131585	773586	8.89%	5.754%
9	16.445	1332	1335	1341	rVB	123049	377631	4.34%	2.809%
10	17.451	1420	1423	1426	rBV	479227	768414	8.84%	5.715%


Sum of corrected areas: 13444835

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF053115\
Data File : BF079639.D
Acq On : 31 May 2015 18:10
Operator : TP/IZ
Sample : G2416-26 5X
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
RAMP440NB-TP5.4(6)

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF052615.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

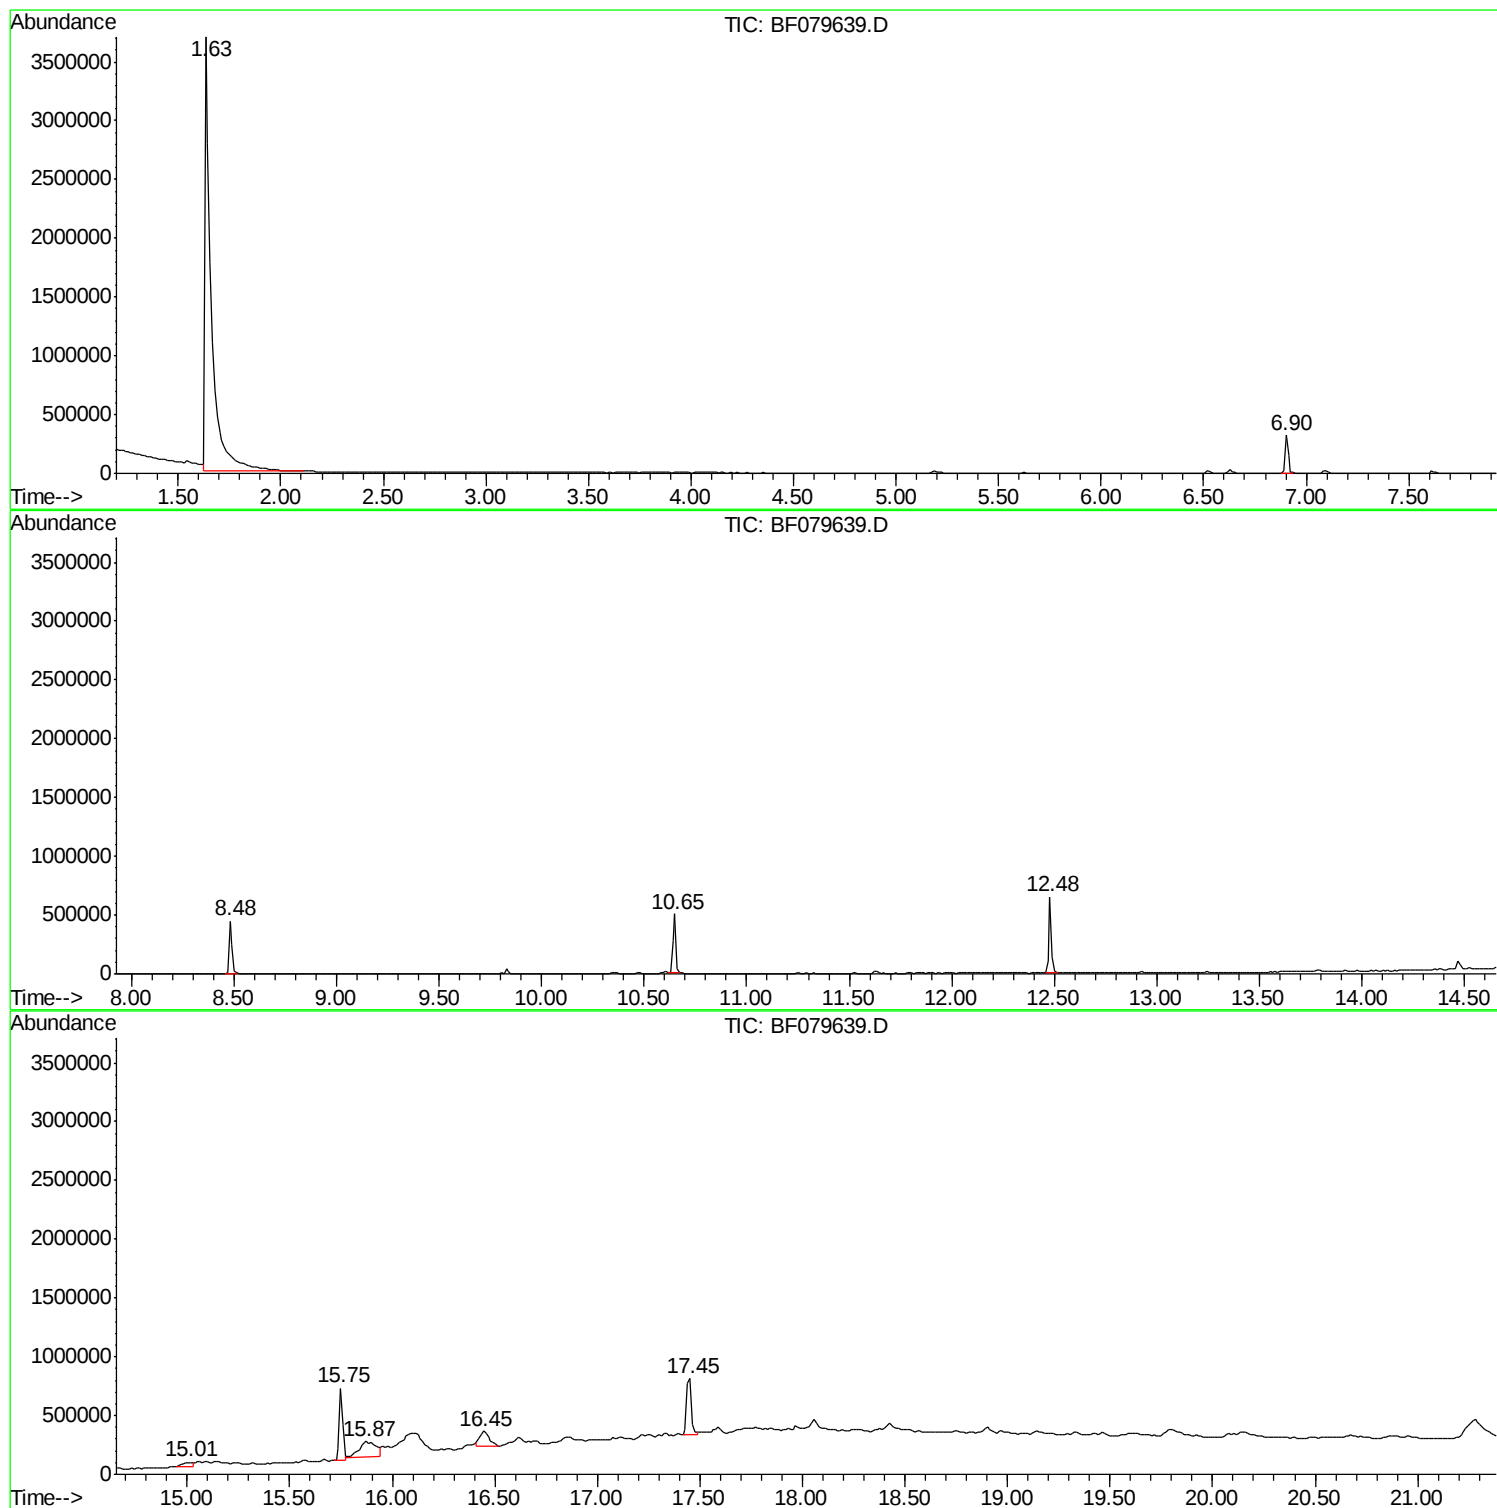

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF053115\
Data File : BF079639.D
Acq On : 31 May 2015 18:10
Operator : TP/IZ
Sample : G2416-26 5X
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
RAMP440NB-TP5.4(6)










Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF052615.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 3,4:9,10-Dibenzopyrene Concentration Rank 4

R.T.	EstConc	Area	Relative to ISTD	R.T.
15.01	2.73 ng	97625	Chrysene-d12	15.75

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	3,4:9,10-Dibenzopyrene	302	C24H14	000189-55-9	60
2		1,2:4,5-Dibenzopyrene	302	C24H14	000192-65-4	55
3		Zirconium dichloride, bis[(eta.5...	302	C11H10Cl2Zr	1000163-91-7	53
4		8-Chloroo-4-(p-chloroanilino)-2-...	302	C16H12Cl2N2	092854-09-6	47
5		3,4:8,9-Dibenzopyrene	302	C24H14	000189-64-0	46

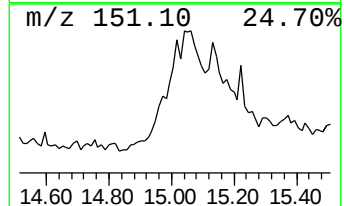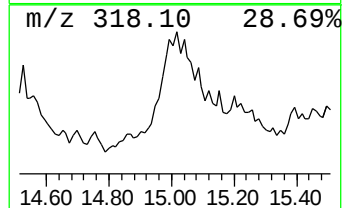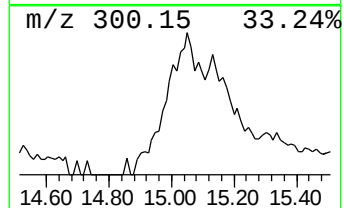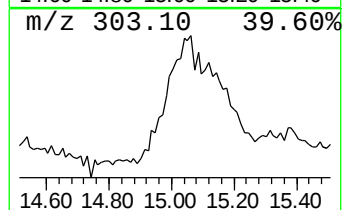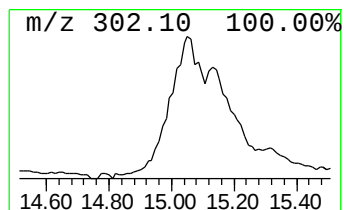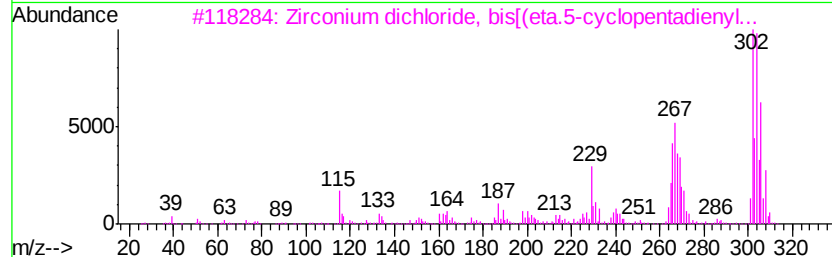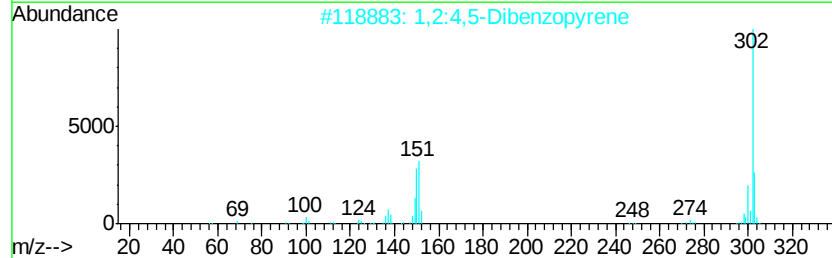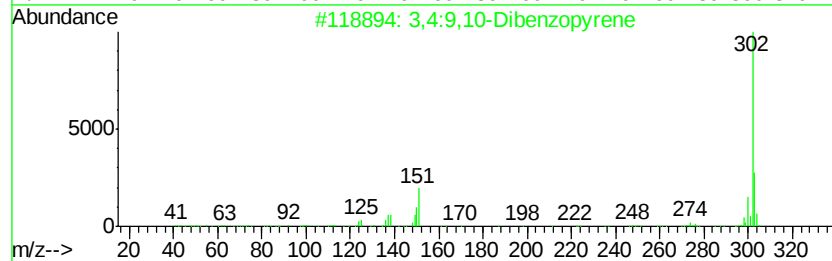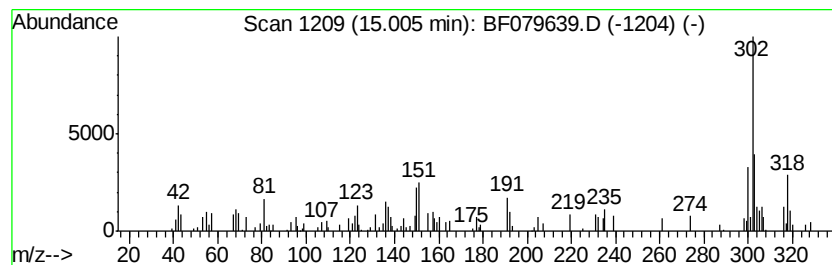

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF053115\
Data File : BF079639.D
Acq On : 31 May 2015 18:10
Operator : TP/IZ
Sample : G2416-26 5X
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
RAMP440NB-TP5.4(6)

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF052615.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---			
					#	RT	Resp	Conc
3,4:9,10-Dibenzop...	15.01	2.7	ng	97625	5	15.75	715077	20.0