
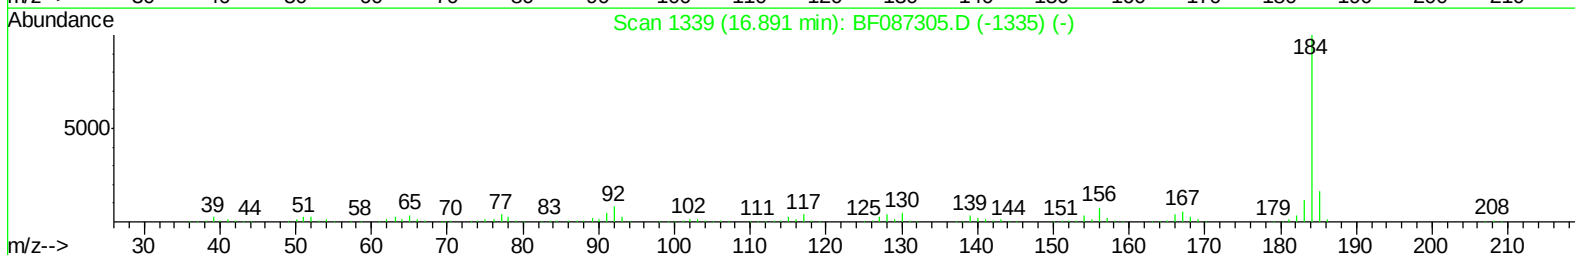
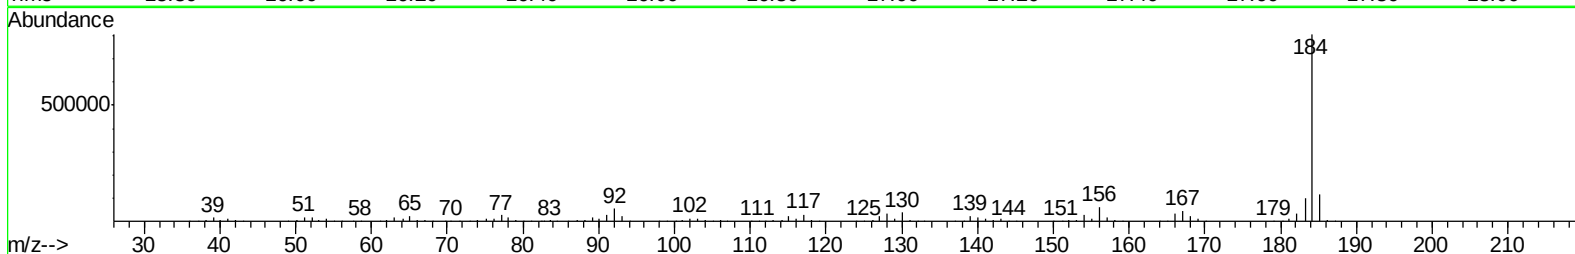


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF053116\
Data File : BF087601.D
Acq On : 1 Jun 2016 2:36
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 01 05:38:44 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF052316.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 01 03:17:16 2016
Response via : Initial Calibration

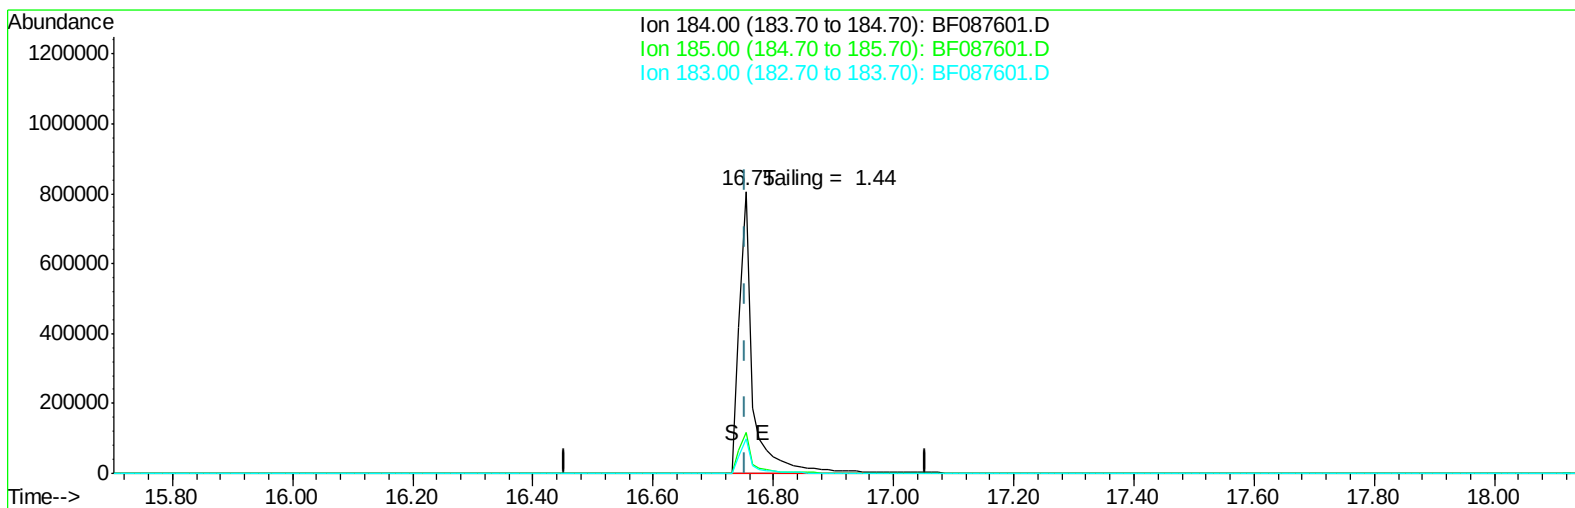

TIC: BF087601.D

(76) Benzidine




16.754min (-0.000) 51760.10ng

response 1277208

Ion	Exp%	Act%
184.00	100	100
185.00	17.00	14.77
183.00	12.20	12.08
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF053116\
Data File : BF087601.D
Acq On : 1 Jun 2016 2:36
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 01 05:38:44 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF052316.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 01 03:17:16 2016
Response via : Initial Calibration

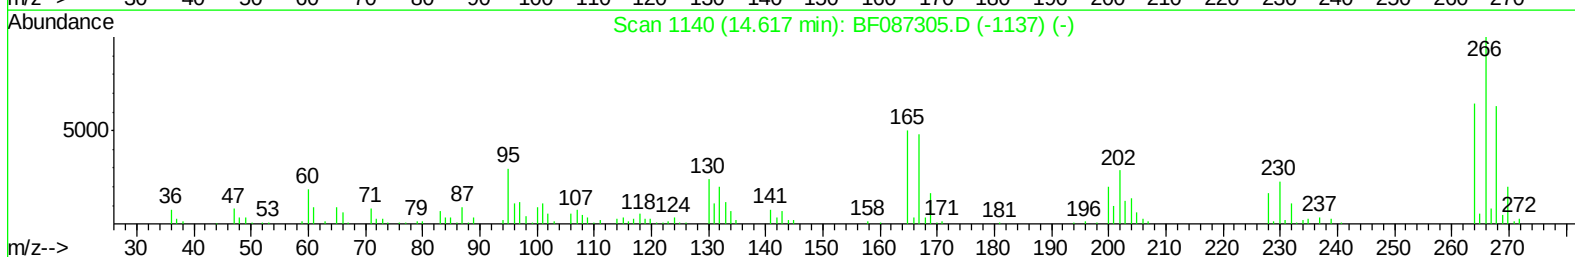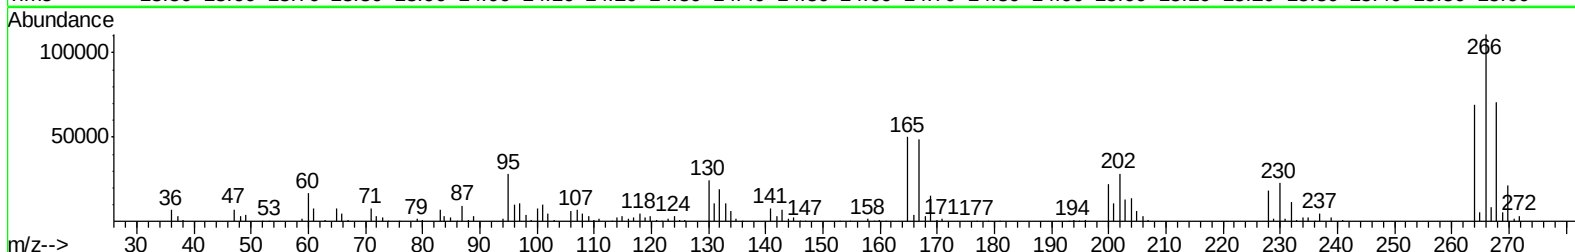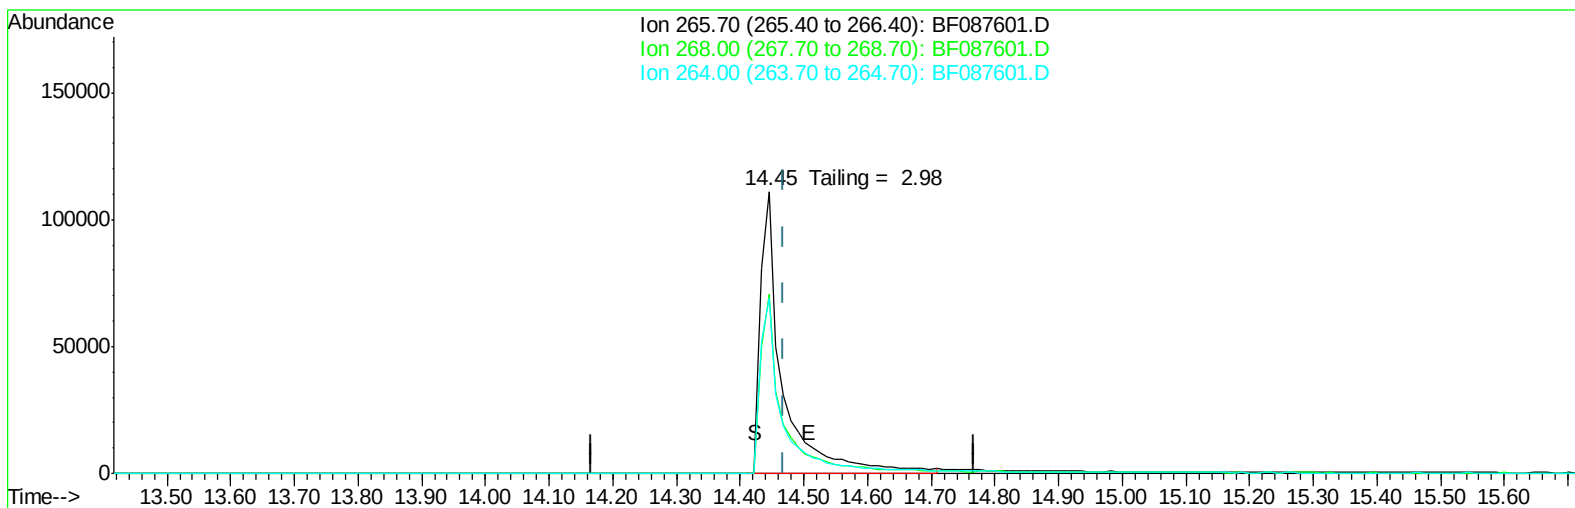

TIC: BF087601.D

(69) Pentachlorophenol (C)

14.445min (-0.023) 0.00ng

response 270792

Ion	Exp%	Act%
265.70	100	100
268.00	64.40	63.53
264.00	66.10	62.43
0.00	0.00	0.00