


Data Path : Z:\HPCHEM1\BNA F\DATA\BF053116\
 Data File : BF087583.D
 Acq On : 31 May 2016 14:54
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF052316.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed May 25 16:26:52 2016

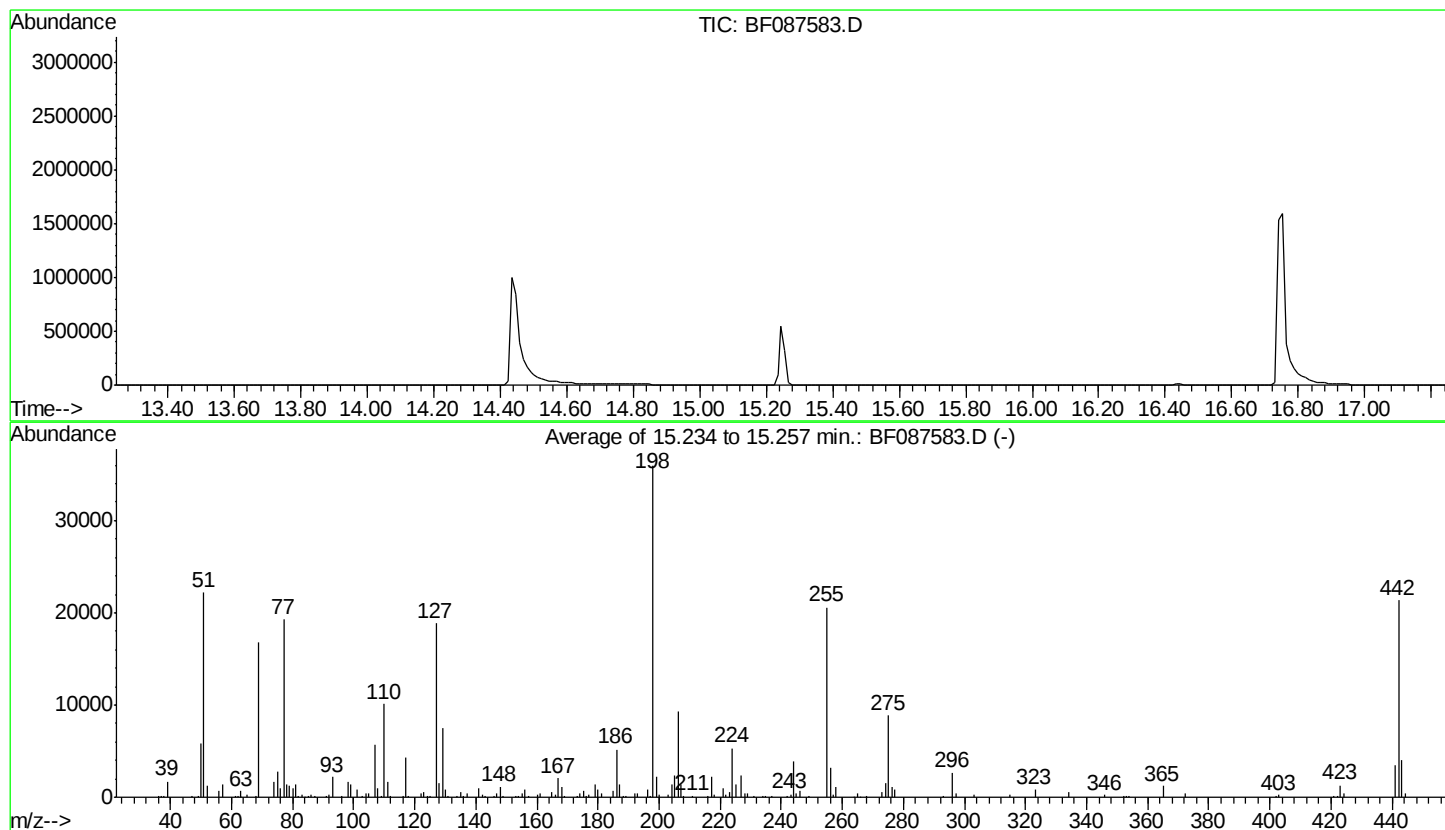

AutoFind: Scans 1194, 1195, 1196; Background Corrected with Scan 1191

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	61.7	22167	PASS
68	69	0.00	2	1.2	197	PASS
69	198	0.00	100	46.7	16791	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	52.5	18871	PASS
197	198	0.00	2	0.3	103	PASS
198	198	100	100	100.0	35954	PASS
199	198	5	9	6.3	2272	PASS
275	198	10	60	24.6	8832	PASS
365	198	1	100	3.4	1231	PASS
441	442	0.01	24	16.5	3511	PASS
442	198	50	100	59.3	21311	PASS
443	442	15	24	18.6	3973	PASS