

Data Path : Z:\HPCHEM1\BNA F\DATA\BF053117\
 Data File : BF095579.D
 Acq On : 31 May 2017 23:21
 Operator : SJ/MA
 Sample : I3341-05
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :

Quant Time: Jun 01 01:37:42 2017
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF050217.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri May 26 16:50:16 2017
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.79	152	270367	20.00	ng	0.05
21) Naphthalene-d8	9.58	136	359787	20.00	ng	-0.18
38) Acenaphthene-d10	12.41	164	170345	20.00	ng	-0.19
63) Phenanthrene-d10	14.81	188	245095	20.00	ng	-0.19
75) Chrysene-d12	18.51	240	206130	20.00	ng	-0.17
86) Perylene-d12	20.18	264	173807	20.00	ng	-0.18
System Monitoring Compounds						
5) 2-Fluorophenol	5.47	112	607898	37.49	ng	-0.24
7) Phenol-d6	7.11	99	750541	38.57	ng	-0.19
23) Nitrobenzene-d5	8.47	82	427049	74.85	ng	-0.19
41) 2,4,6-Tribromophenol	13.71	330	137024	98.22	ng	-0.19
44) 2-Fluorobiphenyl	11.36	172	746458	63.07	ng	-0.18
78) Terphenyl-d14	17.15	244	357498	38.20	ng	-0.17
Target Compounds						Qvalue
19) n-Nitroso-di-n-propylamine	8.47	70	51290	3.90	ng	# 76
49) Dimethylphthalate	12.05	163	197062	14.09	ng	99
70) Phenanthrene	14.85	178	38707	2.75	ng	97
71) Anthracene	14.85	178	38707	2.69	ng	98
74) Fluoranthene	16.61	202	75862	5.25	ng	97
77) Pyrene	16.92	202	63747	4.14	ng	96
80) Benzo(a)anthracene	18.49	228	36894	3.08	ng	95
82) Chrysene	18.54	228	35063	3.02	ng	100
87) Benzo(b)fluoranthene	19.78	252	63069	5.87	ng	# 96
88) Benzo(k)fluoranthene	19.78	252	63069	6.09	ng	99
89) Benzo(a)pyrene	20.13	252	32486	3.28	ng	# 91
91) Benzo(a,h,i)perylene	21.81	276	16105	2.01	ng	97

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA F\DATA\BF053117\
Data File : BF095579.D
Acq On : 31 May 2017 23:21
Operator : SJ/MA
Sample : I3341-05
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :

Quant Time: Jun 01 01:37:42 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF050217.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri May 26 16:50:16 2017
Response via : Initial Calibration

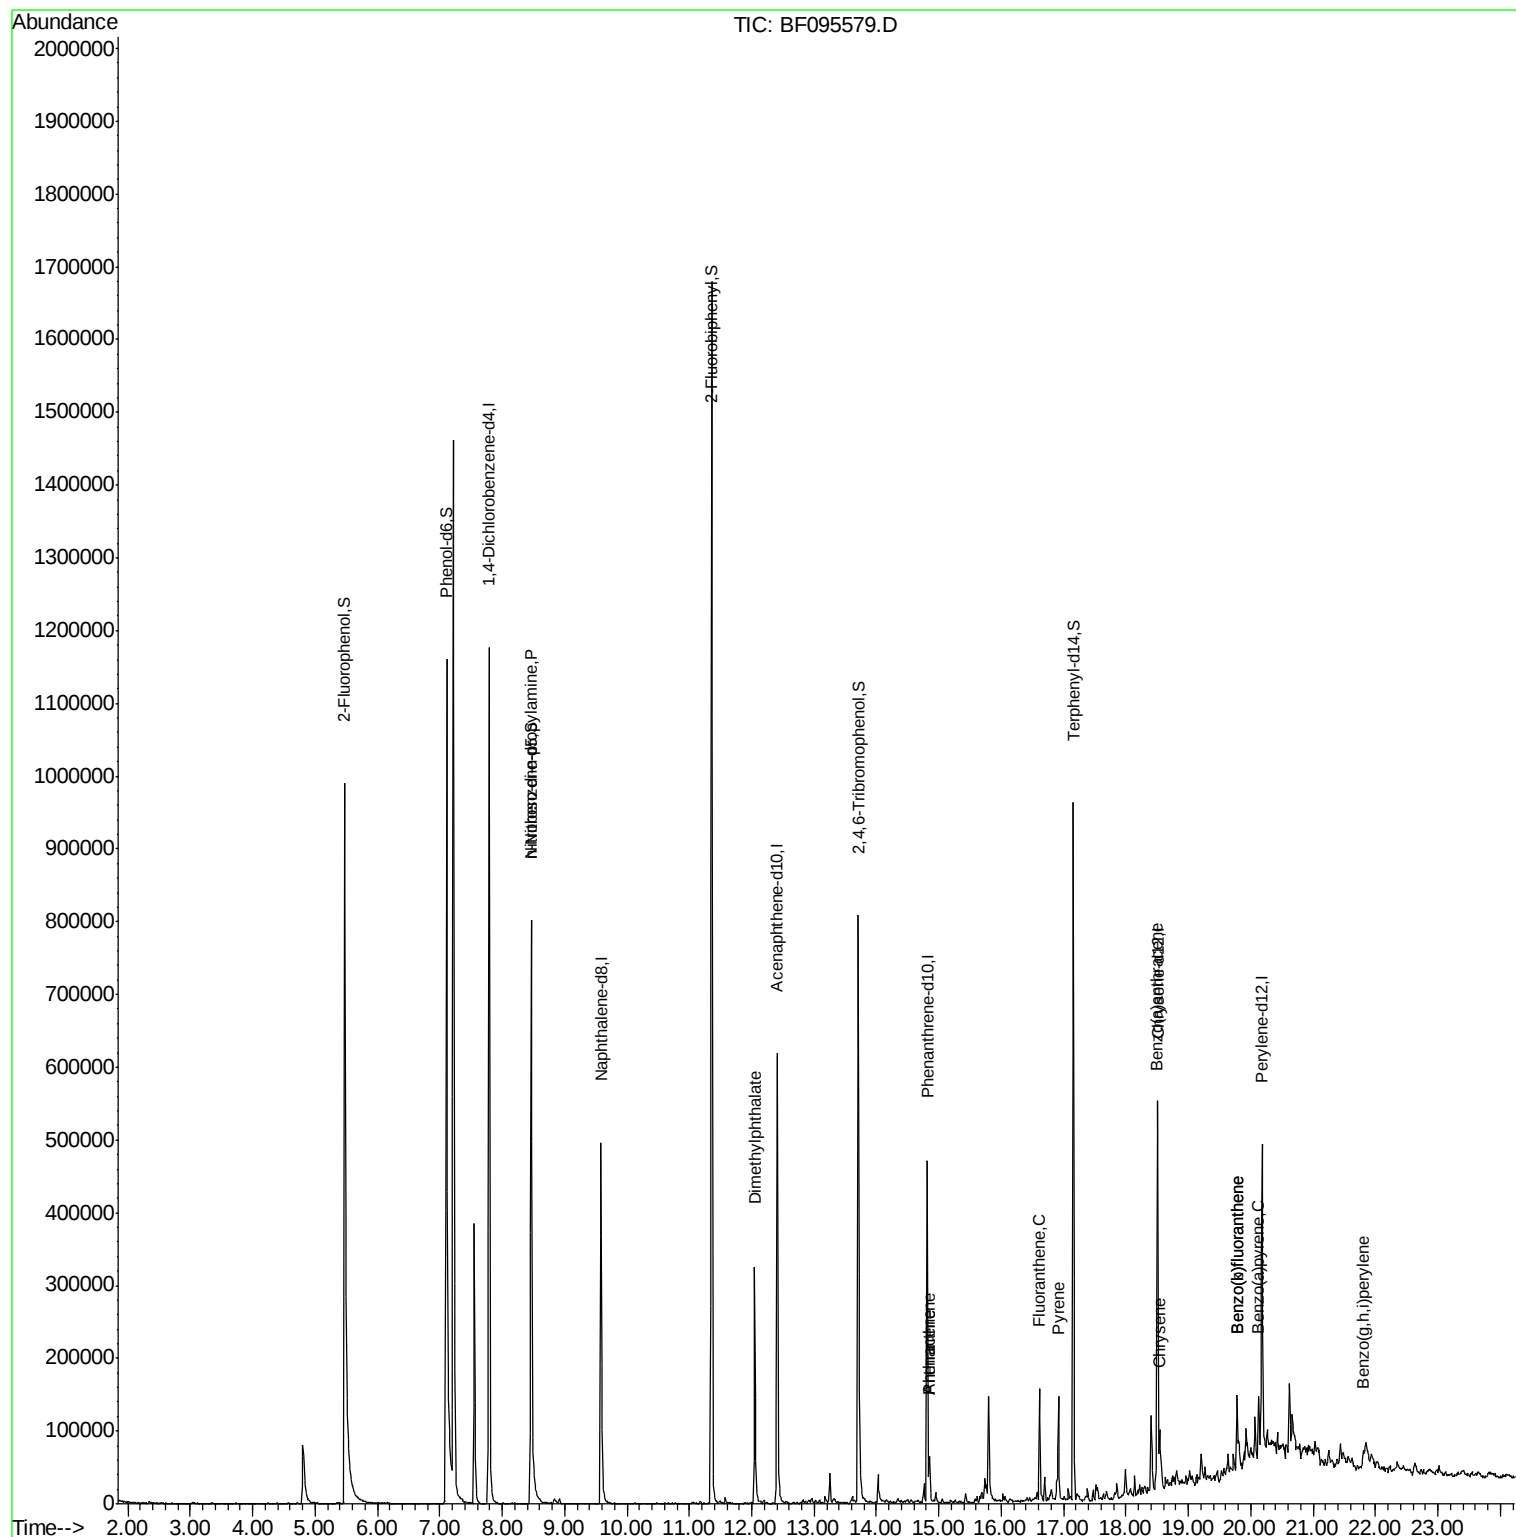



#1

1,4-Dichlorobenzene-d4

Concen: 20.00 ng

RT: 7.79 min Scan# 1012

Delta R.T. 0.05 min

Lab File: BF095579.D

Acq: 31 May 2017 23:21

Instrument :

BNA_F

ClientSampleId :


Tot Ion:152 Resp: 270367

Ion Ratio Lower Upper

152 100

150 154.9 126.2 189.2




115 66.0 52.2 78.2

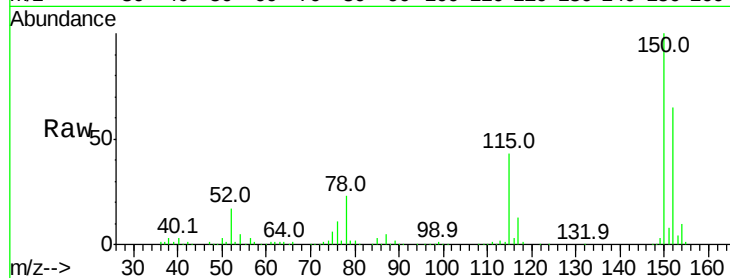

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

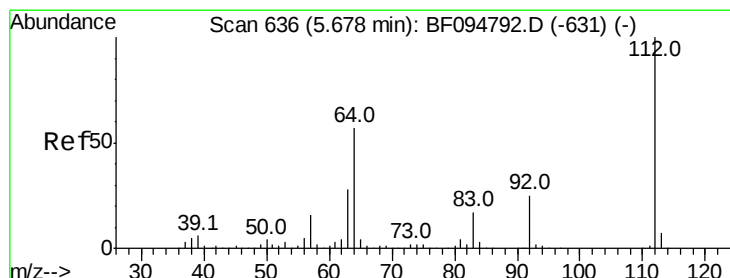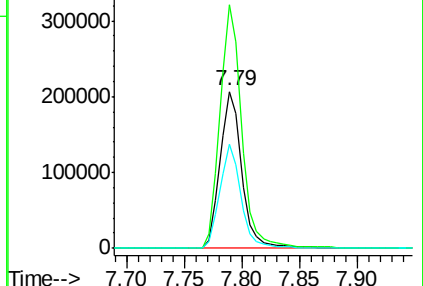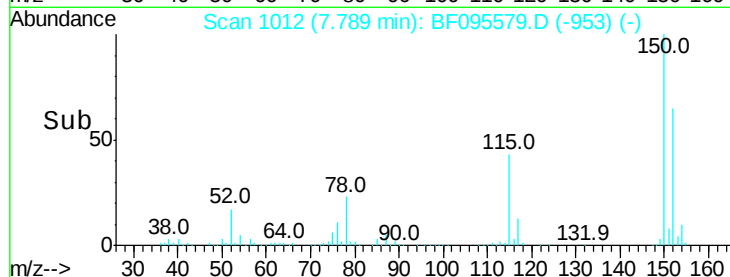

#5

2-Fluorophenol

Concen: 37.49 ng

RT: 5.47 min Scan# 618

Delta R.T. -0.24 min

Lab File: BF095579.D

Acq: 31 May 2017 23:21


Tgt Ion:112 Resp: 607898

Ion Ratio Lower Upper

112 100

64 56.3 46.0 69.0



63 26.8 23.4 35.0

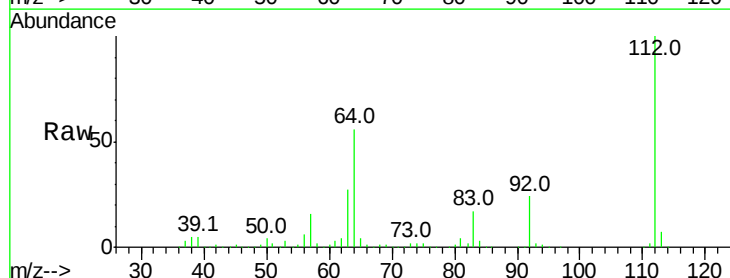

Abundance Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BF0

Ion 63.00 (62.70 to 63.70): BF0

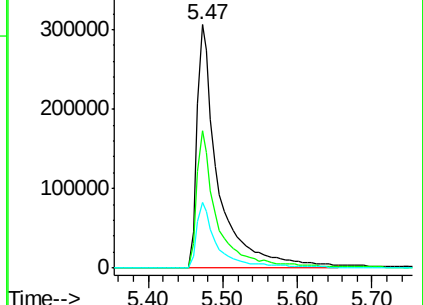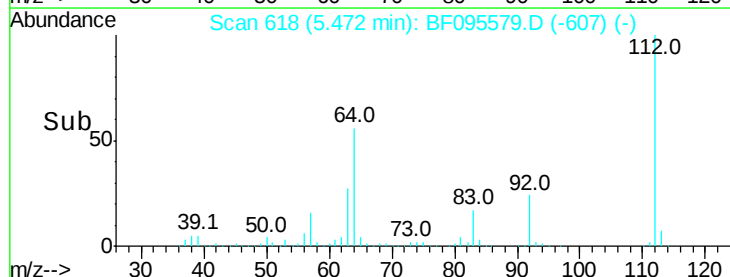



#7

Phenol-d6

Concen: 38.57 ng

RT: 7.11 min Scan# 896

Delta R.T. -0.19 min

Lab File: BF095579.D

Acq: 31 May 2017 23:21

Instrument :

BNA_F

ClientSampleId :


Tot Ion: 99 Resp: 750541

Ion Ratio Lower Upper

99 100

42 15.7 13.5 20.3




71 31.4 24.5 36.7

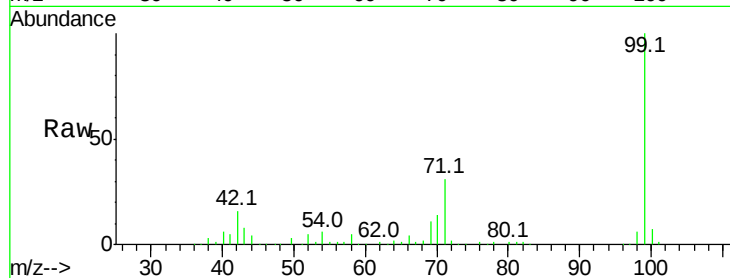

Abundance Ion 99.00 (98.70 to 99.70): BF0

Ion 42.00 (41.70 to 42.70): BF0

Ion 71.00 (70.70 to 71.70): BF0

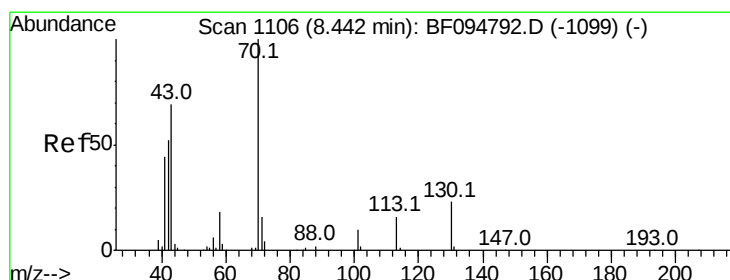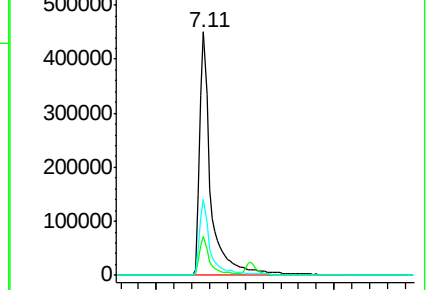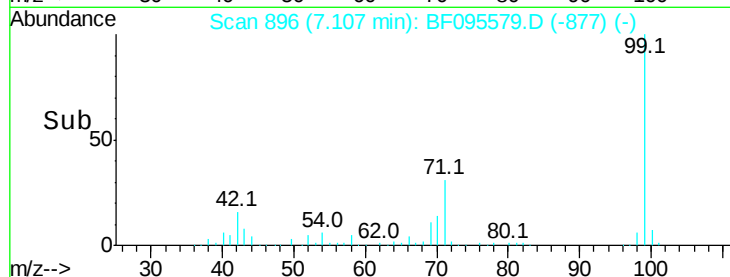

#19

n-Nitroso-di-n-propylamine

Concen: 3.90 ng

RT: 8.47 min Scan# 1127

Delta R.T. 0.01 min

Lab File: BF095579.D

Acq: 31 May 2017 23:21

Tgt Ion: 70 Resp: 51290


Ion Ratio Lower Upper

70 100

42 44.4 47.2 70.8#

101 0.0 7.2 10.8#

130 2.2 15.9 23.9#


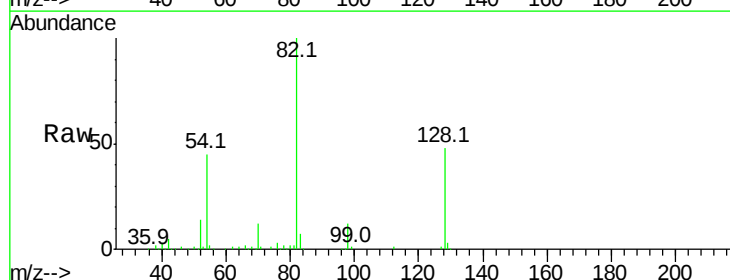


Abundance Ion 70.00 (69.70 to 70.70): BF0

Ion 42.00 (41.70 to 42.70): BF0

Ion 101.00 (100.70 to 101.70): BF0

Ion 130.00 (129.70 to 130.70): BF0

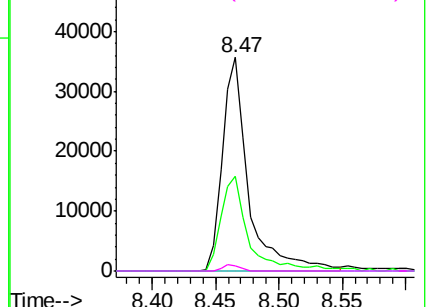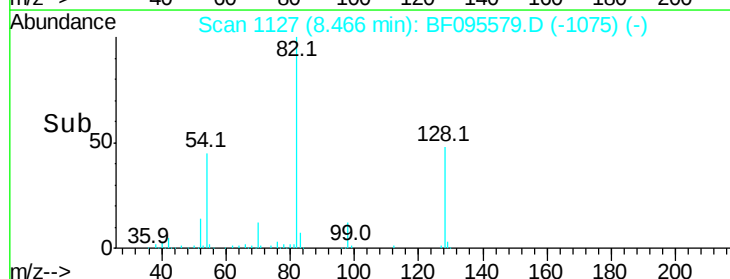







#21
Naphthalene-d8
Concen: 20.00 ng
RT: 9.58 min Scan# 1317
Delta R.T. -0.18 min
Lab File: BF095579.D
Acq: 31 May 2017 23:21

Instrument :
BNA_F
ClientSampleId :

Tot Ion:136	Resp:	359787
Ion Ratio	Lower	Upper
136 100		
137 10.5	8.5	12.7
54 6.5	4.9	7.3
68 5.8	4.1	6.1

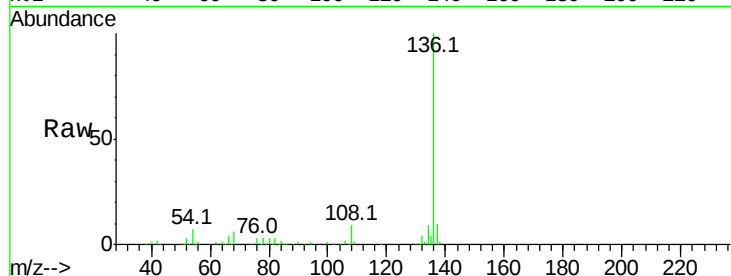


Abundance Ion 136.00 (135.70 to 136.70): E
Ion 137.00 (136.70 to 137.70): E
Ion 54.00 (53.70 to 54.70): BF0
Ion 68.00 (67.70 to 68.70): BF0

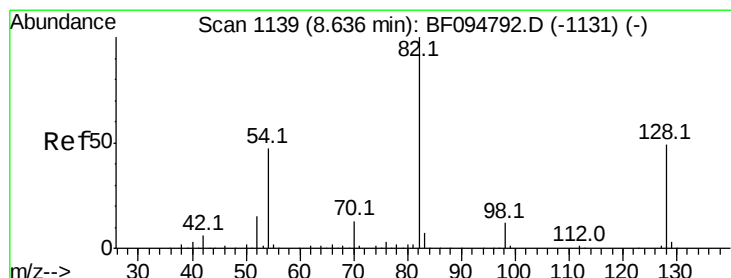
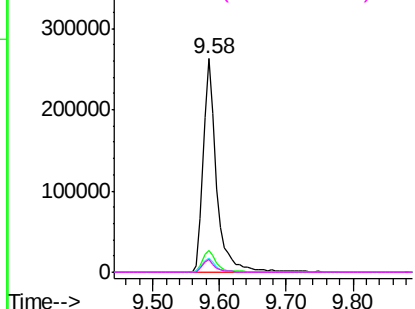


#23
Nitrobenzene-d5
Concen: 74.85 ng
RT: 8.47 min Scan# 1127
Delta R.T. -0.19 min
Lab File: BF095579.D
Acq: 31 May 2017 23:21

Tgt Ion: 82	Resp: 427049
Ion Ratio	Lower Upper
82 100	
128 47.6	34.0 51.0
54 45.4	42.2 63.2

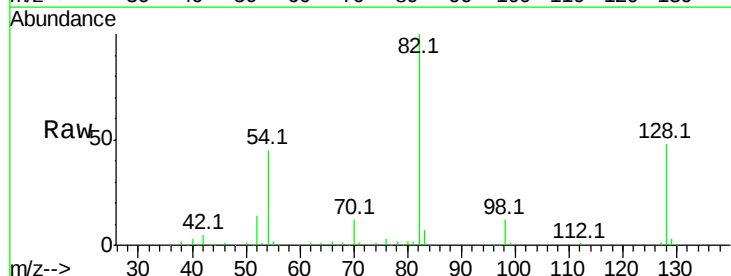

Abundance Ion 82.00 (81.70 to 82.70): BF0
Ion 128.00 (127.70 to 128.70): E
Ion 54.00 (53.70 to 54.70): BF0

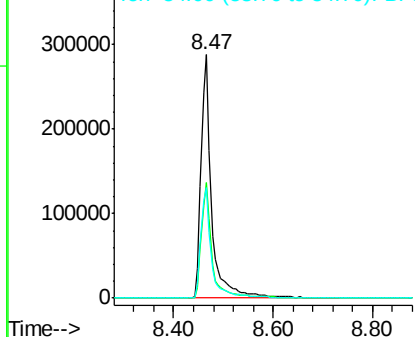



#38

Acenaphthene-d10

Concen: 20.00 ng

RT: 12.41 min Scan# 1797

Delta R.T. -0.19 min

Lab File: BF095579.D

Acq: 31 May 2017 23:21

Instrument :

BNA_F

ClientSampleId :


Tot Ion:164 Resp: 170345

Ion Ratio Lower Upper

164 100

162 105.4 82.6 123.8



160 44.9 36.2 54.2

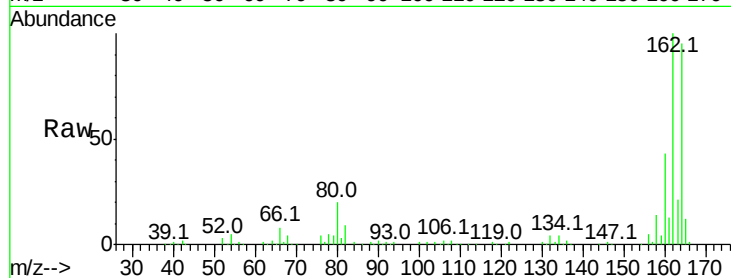

Abundance Ion 164.00 (163.70 to 164.70): E

Ion 162.00 (161.70 to 162.70): E

Ion 160.00 (159.70 to 160.70): E

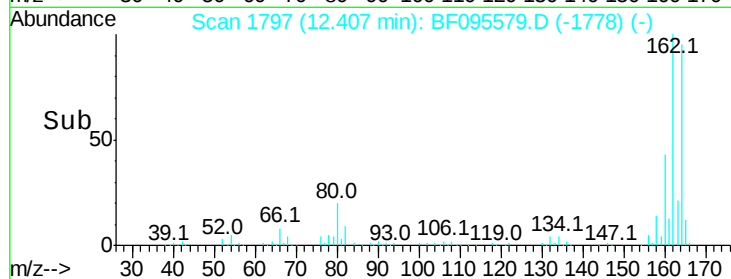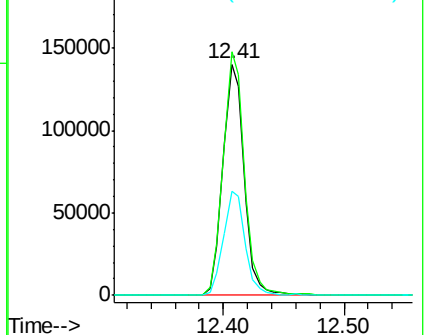

#41

2,4,6-Tribromophenol

Concen: 98.22 ng

RT: 13.71 min Scan# 2018

Delta R.T. -0.19 min

Lab File: BF095579.D

Acq: 31 May 2017 23:21


Tgt Ion:330 Resp: 137024

Ion Ratio Lower Upper

330 100

332 96.0 76.6 115.0



141 39.7 31.4 47.2

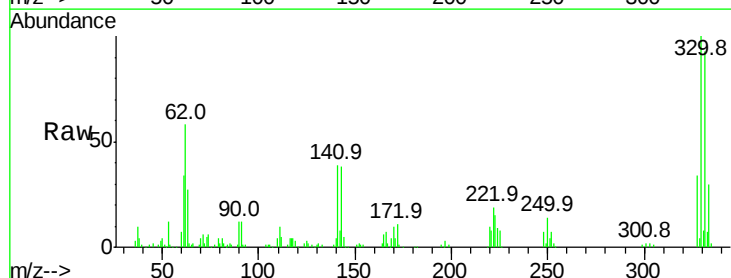

Abundance Ion 329.80 (329.50 to 330.50): E

Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E


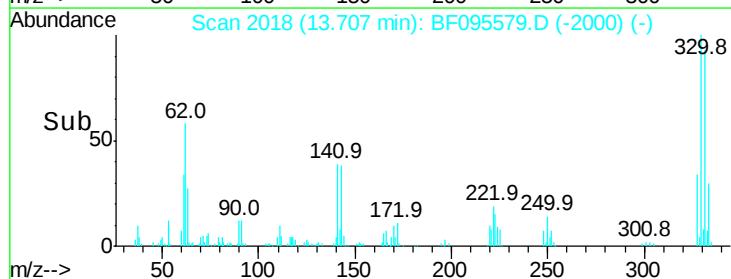
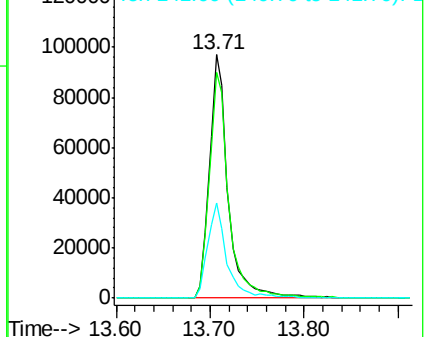




#44
 2-Fluorobiphenyl
 Concen: 63.07 ng
 RT: 11.36 min Scan# 1619
 Delta R.T. -0.18 min
 Lab File: BF095579.D
 Acq: 31 May 2017 23:21




Instrument :
 BNA_F
 ClientSampleId :

Tot Ion	Ratio	Lower	Upper
172	100		
171	35.8	29.6	44.4
170	23.2	19.8	29.8

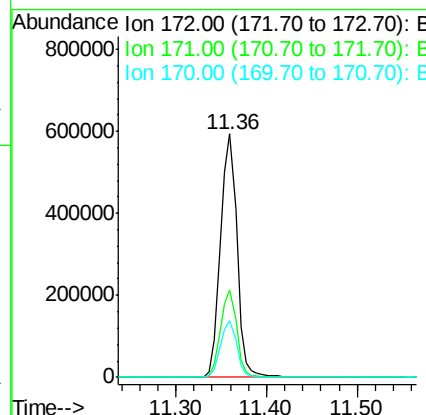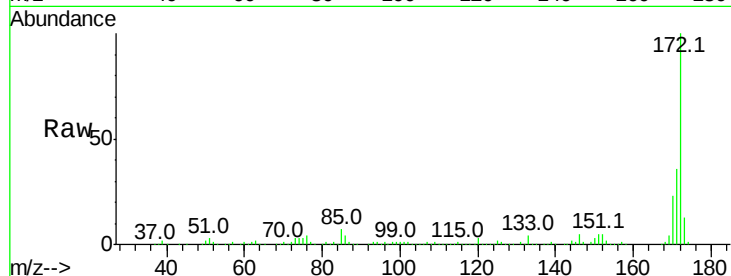

#49
 Dimethylphthalate
 Concen: 14.09 ng
 RT: 12.05 min Scan# 1736
 Delta R.T. -0.19 min
 Lab File: BF095579.D
 Acq: 31 May 2017 23:21

Tgt Ion	Ratio	Lower	Upper
163	100		
194	3.2	2.6	4.0
164	9.8	8.4	12.6



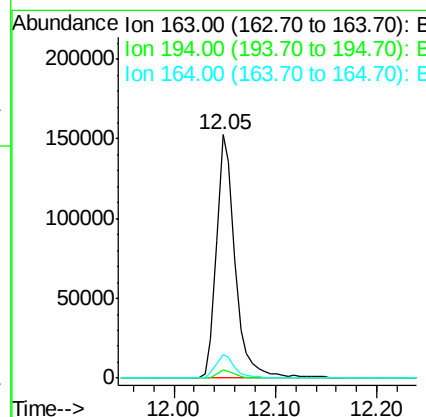
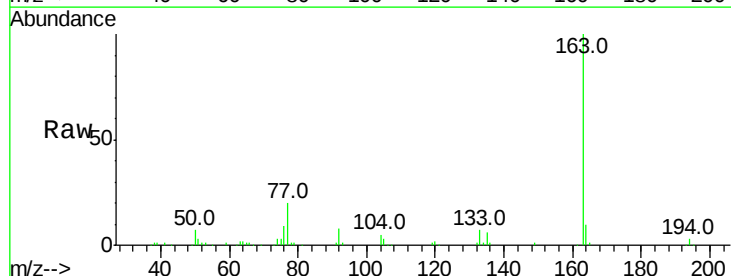




#63
 Phenanthrene-d10
 Concen: 20.00 ng
 RT: 14.81 min Scan# 2206
 Delta R.T. -0.19 min
 Lab File: BF095579.D
 Acq: 31 May 2017 23:21




Instrument :
 BNA_F
 ClientSampleId :


Tot Ion:188 Resp: 245095
 Ion Ratio Lower Upper
 188 100
 94 10.8 9.4 14.2
 80 11.3 10.2 15.2

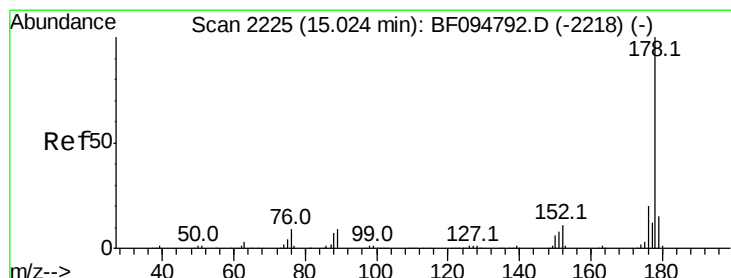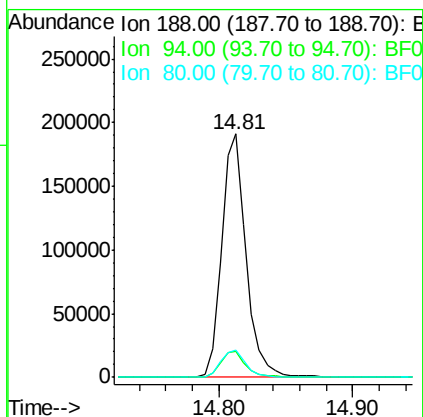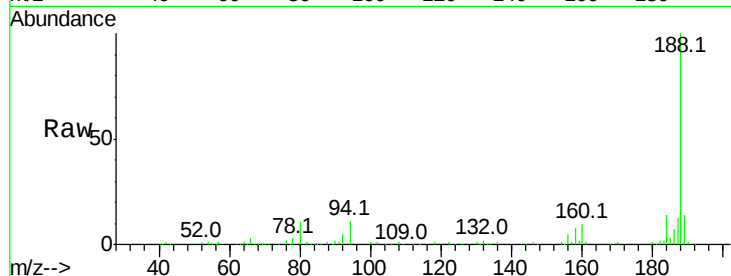

#70
 Phenanthrene
 Concen: 2.75 ng
 RT: 14.85 min Scan# 2212
 Delta R.T. -0.19 min
 Lab File: BF095579.D
 Acq: 31 May 2017 23:21

Tgt Ion:178 Resp: 38707
 Ion Ratio Lower Upper
 178 100
 176 18.6 16.2 24.4
 179 16.3 12.6 19.0



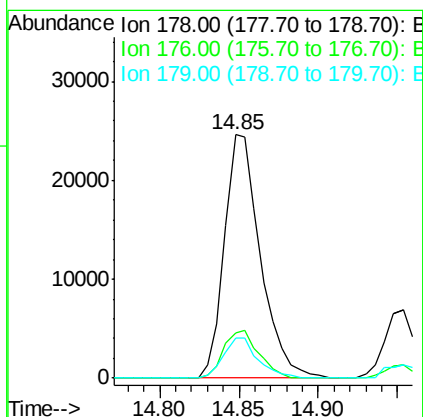
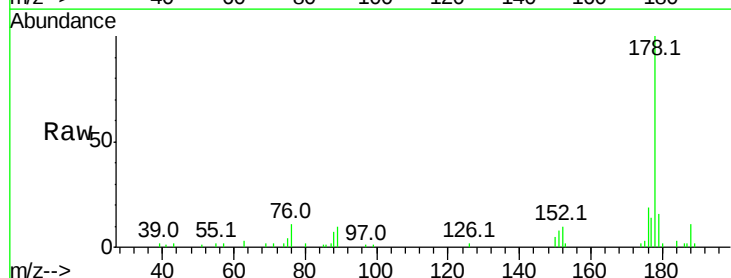


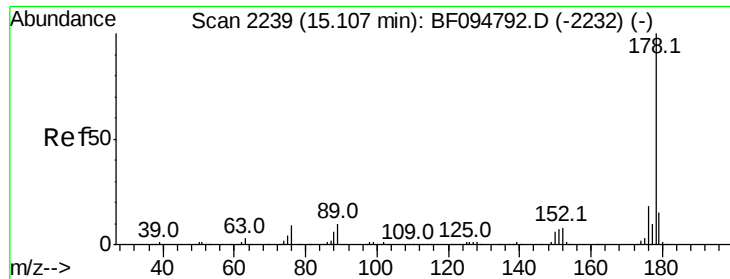

#71
 Anthracene
 Concen: 2.69 ng
 RT: 14.85 min Scan# 2212
 Delta R.T. -0.28 min
 Lab File: BF095579.D
 Acq: 31 May 2017 23:21




Instrument :
 BNA_F
 ClientSampleId :


Tot Ion:178 Resp: 38707
 Ion Ratio Lower Upper
 178 100
 176 18.6 15.8 23.8
 179 16.3 12.7 19.1

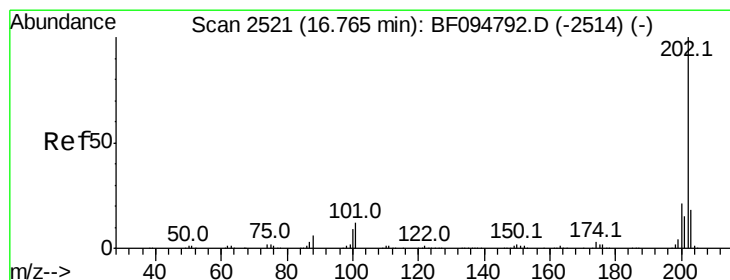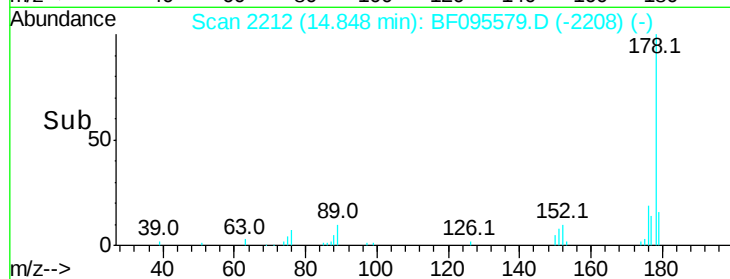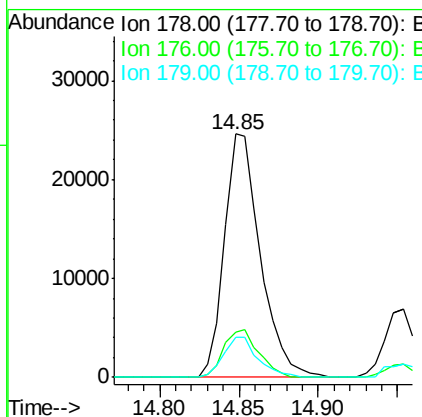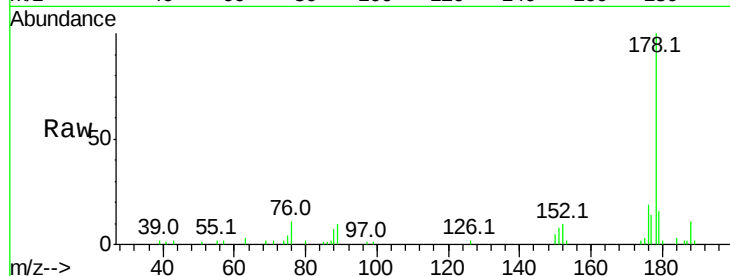

#74
 Fluoranthene
 Concen: 5.25 ng
 RT: 16.61 min Scan# 2512
 Delta R.T. -0.17 min
 Lab File: BF095579.D
 Acq: 31 May 2017 23:21

Tgt Ion:202 Resp: 75862
 Ion Ratio Lower Upper
 202 100
 101 14.1 0.0 33.2
 203 16.5 0.0 38.1

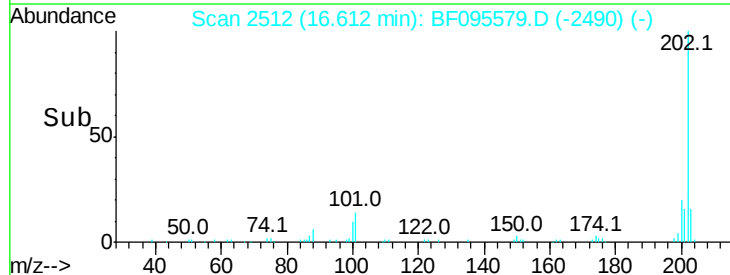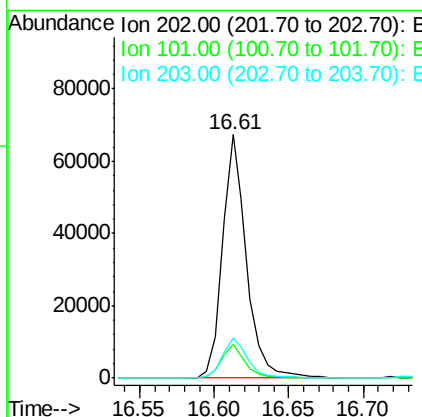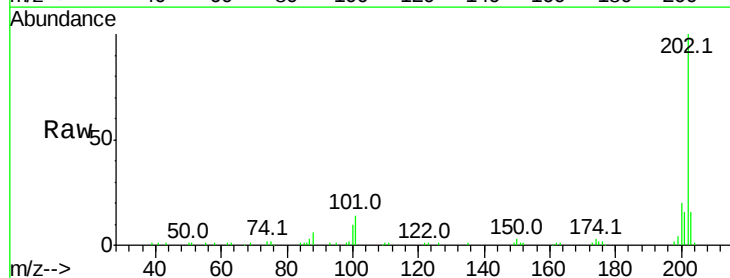

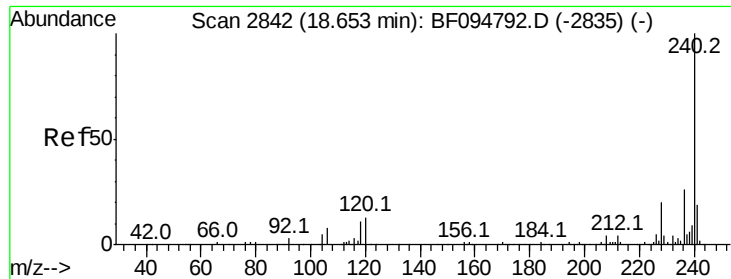

#75

Chrysene-d12

Concen: 20.00 ng

RT: 18.51 min Scan# 2834

Delta R.T. -0.17 min

Lab File: BF095579.D

Acq: 31 May 2017 23:21

Instrument :

BNA_F

ClientSampleId :


Tot Ion:240 Resp: 206130

Ion Ratio Lower Upper

240 100

120 14.3 5.8 8.8#




236 25.5 20.5 30.7

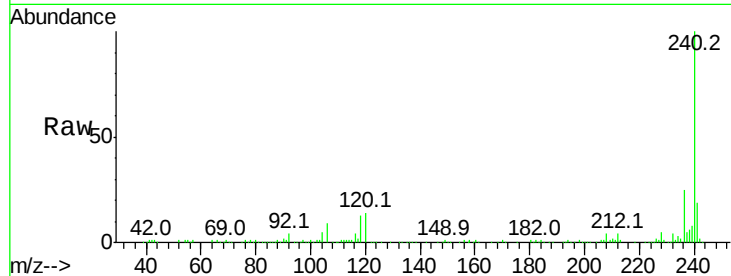

Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

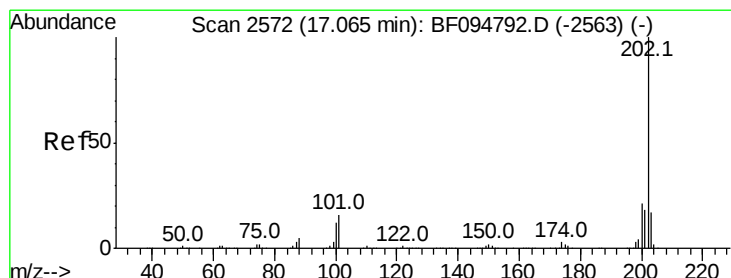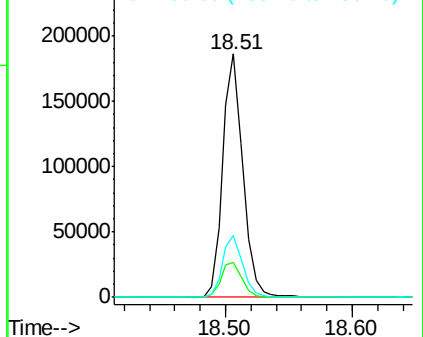

#77

Pyrene

Concen: 4.14 ng

RT: 16.92 min Scan# 2564

Delta R.T. -0.17 min

Lab File: BF095579.D

Acq: 31 May 2017 23:21


Tgt Ion:202 Resp: 63747

Ion Ratio Lower Upper

202 100

200 20.5 17.6 26.4



203 20.6 14.4 21.6

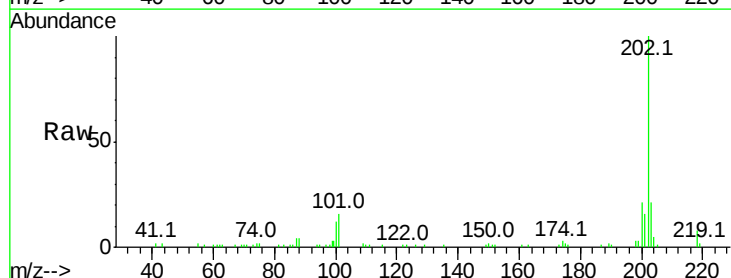

Abundance Ion 202.00 (201.70 to 202.70): E

Ion 200.00 (199.70 to 200.70): E

Ion 203.00 (202.70 to 203.70): E




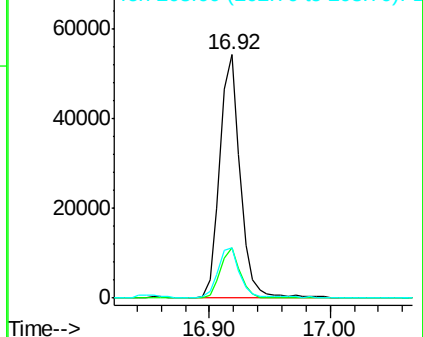




#78
 Terphenyl-d14
 Concen: 38.20 ng
 RT: 17.15 min Scan# 2604
 Delta R.T. -0.17 min
 Lab File: BF095579.D
 Acq: 31 May 2017 23:21




Instrument :
 BNA_F
 ClientSampleId :


Tot Ion:244 Resp: 357498
 Ion Ratio Lower Upper
 244 100
 212 6.8 6.0 9.0
 122 14.4 10.3 15.5

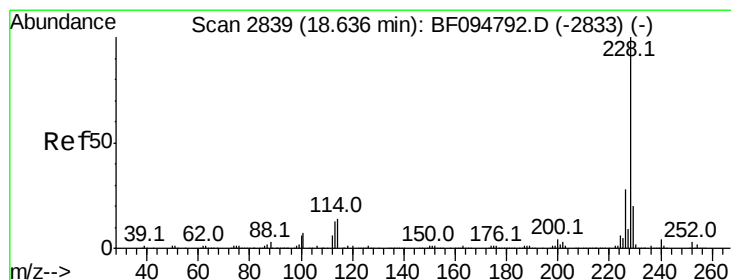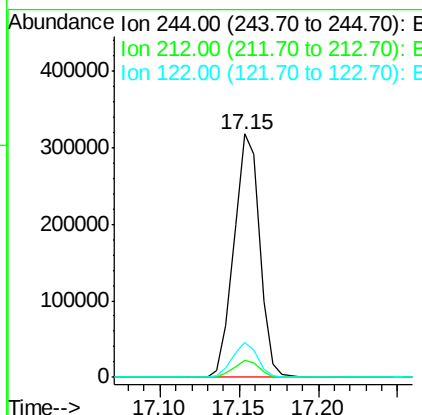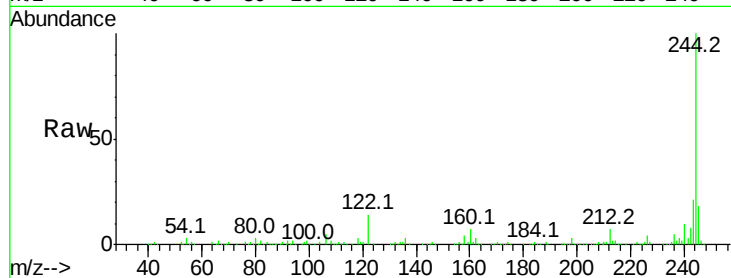

#80
 Benzo(a)anthracene
 Concen: 3.08 ng
 RT: 18.49 min Scan# 2832
 Delta R.T. -0.17 min
 Lab File: BF095579.D
 Acq: 31 May 2017 23:21

Tgt Ion:228 Resp: 36894
 Ion Ratio Lower Upper
 228 100
 226 29.7 22.6 33.8
 229 23.8 16.3 24.5


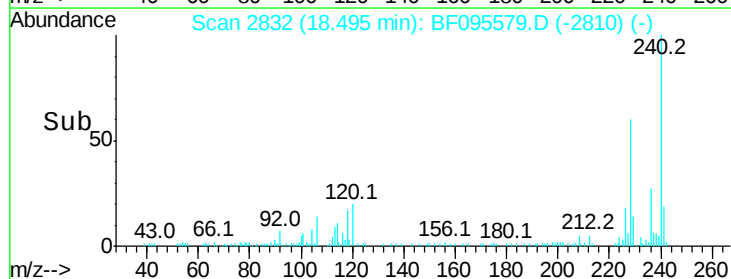
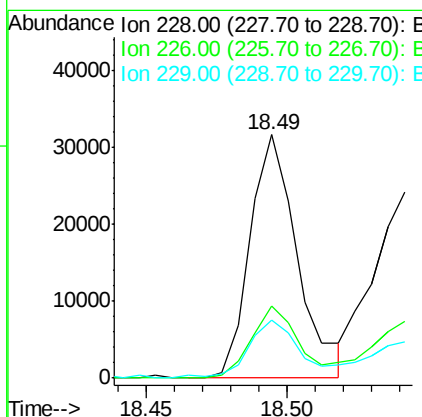
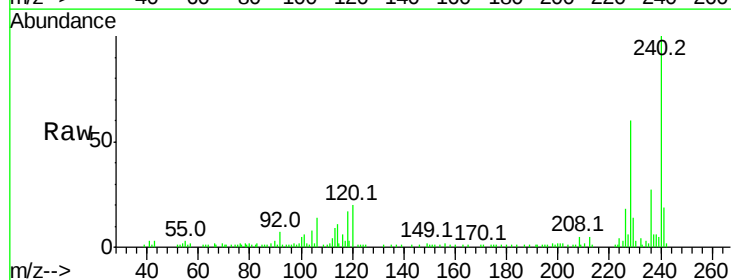


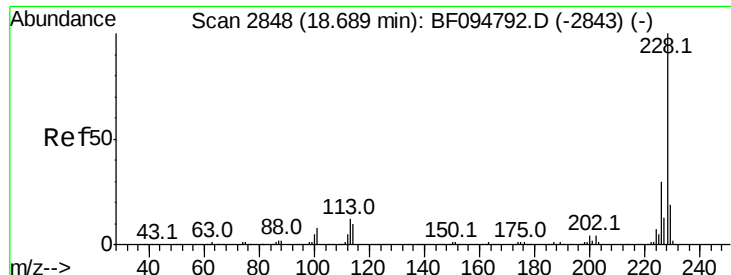

#82
Chrysene
Concen: 3.02 ng
RT: 18.54 min Scan# 2840
Delta R.T. -0.17 min
Lab File: BF095579.D
Acq: 31 May 2017 23:21




Instrument :
BNA_F
ClientSampleId :


Tot Ion:228 Resp: 35063
Ion Ratio Lower Upper
228 100
226 30.9 24.9 37.3
229 19.4 15.8 23.6

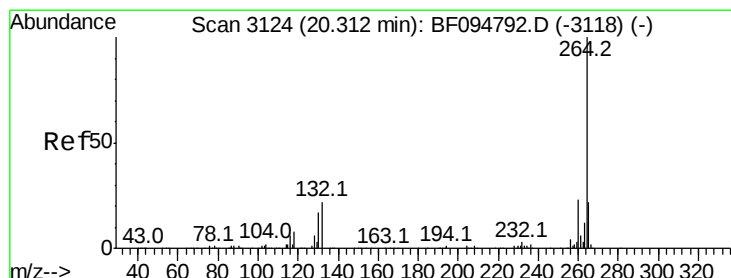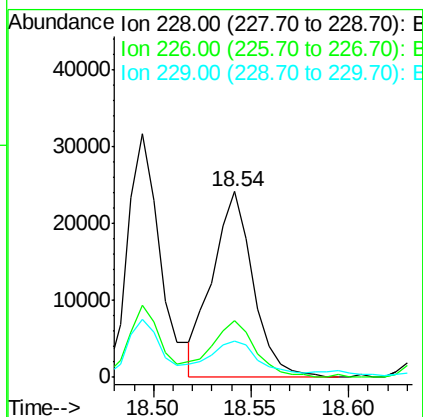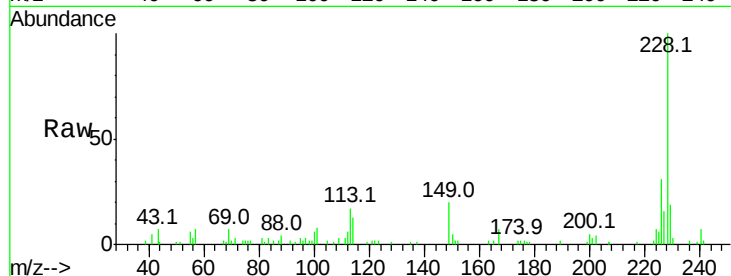

#86
Perylene-d12
Concen: 20.00 ng
RT: 20.18 min Scan# 3118
Delta R.T. -0.18 min
Lab File: BF095579.D
Acq: 31 May 2017 23:21

Tgt Ion:264 Resp: 173807
Ion Ratio Lower Upper
264 100
260 23.8 19.5 29.3
265 21.1 17.2 25.8

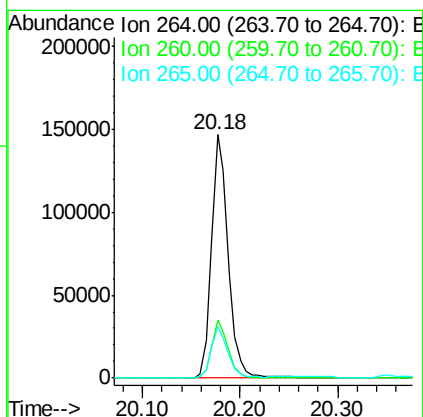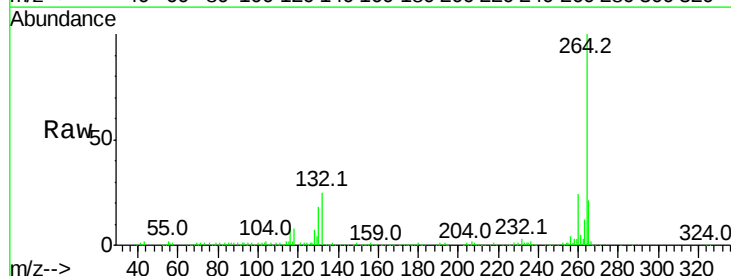

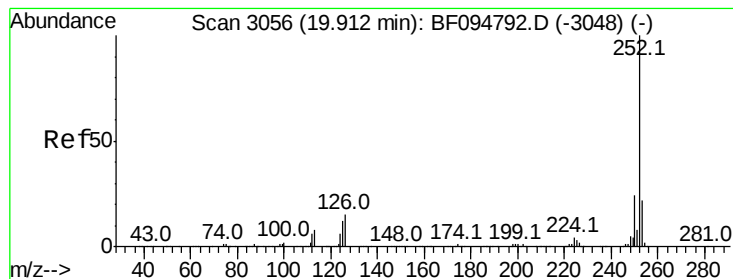

#87

Benzo(b)fluoranthene

Concen: 5.87 ng

RT: 19.78 min Scan# 3050

Delta R.T. -0.16 min

Lab File: BF095579.D

Acq: 31 May 2017 23:21

Instrument :

BNA_F

ClientSampleId :


Tot Ion:252 Resp: 63069

Ion Ratio Lower Upper

252 100

253 22.4 18.1 27.1




125 16.5 9.8 14.8#

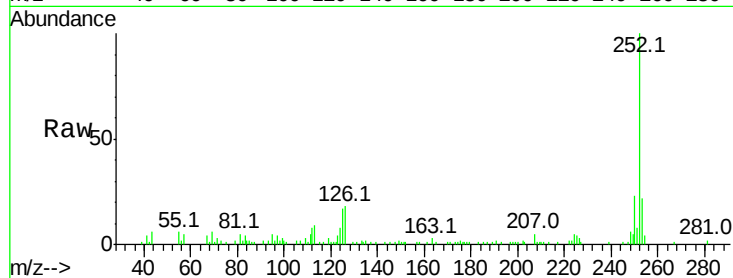

Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

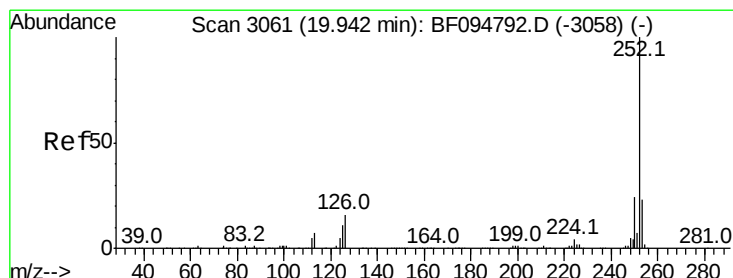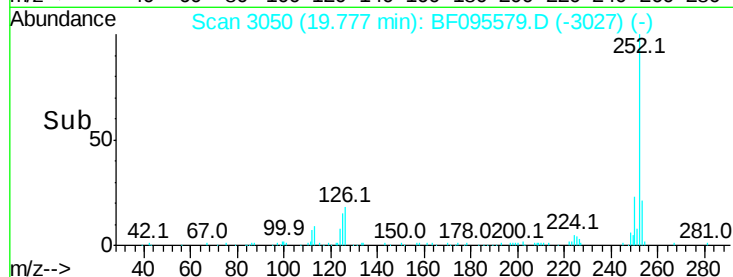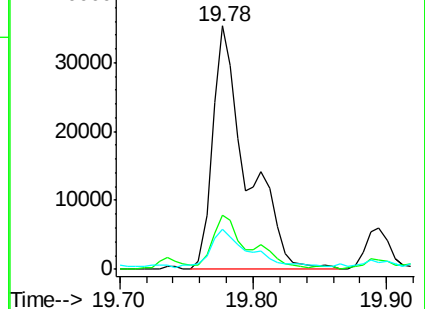

#88

Benzo(k)fluoranthene

Concen: 6.09 ng

RT: 19.78 min Scan# 3050

Delta R.T. -0.19 min

Lab File: BF095579.D

Acq: 31 May 2017 23:21


Tgt Ion:252 Resp: 63069

Ion Ratio Lower Upper

252 100

253 22.4 18.4 27.6



125 16.5 13.1 19.7

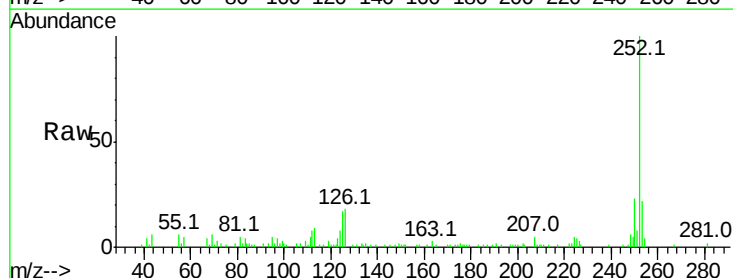


Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E



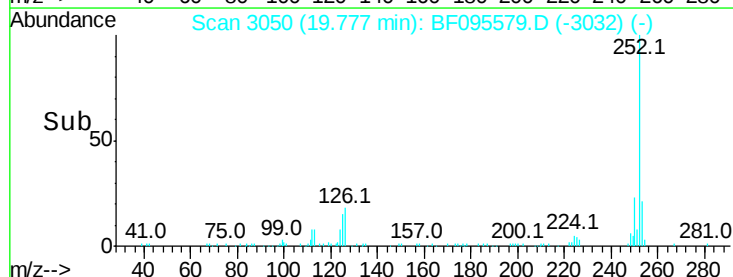
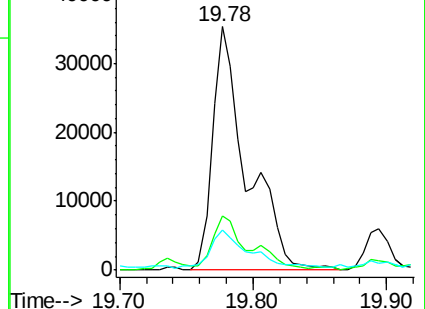


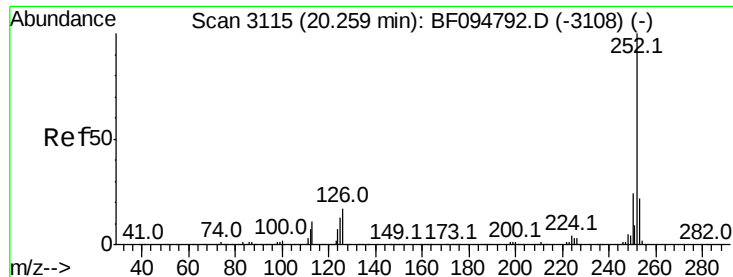

#89
Benzo(a)pyrene
Concen: 3.28 ng
RT: 20.13 min Scan# 3110
Delta R.T. -0.17 min
Lab File: BF095579.D
Acq: 31 May 2017 23:21

Instrument :
BNA_F
ClientSampleId :

Tot Ion:252 Resp: 32486
Ion Ratio Lower Upper
252 100
253 25.8 17.5 26.3
125 17.8 11.0 16.4#

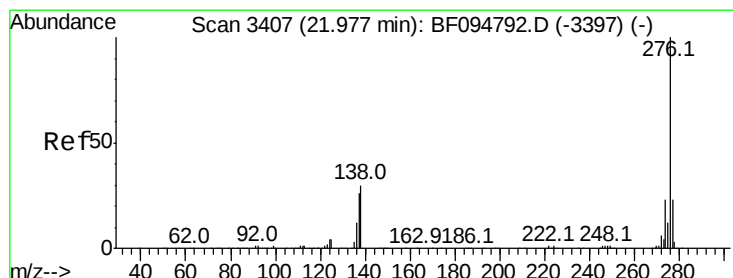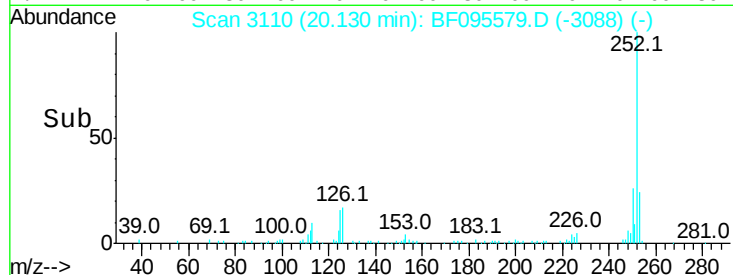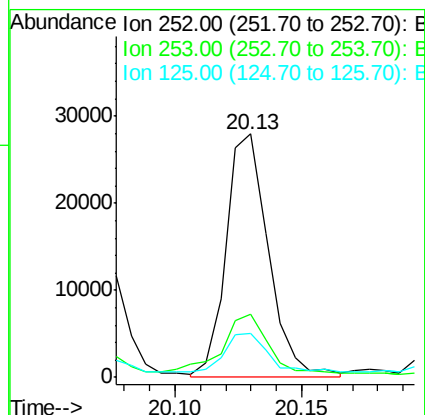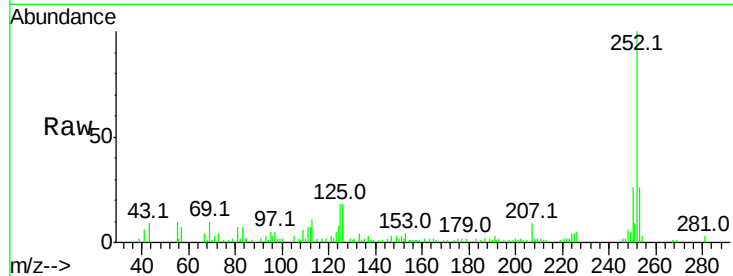

#91
Benzo(g,h,i)perylene
Concen: 2.01 ng
RT: 21.81 min Scan# 3395
Delta R.T. -0.26 min
Lab File: BF095579.D
Acq: 31 May 2017 23:21

Tgt Ion:276 Resp: 16105
Ion Ratio Lower Upper
276 100
277 25.4 18.6 28.0
138 32.5 25.4 38.0

