
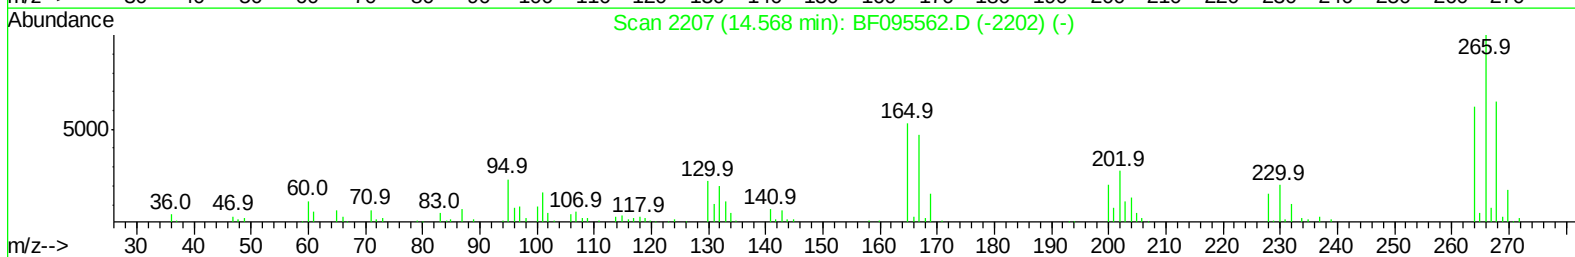
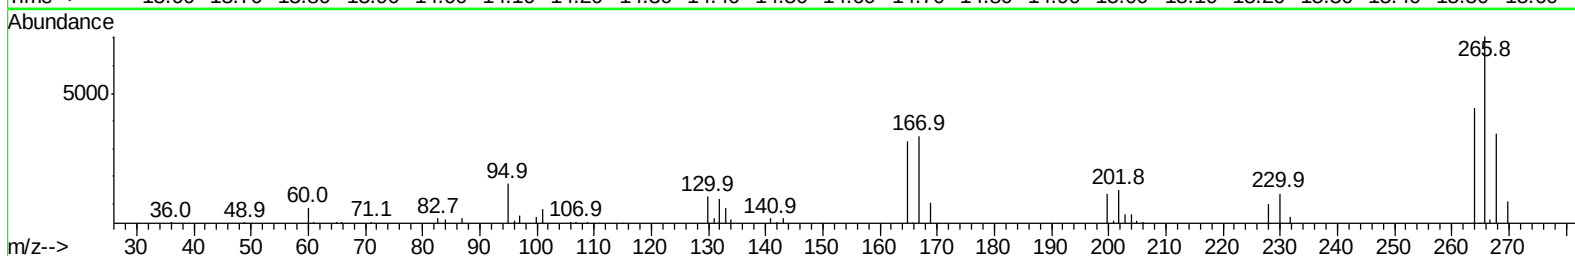


Data Path : Z:\HPCHEM1\BNA F\DATA\BF053117\
Data File : BF095584.D
Acq On : 1 Jun 2017 3:04
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 01 09:00:02 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF050217.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 01 03:03:02 2017
Response via : Initial Calibration

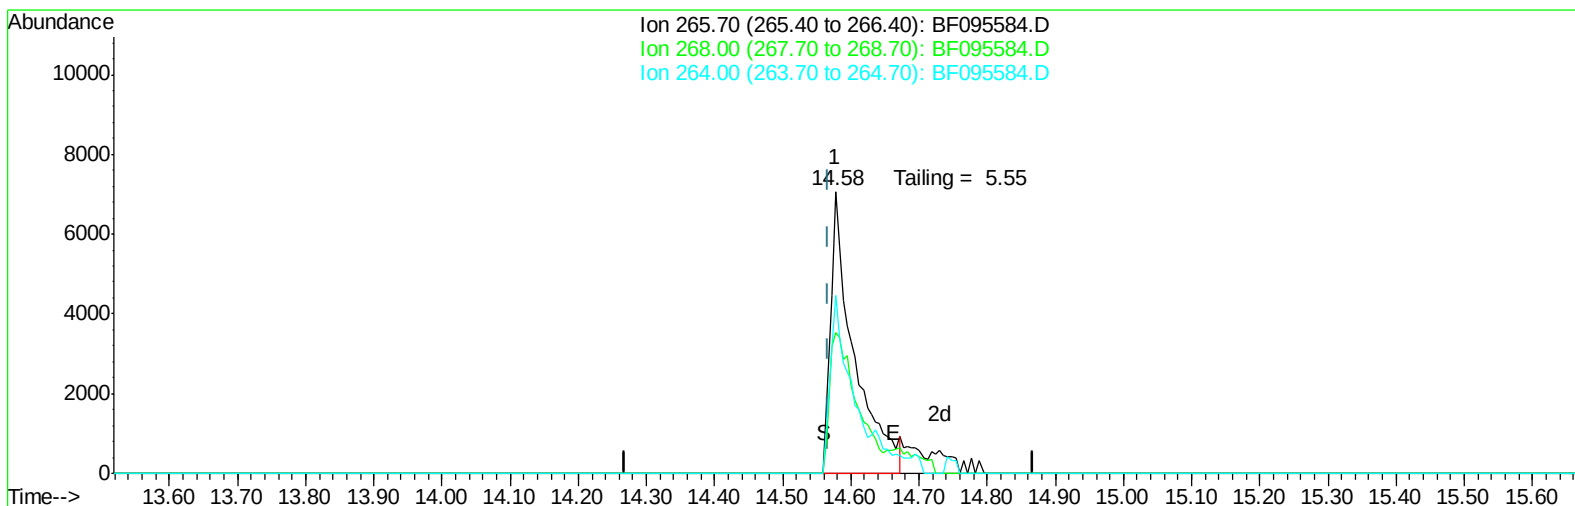

TIC: BF095584.D

(69) Pentachlorophenol (C)



14.577min (+0.009) 0.00ng

response 16511

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	50.10#
264.00	64.60	63.07
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\DATA\BF053117\
Data File : BF095584.D
Acq On : 1 Jun 2017 3:04
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 01 09:00:02 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF050217.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 01 03:03:02 2017
Response via : Initial Calibration

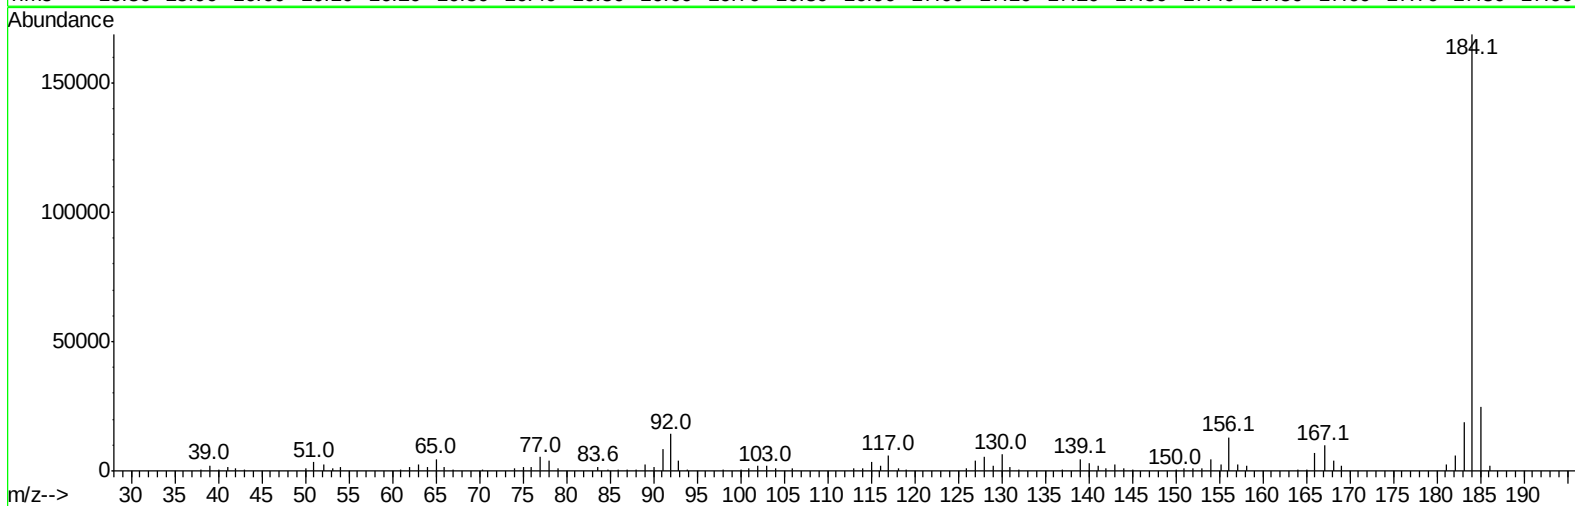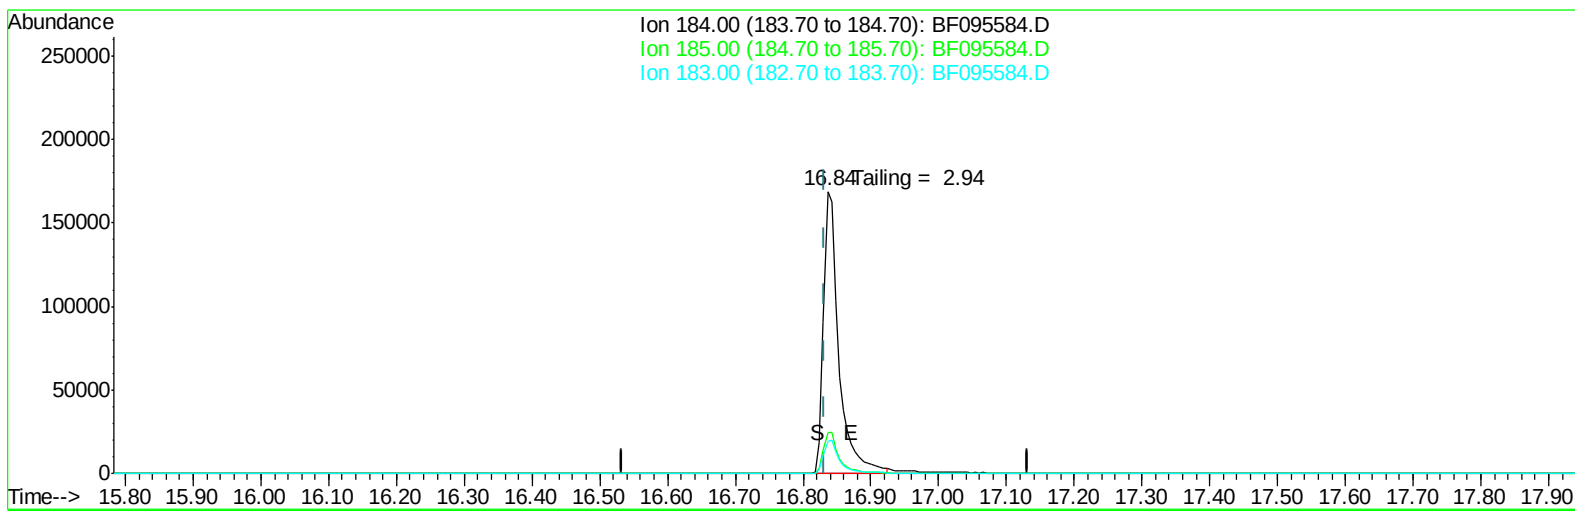

TIC: BF095584.D

(76) Benzidine

16.836min (+0.003) 0.00ng

response 262934

Ion	Exp%	Act%
184.00	100	100
185.00	19.40	14.69#
183.00	12.20	11.24
0.00	0.00	0.00