


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF053117\
 Data File : BF095561.D
 Acq On : 31 May 2017 13:36
 Operator : SJ/MA
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF050217.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Jun 01 03:03:02 2017

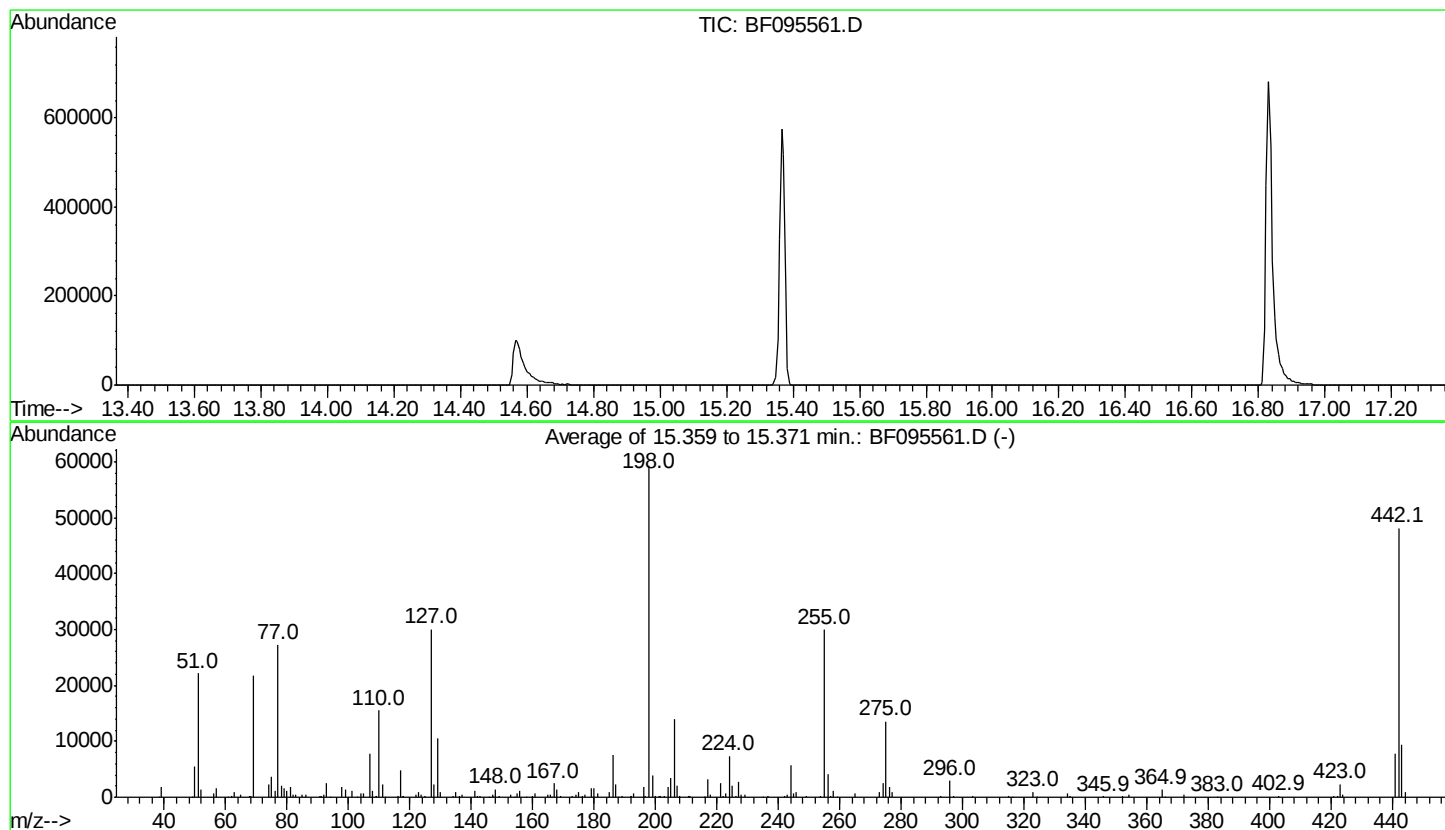

AutoFind: Scans 2282, 2283, 2284; Background Corrected with Scan 2276

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.4	22205	PASS
68	69	0.00	2	0.8	180	PASS
69	198	0.00	100	36.7	21784	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	50.7	30077	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	59304	PASS
199	198	5	9	6.6	3903	PASS
275	198	10	60	22.8	13510	PASS
365	198	1	100	2.2	1318	PASS
441	442	0.01	24	16.1	7719	PASS
442	198	50	100	81.1	48080	PASS
443	442	15	24	19.8	9501	PASS