
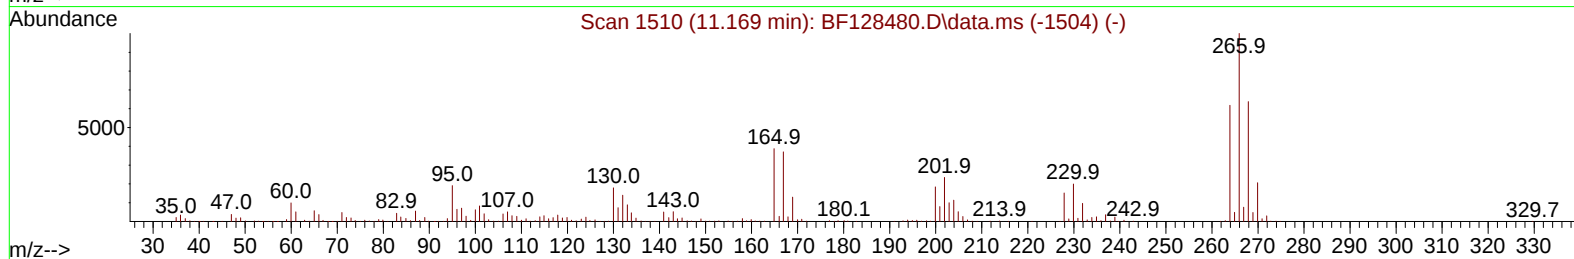
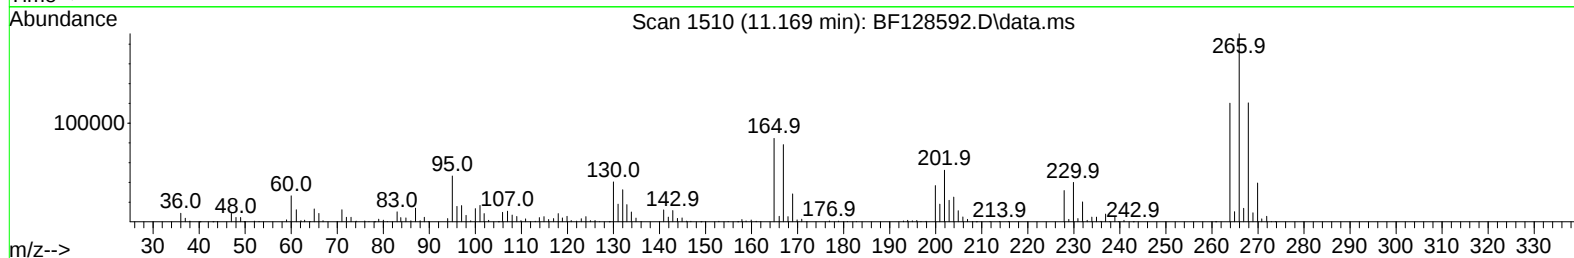


```
Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF053122\  
Data File : BF128592.D  
Acq On    : 31 May 2022  13:35  
Operator  : CG\JU  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1    Sample Multiplier: 1
```

Quant Time: Jun 01 06:15:56 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri May 27 01:51:59 2022
Response via : Initial Calibration

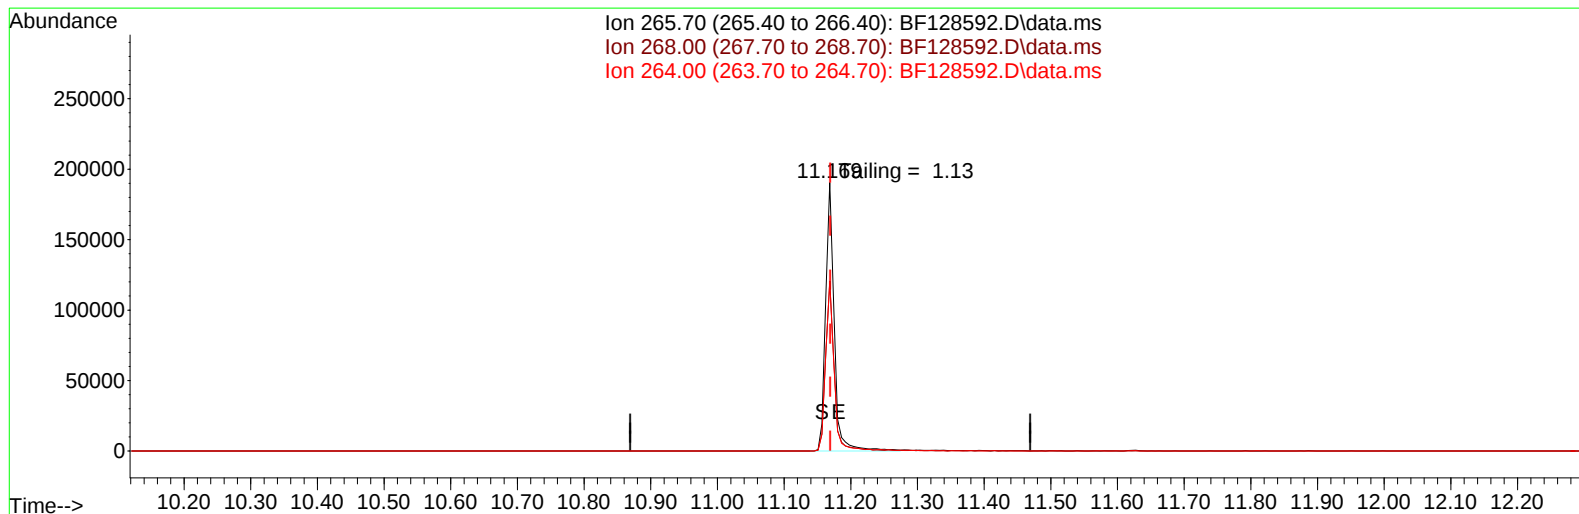

TIC: BF128592.D\data.ms

(70) Pentachlorophenol (C)




11.169min (-0.001) 421078.16 ng

response **172732**

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.70	63.29
264.00	61.80	63.13
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF053122\
Data File : BF128592.D
Acq On : 31 May 2022 13:35
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 01 06:15:56 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri May 27 01:51:59 2022
Response via : Initial Calibration

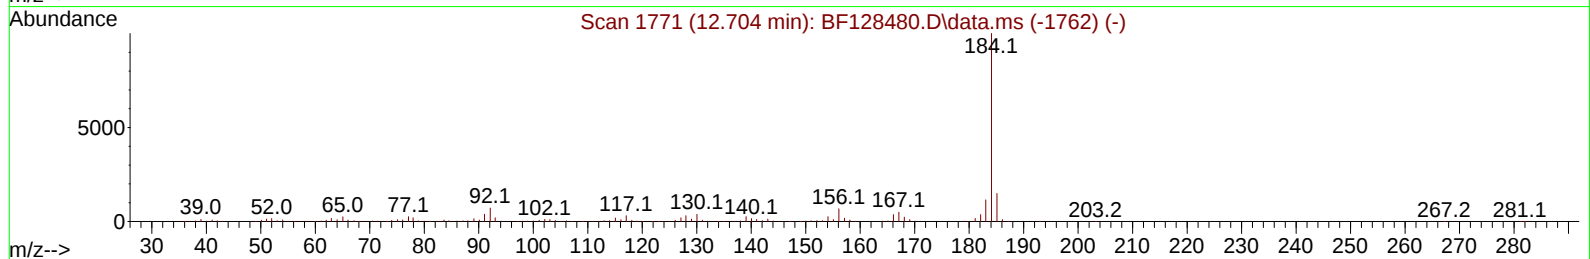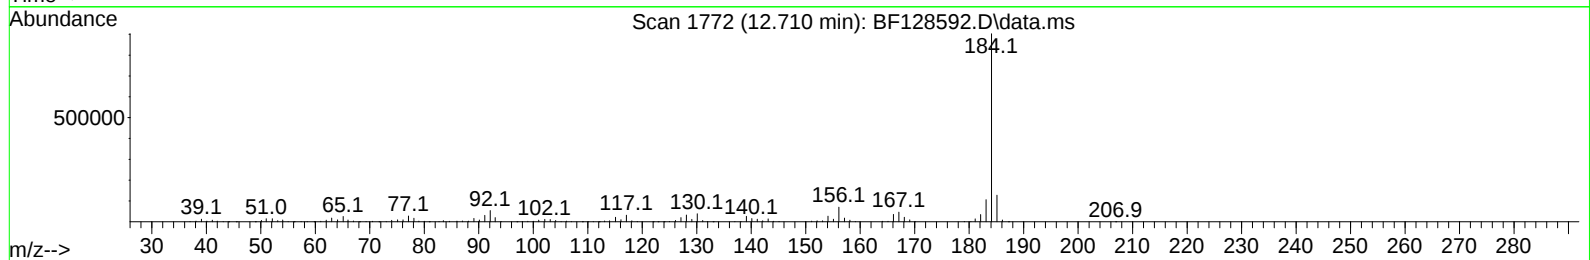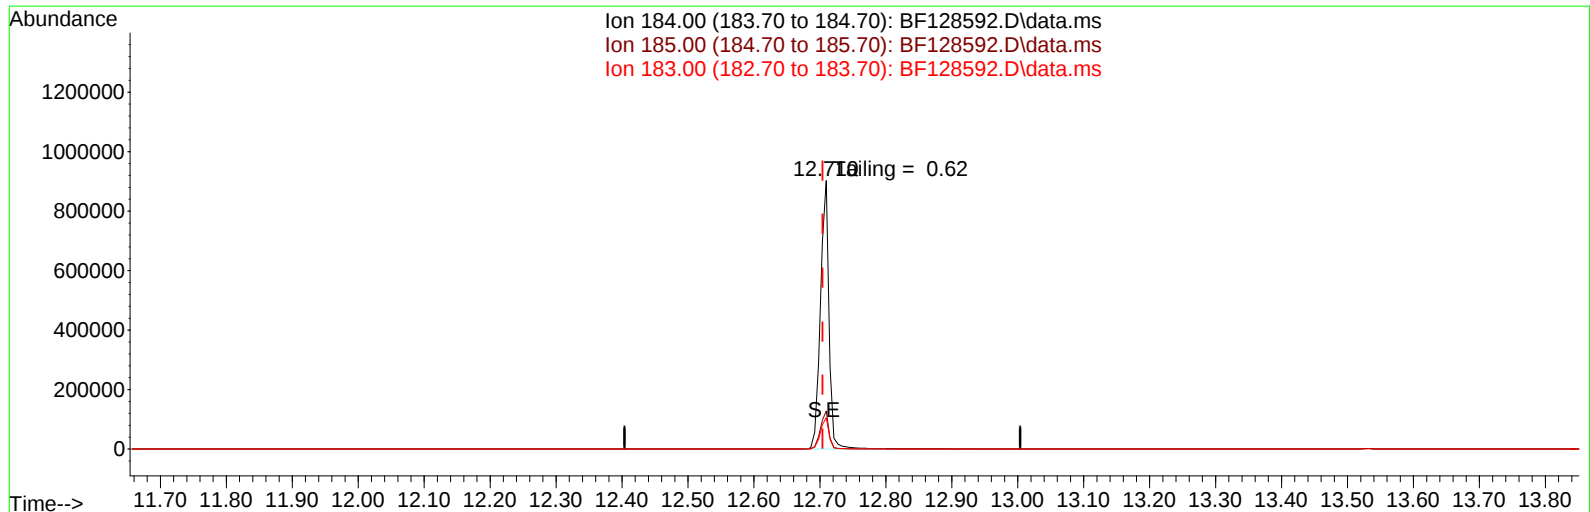

TIC: BF128592.D\data.ms

(77) Benzidine

12.710min (+ 0.006) 310188.75 ng

response 822789

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.90	14.15
183.00	11.60	11.72
0.00	0.00	0.00