

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF053122\
 Data File : BF128588.D
 Acq On : 31 May 2022 10:32
 Operator : CG\JU
 Sample : PB145184BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB145184BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052622.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF128588.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.469	535	541	544	rBV	2845298	2897608	48.23%	9.632%
2	6.469	705	711	714	rBV	2740688	2929691	48.77%	9.738%
3	6.839	770	774	777	rBV	1108373	831622	13.84%	2.764%
4	7.404	864	870	873	rBV	2693139	2914445	48.51%	9.688%
5	8.122	987	992	995	rBV	1274427	1136899	18.92%	3.779%
6	9.204	1169	1176	1179	rBV	5131067	5314332	88.46%	17.665%
7	9.880	1285	1291	1294	rBV	1527340	1346028	22.41%	4.474%
8	10.669	1419	1425	1444	rBV	2630123	2456238	40.89%	8.165%
9	11.369	1540	1544	1547	rBV	1751789	1446543	24.08%	4.808%
10	12.963	1809	1815	1818	rBV	5559570	6007502	100.00%	19.969%
11	14.010	1989	1993	1996	rBV	1466548	1269610	21.13%	4.220%
12	14.104	2003	2009	2018	rBV	136627	160337	2.67%	0.533%
13	15.133	2180	2184	2189	rVB	51065	60406	1.01%	0.201%
14	15.480	2237	2243	2247	rBV	821543	1053490	17.54%	3.502%
15	15.515	2247	2249	2256	rVB	75144	91383	1.52%	0.304%
16	15.951	2319	2323	2329	rBV	59397	94020	1.57%	0.313%
17	16.462	2406	2410	2416	rVB2	45458	74063	1.23%	0.246%

Sum of corrected areas: 30084217

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF053122\
Data File : BF128588.D
Acq On : 31 May 2022 10:32
Operator : CG\JU
Sample : PB145184BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB145184BL










Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Triphenylphosphine oxide Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
14.104	2.53 ng	160337	Chrysene-d12	14.010

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Triphenylphosphine oxide	278	C18H15OP	000791-28-6	95
2			Formaldehyde, (triphenylphosphor...	304	C19H17N2P	015990-54-2	64
3			(E)-7-Benzylidene-1-azabicyclo[3...	293	C15H19N03S	1000483-83-4	62
4			Cobalt,(.eta.<5>-2,4-cyclopentad...	277	C16H15BCo	036682-12-9	32
5			Vanadium, cycloheptatrienyl-(pen...	277	C17H22V	1000155-20-5	25

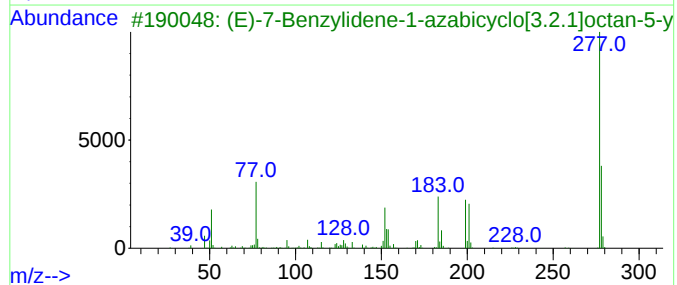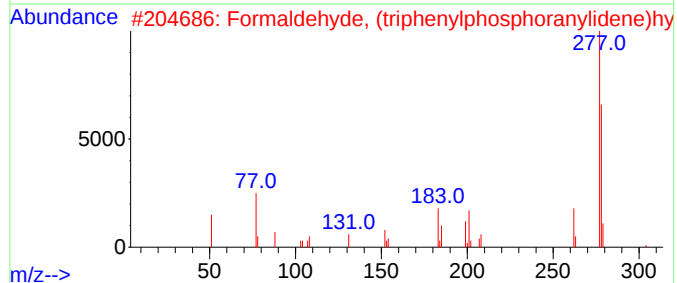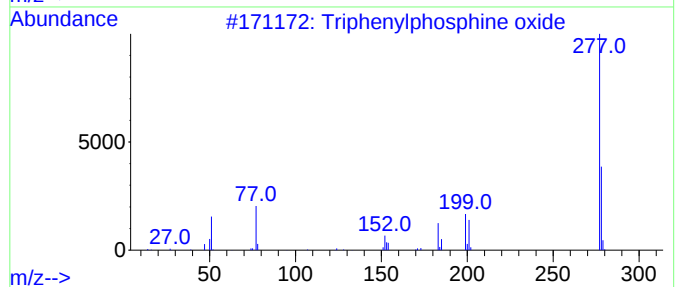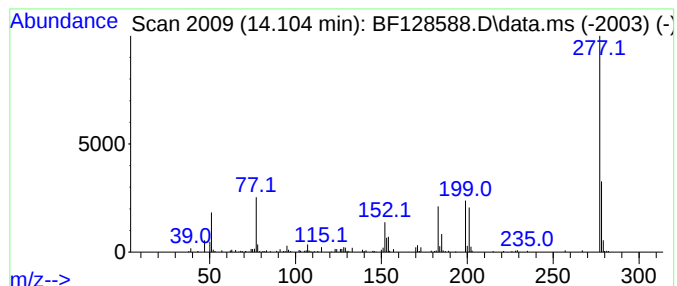

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF053122\
Data File : BF128588.D
Acq On : 31 May 2022 10:32
Operator : CG\JU
Sample : PB145184BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB145184BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
Triphenylphosph...	14.104	2.5	ng	160337	5	14.010	1269610	20.0