

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF053122\
 Data File : BF128614.D
 Acq On : 01 Jun 2022 01:06
 Operator : CG\JU
 Sample : N2952-15 5X
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 P037-SS002-0006-01

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052622.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF128614.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.893	269	273	277	rVB	8398	10861	1.52%	0.170%
2	5.522	546	550	559	rBV	401418	427111	59.79%	6.703%
3	6.546	721	724	734	rBV	329273	408224	57.14%	6.407%
4	6.840	771	774	778	rBV	692280	620623	86.87%	9.740%
5	7.404	866	870	873	rBV	320602	274973	38.49%	4.315%
6	8.128	989	993	996	rBV	899649	714387	100.00%	11.211%
7	9.198	1172	1175	1183	rBV	557366	489525	68.52%	7.682%
8	9.887	1288	1292	1295	rBV	752044	703649	98.50%	11.043%
9	10.675	1423	1426	1435	rBV	241076	229994	32.19%	3.609%
10	10.786	1441	1445	1453	rVB5	5697	11968	1.68%	0.188%
11	11.369	1541	1544	1548	rBV	717033	626876	87.75%	9.838%
12	11.728	1600	1605	1608	rBV5	6692	9093	1.27%	0.143%
13	11.904	1632	1635	1638	rBV5	14677	17811	2.49%	0.280%
14	12.098	1666	1668	1672	rBV5	8678	9865	1.38%	0.155%
15	12.575	1745	1749	1755	rVB2	111243	141226	19.77%	2.216%
16	12.880	1796	1801	1809	rBV7	10332	23572	3.30%	0.370%
17	12.957	1810	1814	1818	rBV	501481	425136	59.51%	6.672%
18	13.351	1877	1881	1886	rVB3	74212	92502	12.95%	1.452%
19	13.592	1919	1922	1929	rVB	32951	48226	6.75%	0.757%
20	14.016	1990	1994	1998	rBV	566146	508960	71.24%	7.987%
21	14.057	1998	2001	2006	rVB2	53190	68740	9.62%	1.079%
22	14.110	2007	2010	2016	rVB	154889	153524	21.49%	2.409%
23	15.486	2240	2244	2250	rVB	293236	355158	49.72%	5.574%




Sum of corrected areas: 6372004

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF053122\
Data File : BF128614.D
Acq On : 01 Jun 2022 01:06
Operator : CG\JU
Sample : N2952-15 5X
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
P037-SS002-0006-01

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

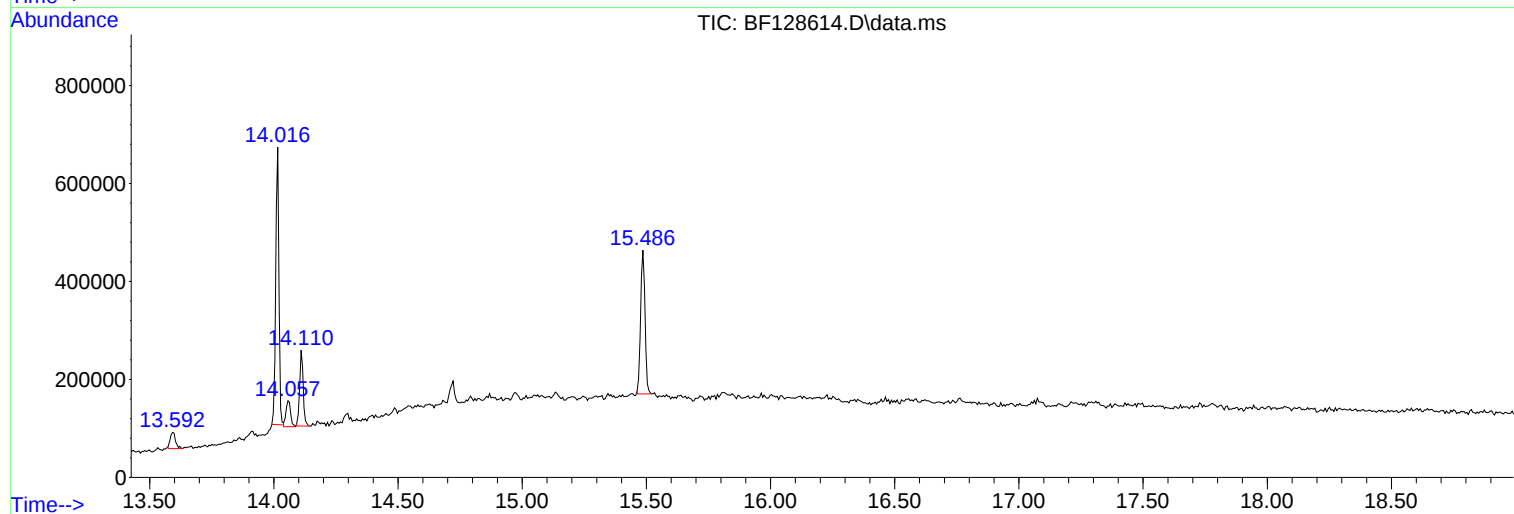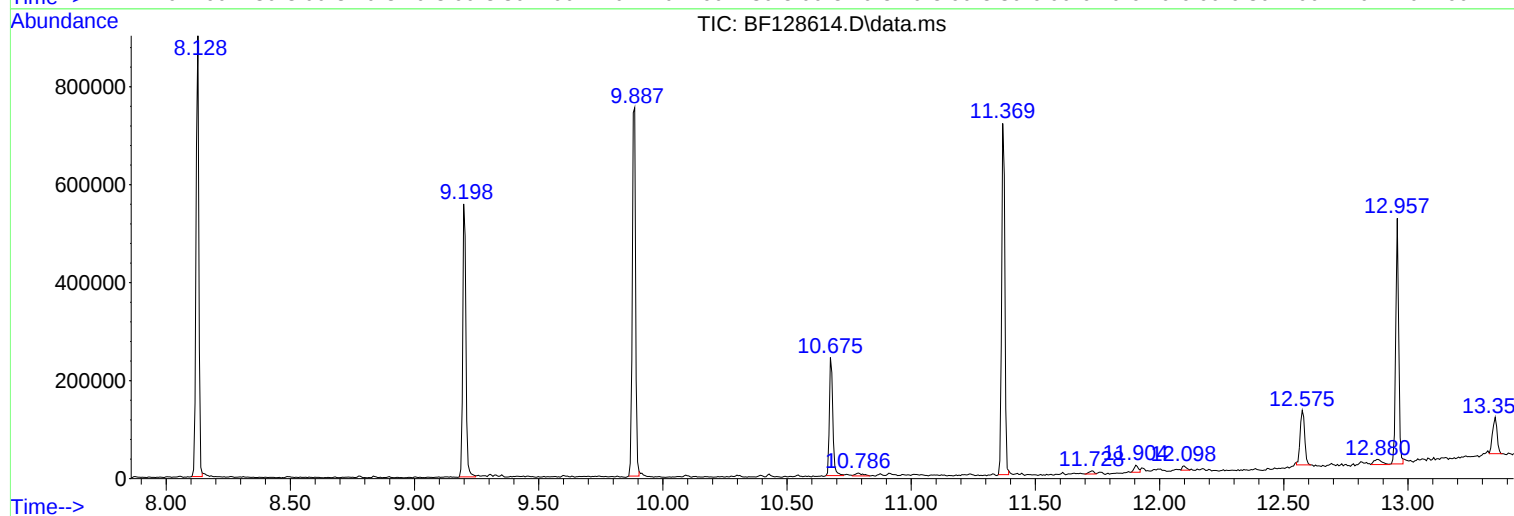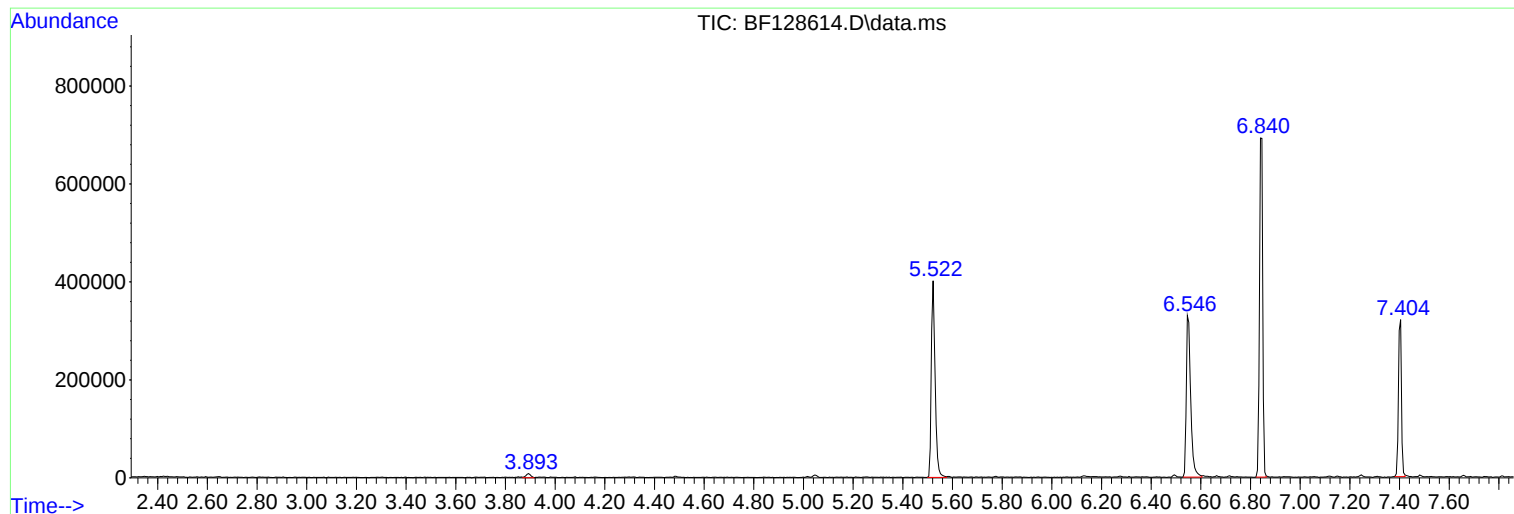

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF053122\
Data File : BF128614.D
Acq On : 01 Jun 2022 01:06
Operator : CG\JU
Sample : N2952-15 5X
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
P037-SS002-0006-01










Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown12.575 Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
12.575	4.51 ng	141226	Phenanthrene-d10	11.369

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Undecanoyl chloride	204	C11H21ClO	017746-05-3	43
2			2-Oxecanone, 10-methyl-, (.+/-.)-	170	C10H18O2	065371-24-6	38
3			n-Heptylamine, N-acetyl-1-cyano-	182	C10H18N2O	1000227-03-9	38
4			2,3-Dihydro-6-hydroxy-3-oxo-2-(p...	209	C10H15N3O2	014628-38-7	38
5			L-Glutamic acid, N-methyl-N-etho...	261	C11H19NO6	1000454-91-1	35

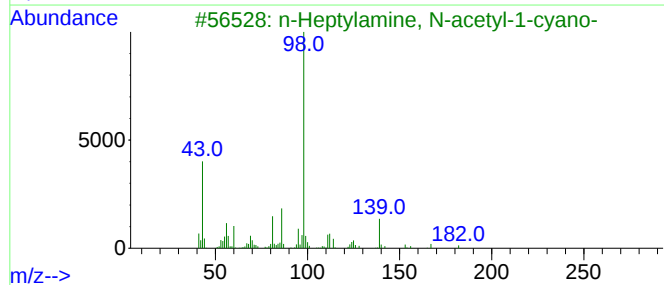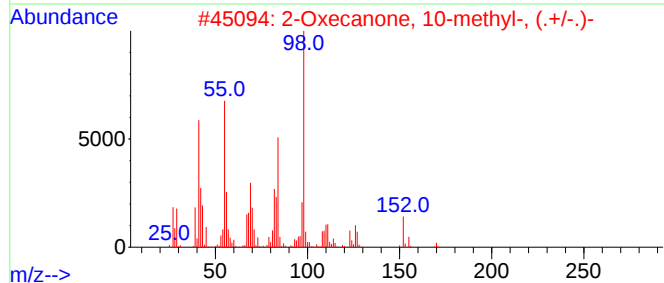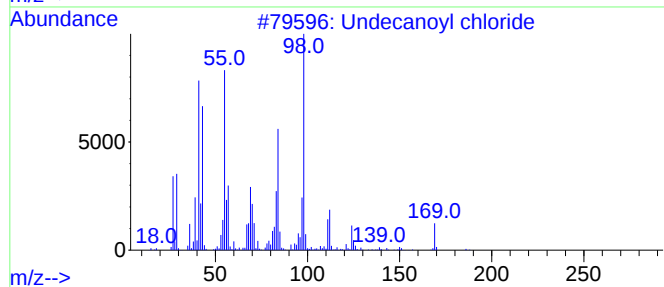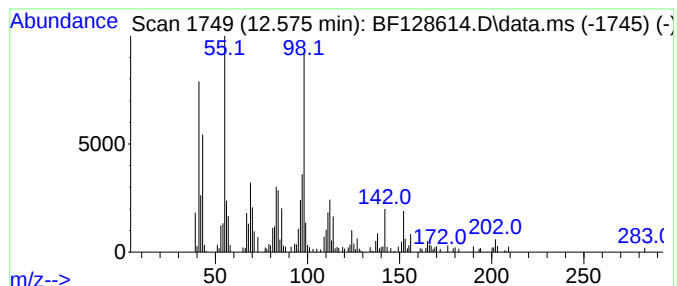

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF053122\
Data File : BF128614.D
Acq On : 01 Jun 2022 01:06
Operator : CG\JU
Sample : N2952-15 5X
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
P037-SS002-0006-01










Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 Myristoyl chloride Concentration Rank 3

R.T.	EstConc	Area	Relative to ISTD	R.T.
13.351	3.63 ng	92502	Chrysene-d12	14.016

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Myristoyl chloride	246	C14H27ClO	000112-64-1	50
2			3-(2-Oxocyclohexyl)propionaldehyde	154	C9H14O2	002568-20-9	50
3			Bicyclo[5.3.1]undecan-11-one	166	C11H18O	013348-11-3	46
4			3-Furanmethanol	98	C5H6O2	004412-91-3	46
5			Cyclohexanone, 2-butyl-	154	C10H18O	001126-18-7	38

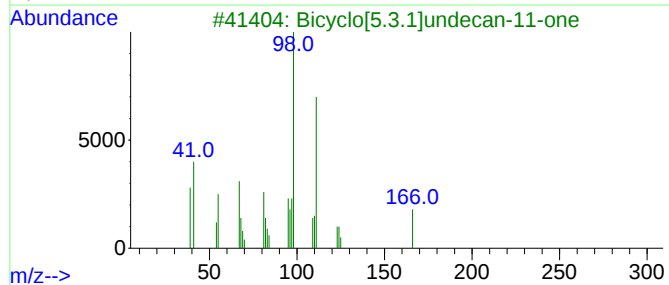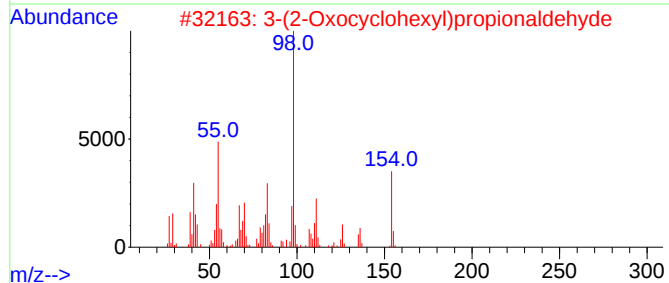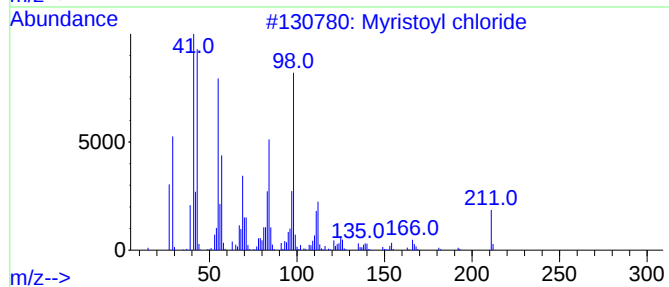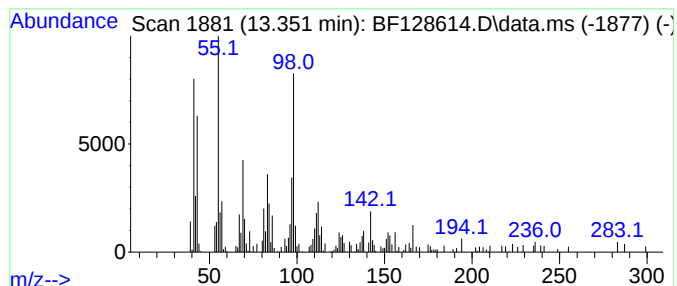

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF053122\
Data File : BF128614.D
Acq On : 01 Jun 2022 01:06
Operator : CG\JU
Sample : N2952-15 5X
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
P037-SS002-0006-01










Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 3 Triphenylphosphine oxide Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
14.110	6.03 ng	153524	Chrysene-d12	14.016

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Triphenylphosphine oxide	278	C18H15OP	000791-28-6	97
2			(E)-7-Benzylidene-1-azabicyclo[3...]	293	C15H19NO3S	1000483-83-4	91
3			Formaldehyde, (triphenylphosphor...]	304	C19H17N2P	015990-54-2	38
4			(Carbethoxymethyl)-triphenylphos...	428	C22H22BrO2P	001530-45-6	38
5			[1,2,4]Triazolo[1,5-a]pyrimidine...	278	C15H14N6	1000350-69-0	12

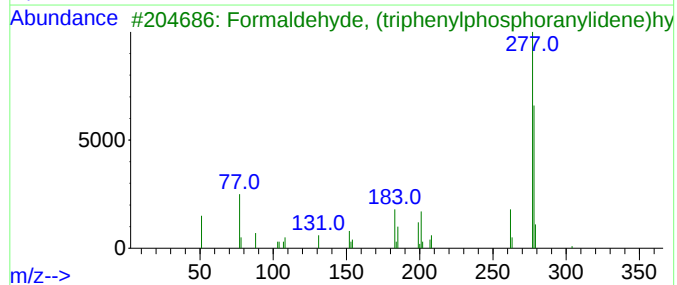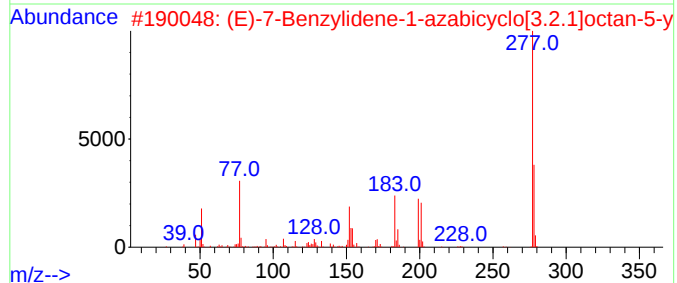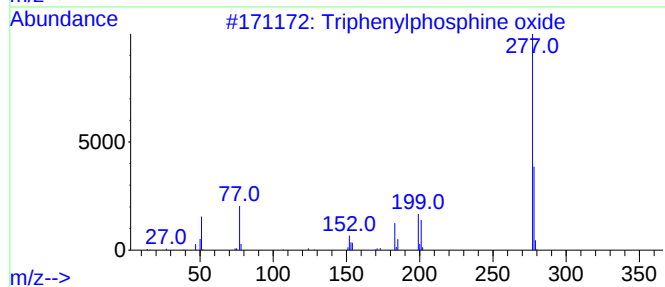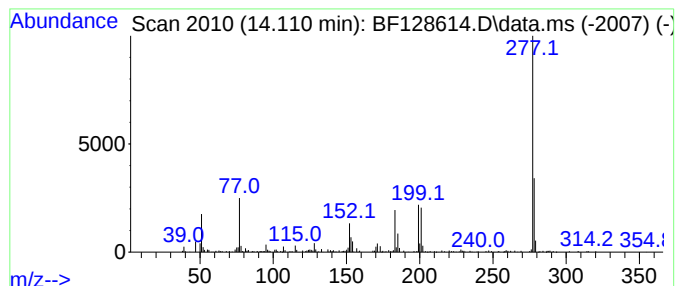

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF053122\
Data File : BF128614.D
Acq On : 01 Jun 2022 01:06
Operator : CG\JU
Sample : N2952-15 5X
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
P037-SS002-0006-01

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown12.575	12.575	4.5	ng	141226	4	11.369	626876	20.0
Myristoyl chloride	13.351	3.6	ng	92502	5	14.016	508960	20.0
Triphenylphosph...	14.110	6.0	ng	153524	5	14.016	508960	20.0