
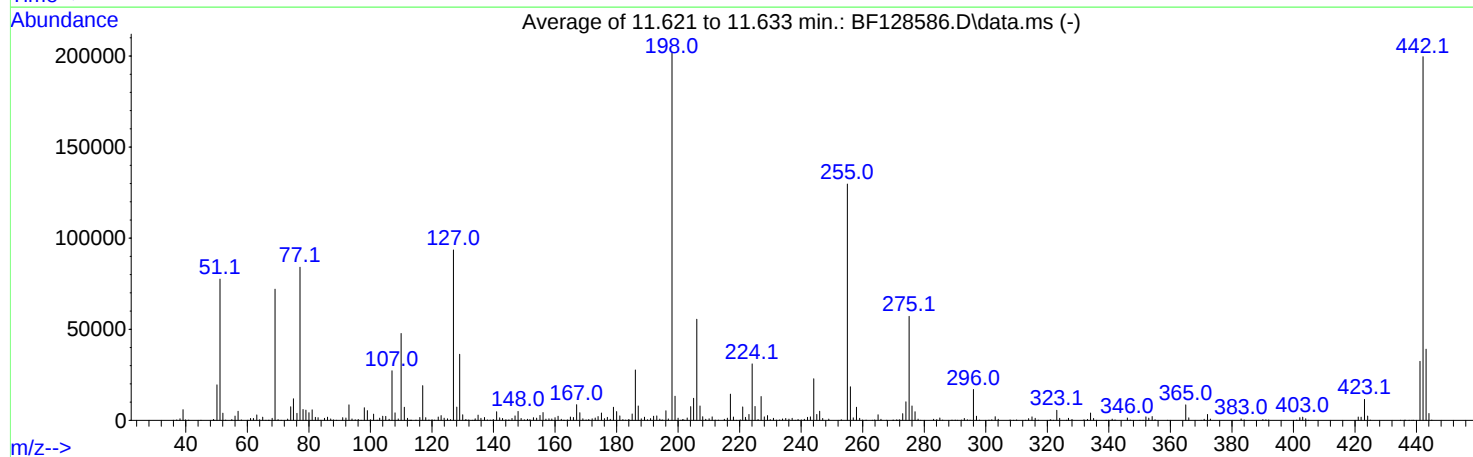


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF053122\
Data File : BF128586.D
Acq On : 31 May 2022 09:34
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052622.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri May 27 01:51:59 2022

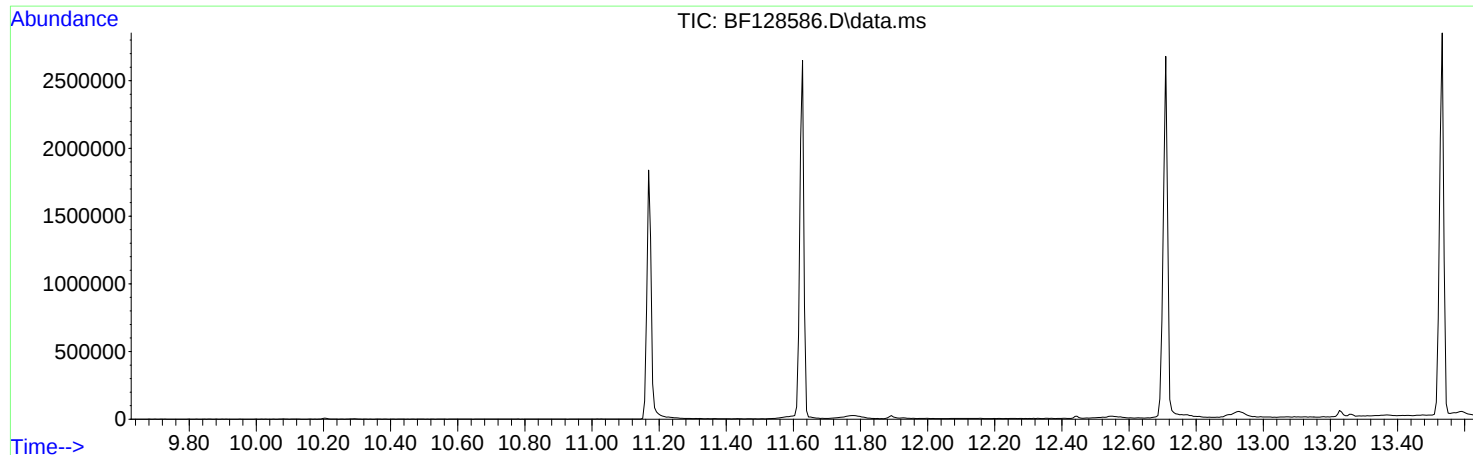


AutoFind: Scans 1587, 1588, 1589; Background Corrected with Scan 1581

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.4	77515	PASS
68	69	0.00	2	1.6	1182	PASS
69	198	0.00	100	35.7	71998	PASS
70	69	0.00	2	0.6	450	PASS
127	198	10	80	46.3	93581	PASS
197	198	0.00	2	0.4	813	PASS
198	198	100	100	100.0	201917	PASS
199	198	5	9	6.6	13262	PASS
275	198	10	60	28.3	57128	PASS
365	198	1	100	4.2	8564	PASS
441	198	0.01	100	16.1	32411	PASS
442	442	50	100	100.0	199595	PASS
443	442	15	24	19.6	39053	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF053122\
Data File : BF128586.D
Acq On : 31 May 2022 09:34
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jun 01 06:12:29 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri May 27 01:51:59 2022
Response via : Initial Calibration

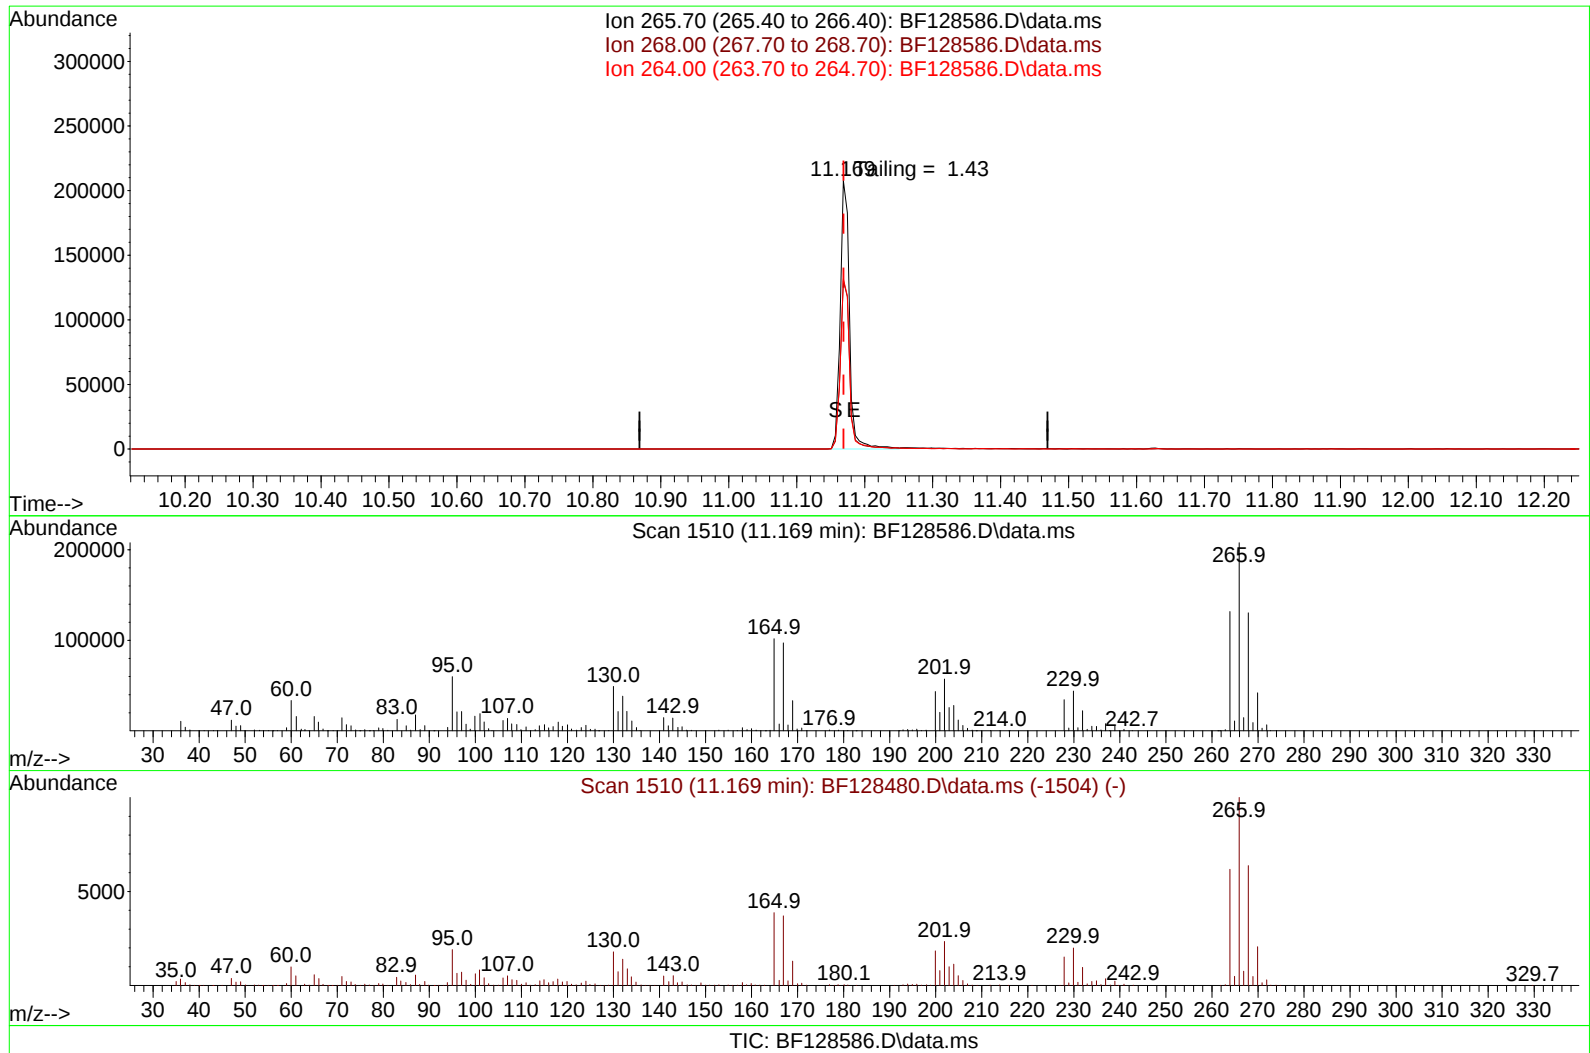

(70) Pentachlorophenol (C)

11.169min (-0.000) 26047.65 ng




response 196135

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.70	62.73
264.00	61.80	63.46
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF053122\
Data File : BF128586.D
Acq On : 31 May 2022 09:34
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jun 01 06:12:29 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri May 27 01:51:59 2022
Response via : Initial Calibration

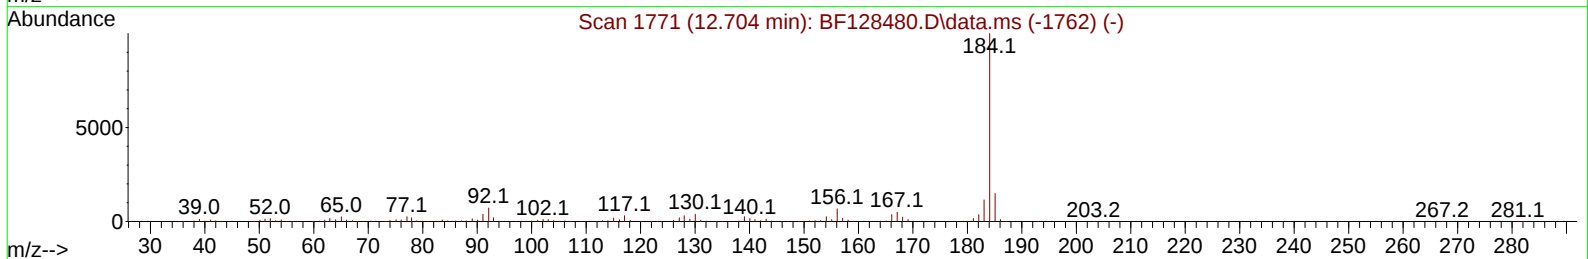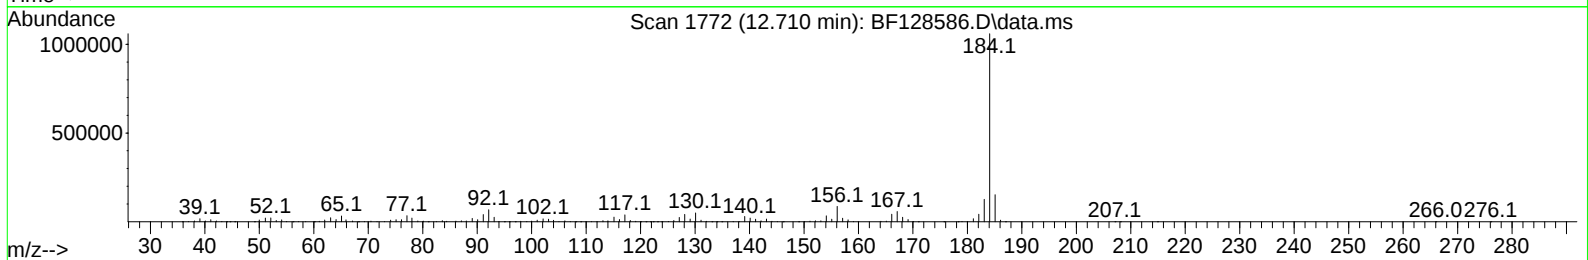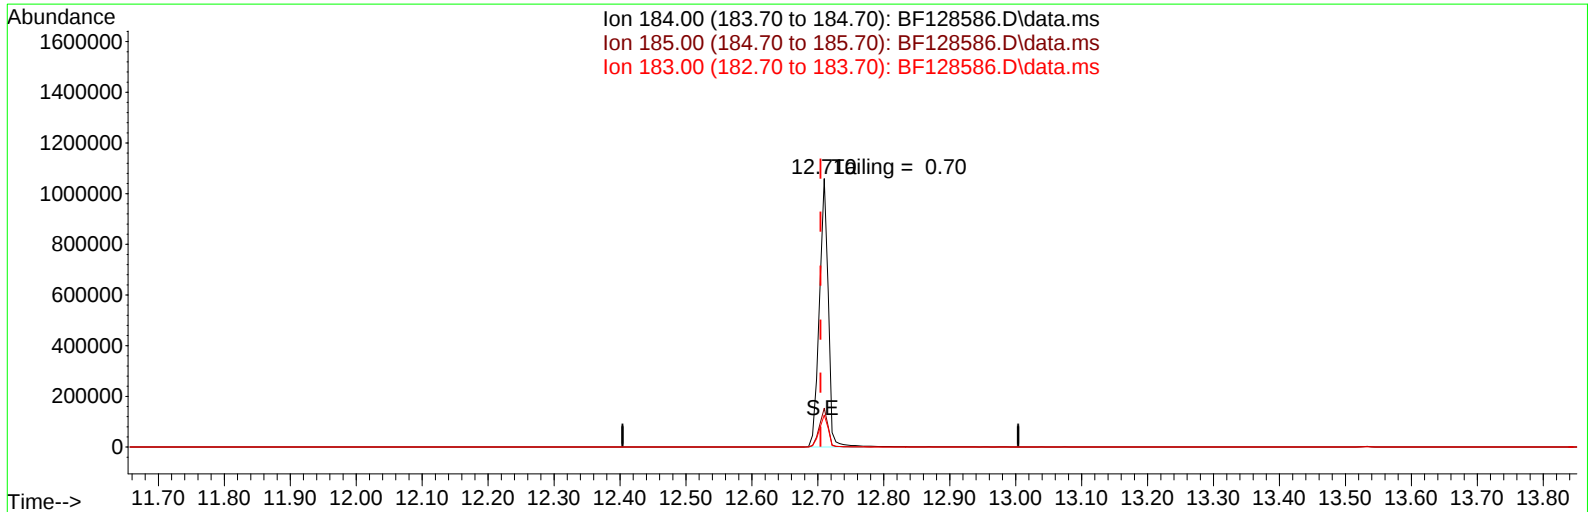

TIC: BF128586.D\data.ms

(77) Benzidine

12.710min (+ 0.006) 518607.46 ng

response 992845

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.90	14.42
183.00	11.60	11.93
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
5/31/2022	BNA_F	<u>BF128586.D</u>
Compound Name	Response	Retention Time
DDT	462495	13.533
DDD	10352	13.227
DDE	1596	12.892
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
11948	474443	2.52

Instrument :
BNA_F
ClientSampleId :
DFTPP