
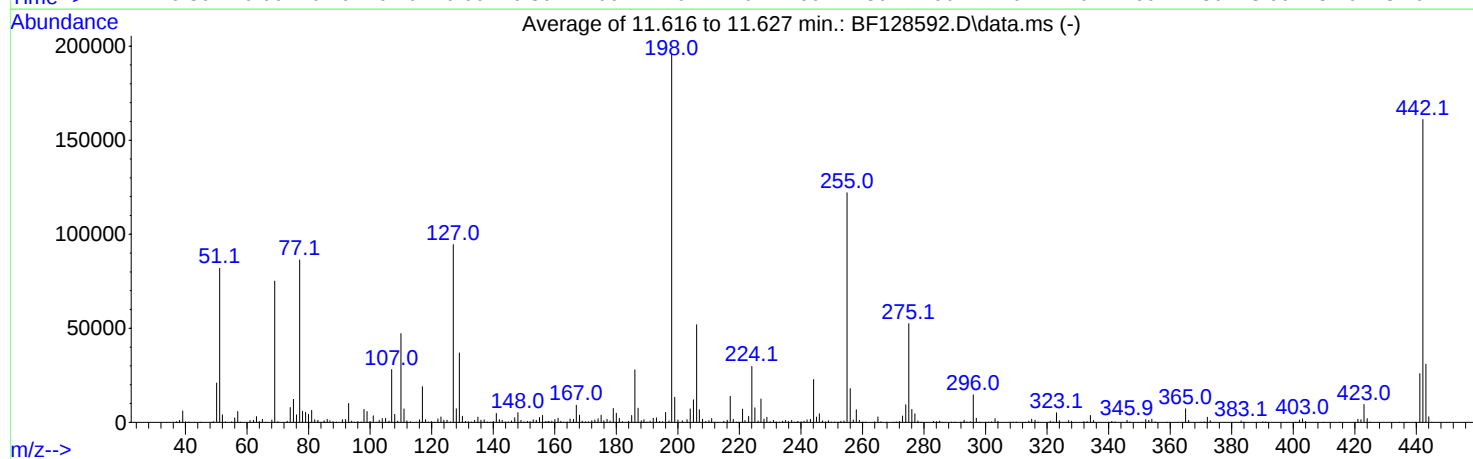


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF053122\
 Data File : BF128592.D
 Acq On : 31 May 2022 13:35
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052622.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri May 27 01:51:59 2022

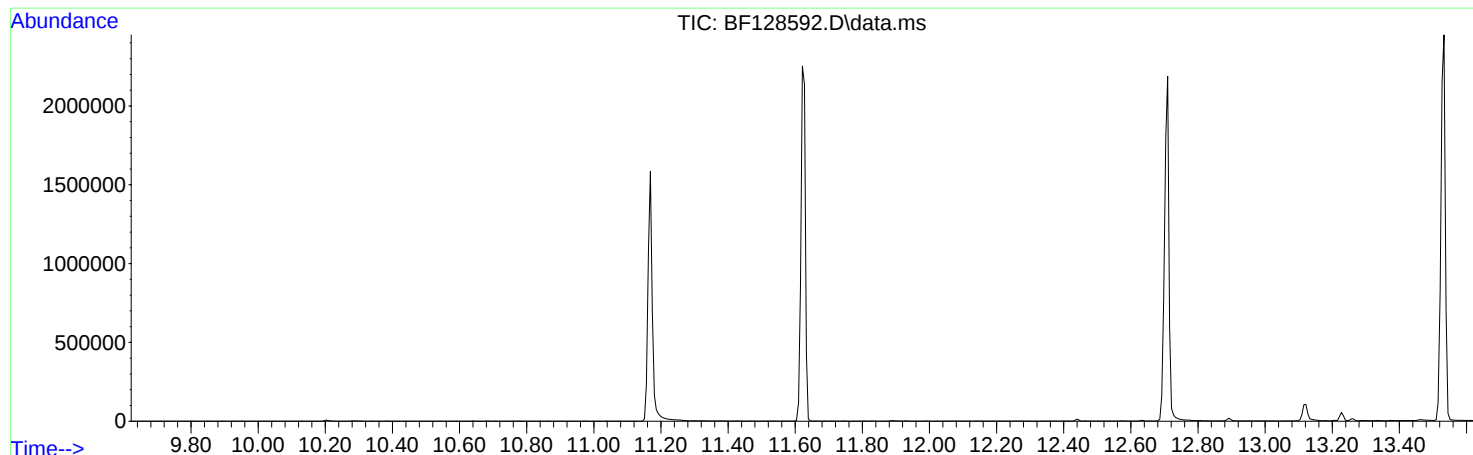




AutoFind: Scans 1586, 1587, 1588; Background Corrected with Scan 1581

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	41.9	81888	PASS
68	69	0.00	2	1.8	1326	PASS
69	198	0.00	100	38.4	75155	PASS
70	69	0.00	2	0.4	328	PASS
127	198	10	80	48.3	94536	PASS
197	198	0.00	2	0.4	767	PASS
198	198	100	100	100.0	195568	PASS
199	198	5	9	6.8	13349	PASS
275	198	10	60	26.8	52499	PASS
365	198	1	100	3.7	7275	PASS
441	198	0.01	100	13.3	25960	PASS
442	442	50	100	100.0	161045	PASS
443	442	15	24	19.2	30997	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF053122\
Data File : BF128592.D
Acq On : 31 May 2022 13:35
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jun 01 06:15:56 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri May 27 01:51:59 2022
Response via : Initial Calibration

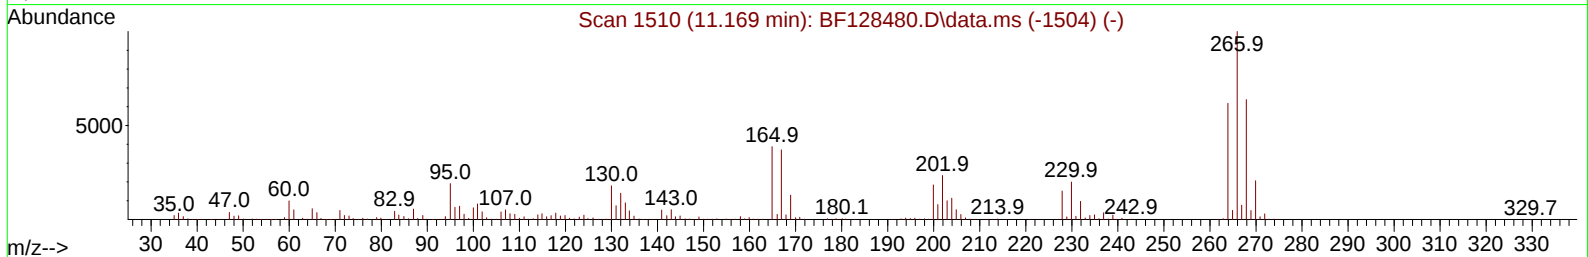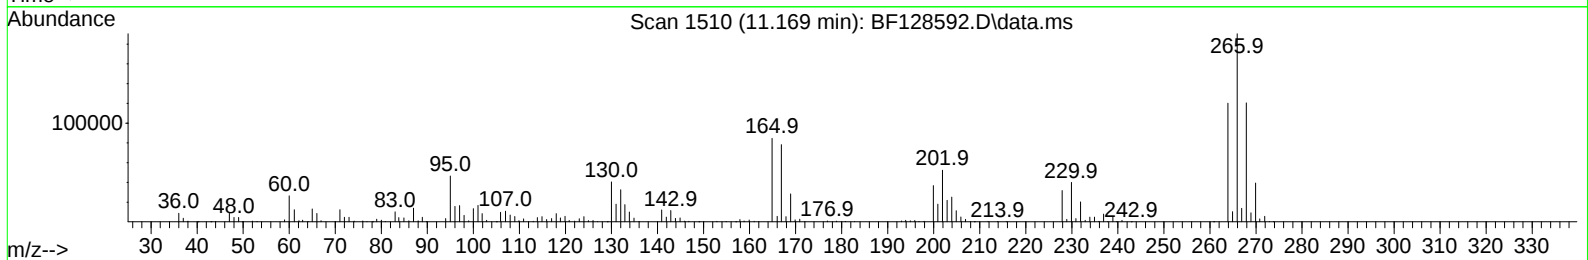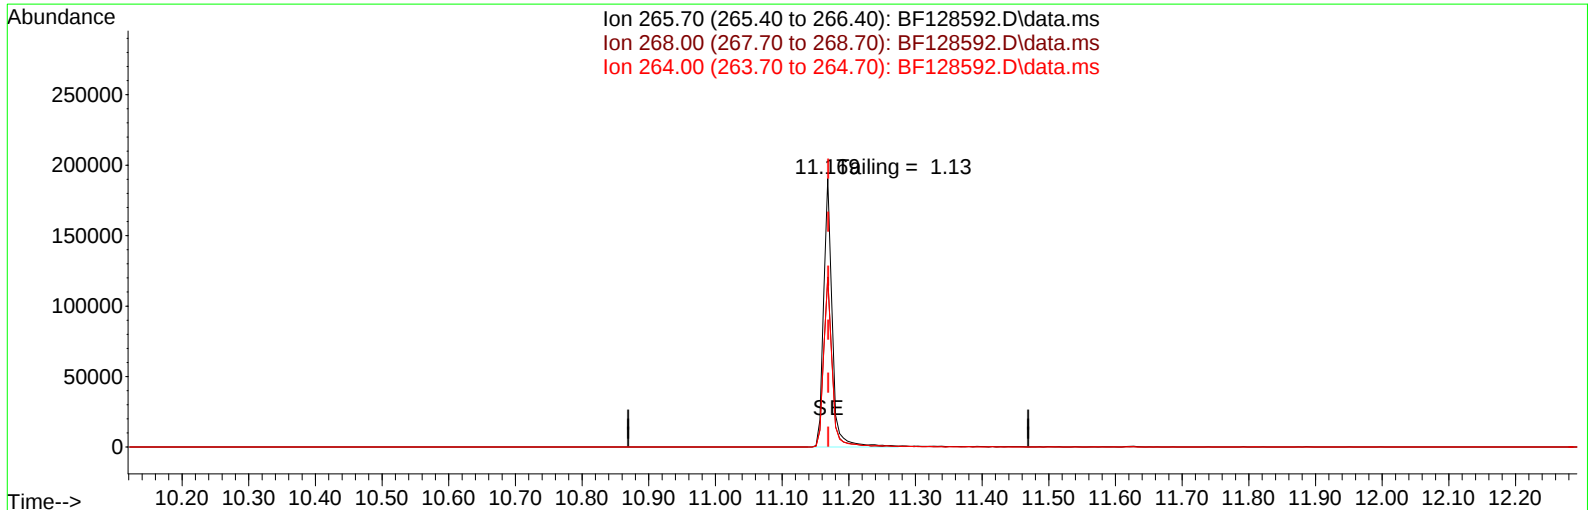

TIC: BF128592.D\data.ms

(70) Pentachlorophenol (C)

11.169min (-0.001) 421078.16 ng




response 172732

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.70	63.29
264.00	61.80	63.13
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF053122\
 Data File : BF128592.D
 Acq On : 31 May 2022 13:35
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Jun 01 06:15:56 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052622.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri May 27 01:51:59 2022
 Response via : Initial Calibration

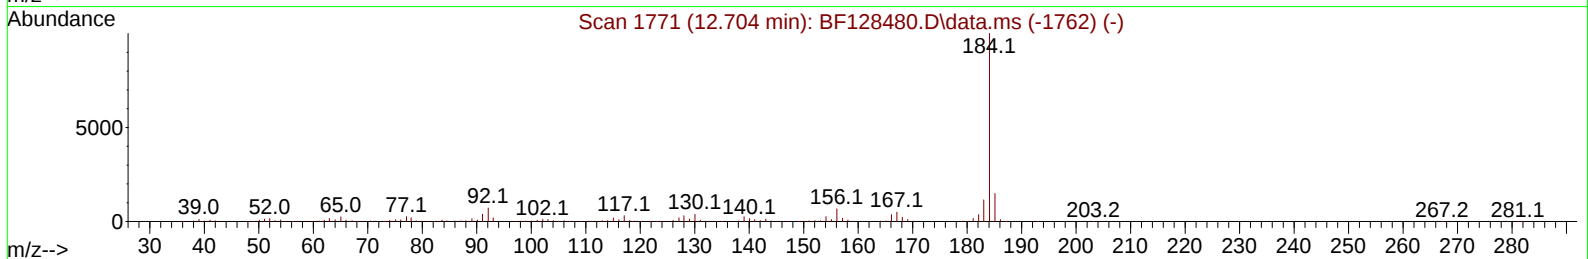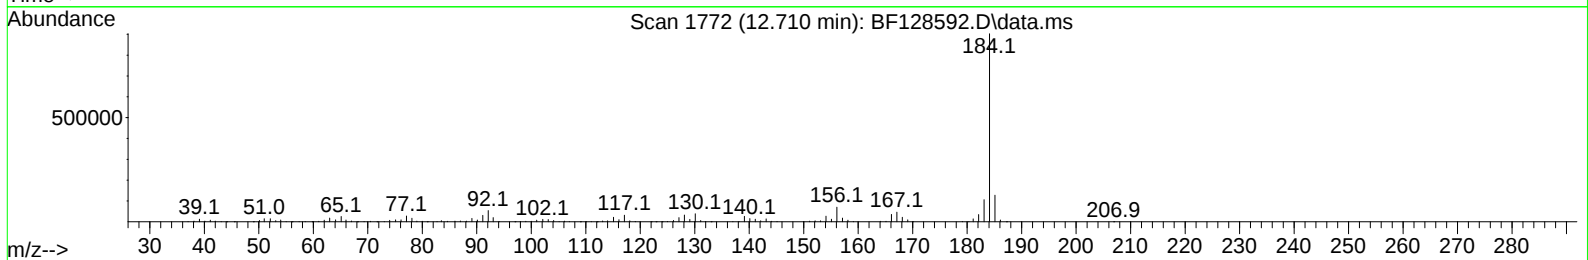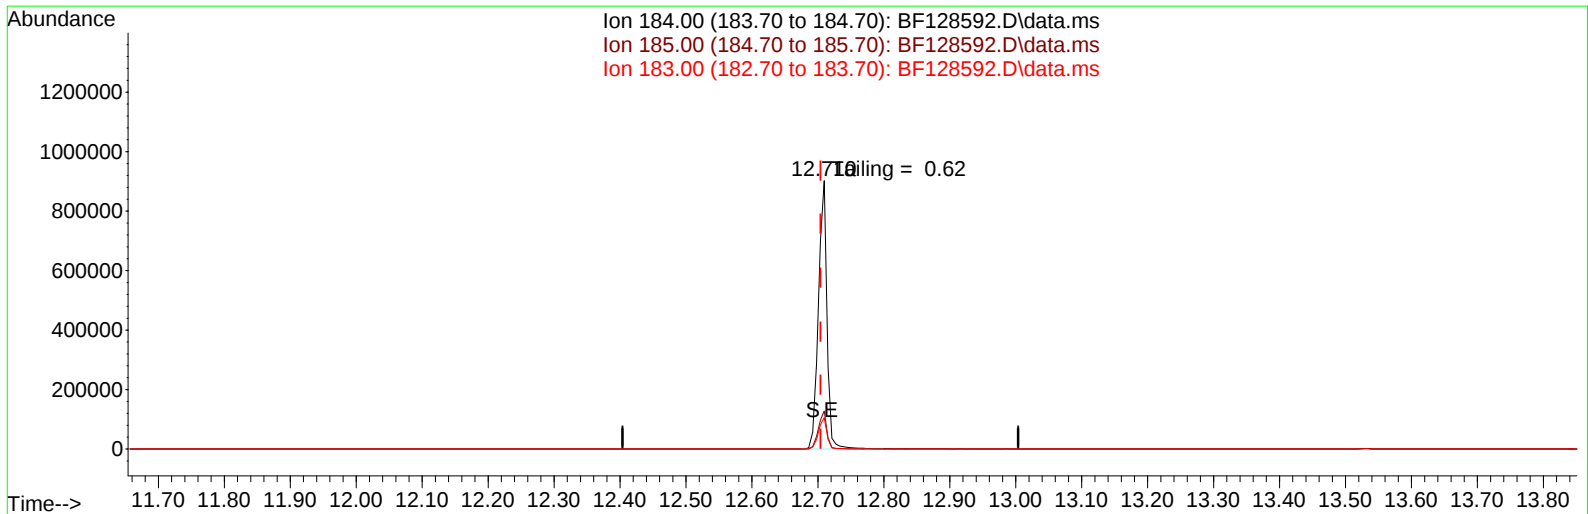

TIC: BF128592.D\data.ms

(77) Benzidine

12.710min (+ 0.006) 310188.75 ng

response 822789

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.90	14.15
183.00	11.60	11.72
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
5/31/2022	BNA_F	<u>BF128592.D</u>
Compound Name	Response	Retention Time
DDT	430277	13.533
DDD	11351	13.227
DDE	2425	12.892
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
13776	444053	3.10

Instrument :
BNA_F
ClientSampleId :
DFTPP