

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF053123\
 Data File : BF133542.D
 Acq On : 31 May 2023 16:44
 Operator : CG\JU
 Sample : 02977-02
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 FOUNDATION-TEST-PIT

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052523.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF133542.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.757	109	114	121	rVB	277037	379076	8.24%	1.370%
2	4.045	327	333	340	rBV	57036	73518	1.60%	0.266%
3	4.428	393	398	402	rVB	62778	67088	1.46%	0.242%
4	4.628	427	432	436	rVB	109748	121913	2.65%	0.441%
5	4.692	436	443	447	rBV	93074	93810	2.04%	0.339%
6	5.051	499	504	511	rVB2	498004	784192	17.06%	2.834%
7	5.451	564	572	575	rBV	3150815	3196698	69.53%	11.551%
8	6.457	737	743	746	rBV	2952024	2989430	65.02%	10.802%
9	6.833	803	807	810	rBV	869847	760595	16.54%	2.748%
10	7.392	897	902	905	rBV	2288479	2322040	50.50%	8.390%
11	8.110	1021	1024	1028	rBV	1167156	1013786	22.05%	3.663%
12	9.192	1204	1208	1211	rBV	4603306	3981313	86.59%	14.386%
13	9.869	1319	1323	1326	rBV	1385070	1109327	24.13%	4.008%
14	10.657	1452	1457	1460	rBV	3070406	2774640	60.35%	10.026%
15	11.351	1572	1575	1579	rBV	1394727	1200906	26.12%	4.339%
16	12.951	1841	1847	1850	rBV	4379108	4597742	100.00%	16.613%
17	13.421	1922	1927	1934	rBV	82023	80509	1.75%	0.291%
18	13.992	2017	2024	2027	rBV	1173193	1258424	27.37%	4.547%
19	14.015	2027	2028	2033	rVB	108808	82452	1.79%	0.298%
20	15.451	2266	2272	2277	rBV	676614	788151	17.14%	2.848%




Sum of corrected areas: 27675610

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF053123\
Data File : BF133542.D
Acq On : 31 May 2023 16:44
Operator : CG\JU
Sample : 02977-02
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
FOUNDATION-TEST-PIT

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052523.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

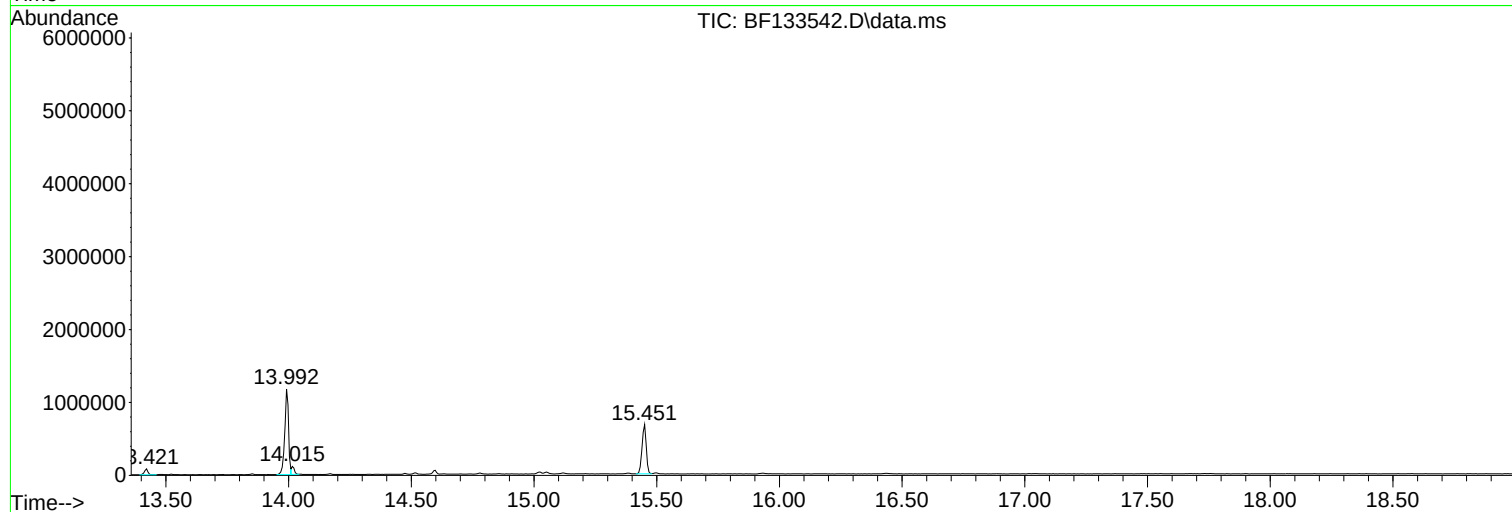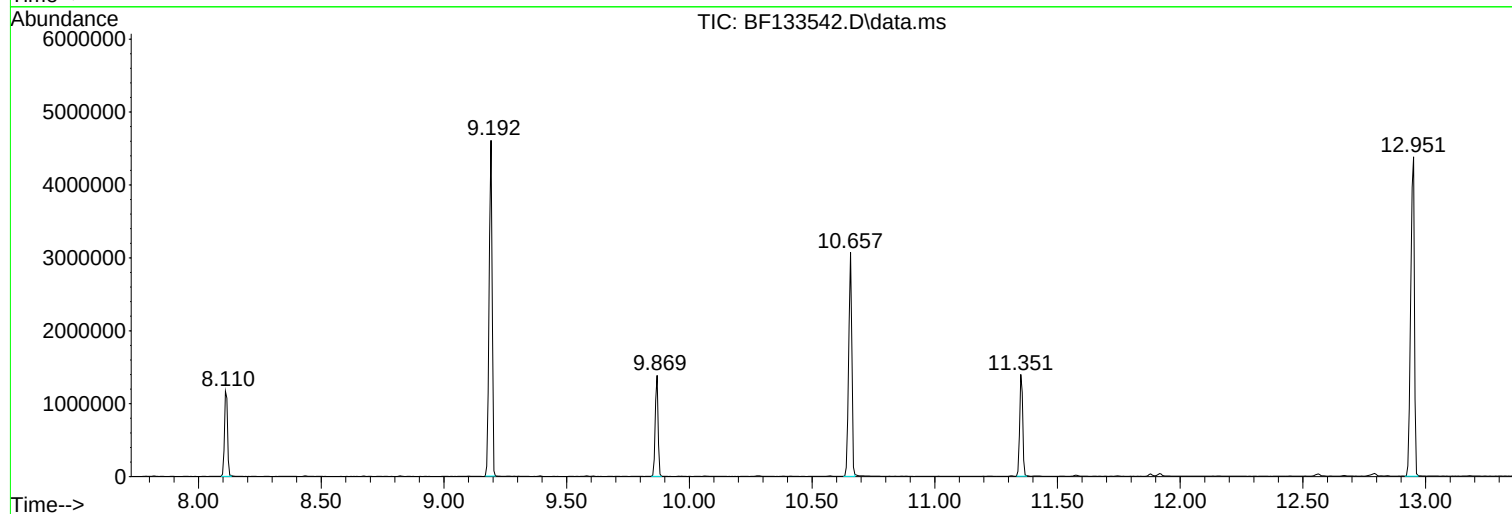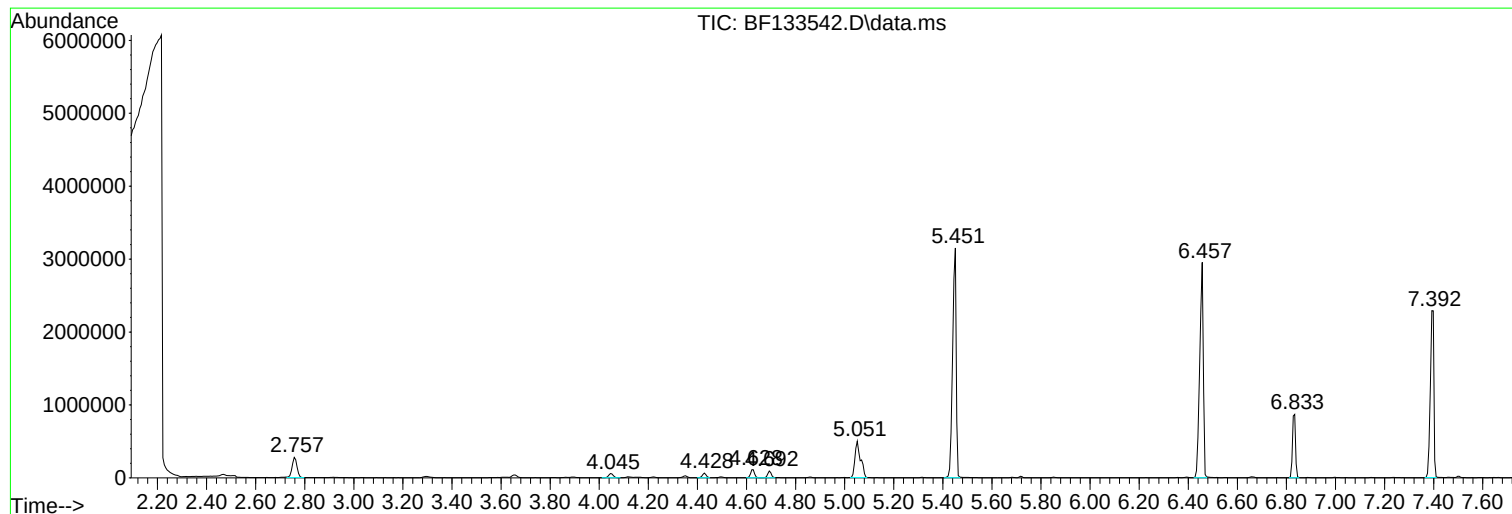

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF053123\
Data File : BF133542.D
Acq On : 31 May 2023 16:44
Operator : CG\JU
Sample : 02977-02
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
FOUNDATION-TEST-PIT

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052523.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF053123\
Data File : BF133542.D
Acq On : 31 May 2023 16:44
Operator : CG\JU
Sample : 02977-02
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
FOUNDATION-TEST-PIT

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052523.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------