


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF053123\
Data File : BF133534.D
Acq On : 31 May 2023 11:20
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052523.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue May 30 12:58:40 2023

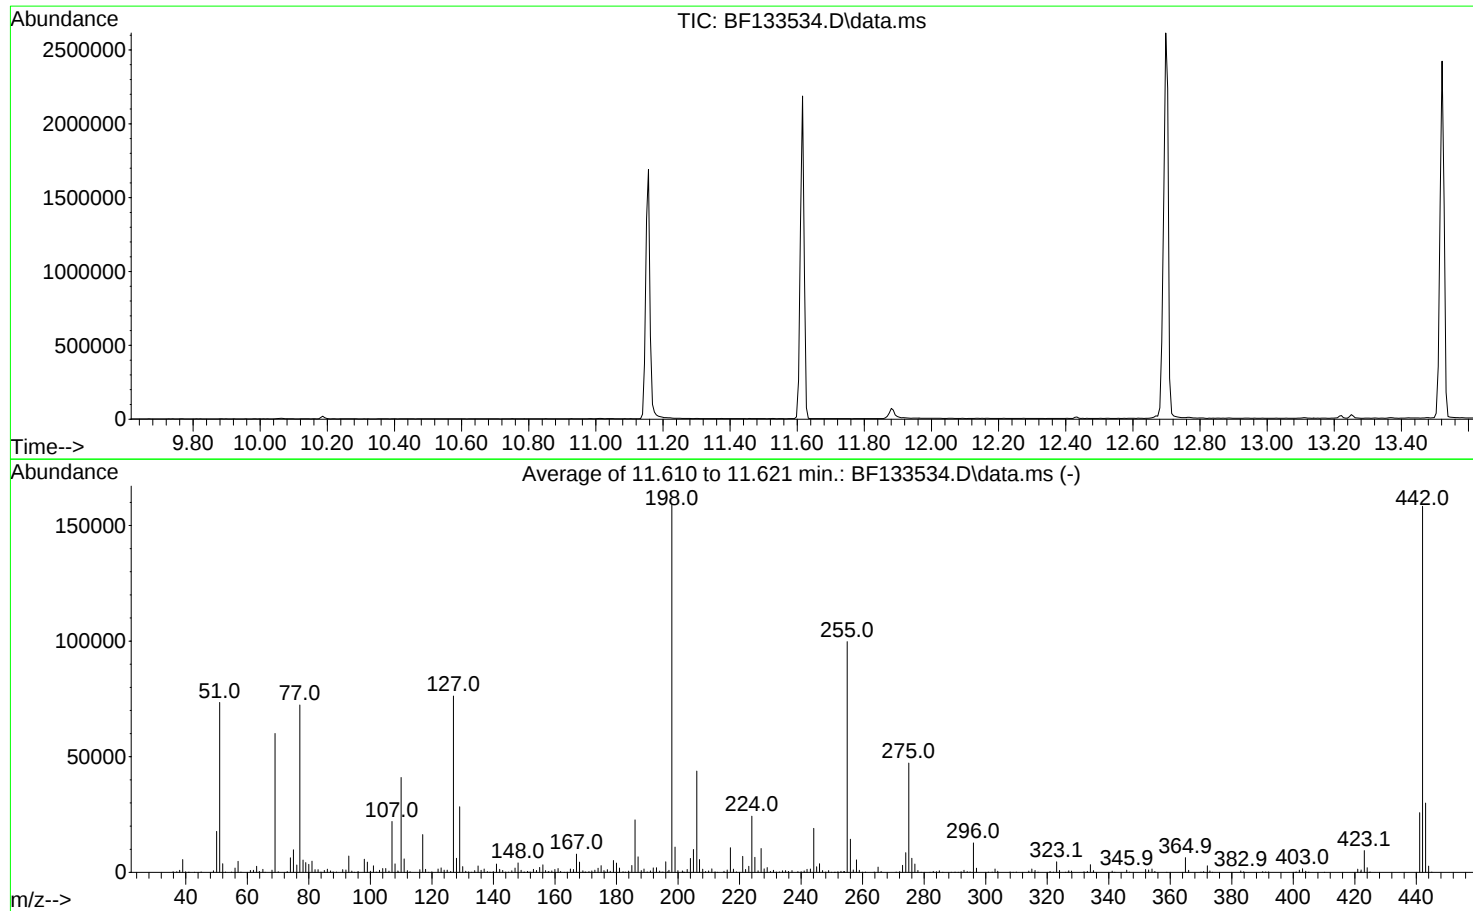

AutoFind: Scans 1619, 1620, 1621; Background Corrected with Scan 1614

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	46.2	73477	PASS
68	69	0.00	2	1.7	999	PASS
69	198	0.00	100	37.7	60043	PASS
70	69	0.00	2	0.5	296	PASS
127	198	10	80	48.0	76285	PASS
197	198	0.00	2	0.6	888	PASS
198	198	100	100	100.0	159075	PASS
199	198	5	9	6.9	10962	PASS
275	198	10	60	29.7	47293	PASS
365	198	1	100	4.0	6371	PASS
441	198	0.01	100	16.2	25796	PASS
442	442	50	100	100.0	158299	PASS
443	442	15	24	18.9	29987	PASS

DDT Breakdown


Date	Instrument Name	DFTPP Data File
5/31/2023	BNA_F	<u>BF133534.D</u>
Compound Name	Response	Retention Time
DDT	401948	13.521
DDD	7195	13.251
DDE	418	12.892
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
7613	409561	1.86

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF053123\
 Data File : BF133534.D
 Acq On : 31 May 2023 11:20
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: May 31 13:00:34 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052523.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue May 30 12:58:40 2023
 Response via : Initial Calibration

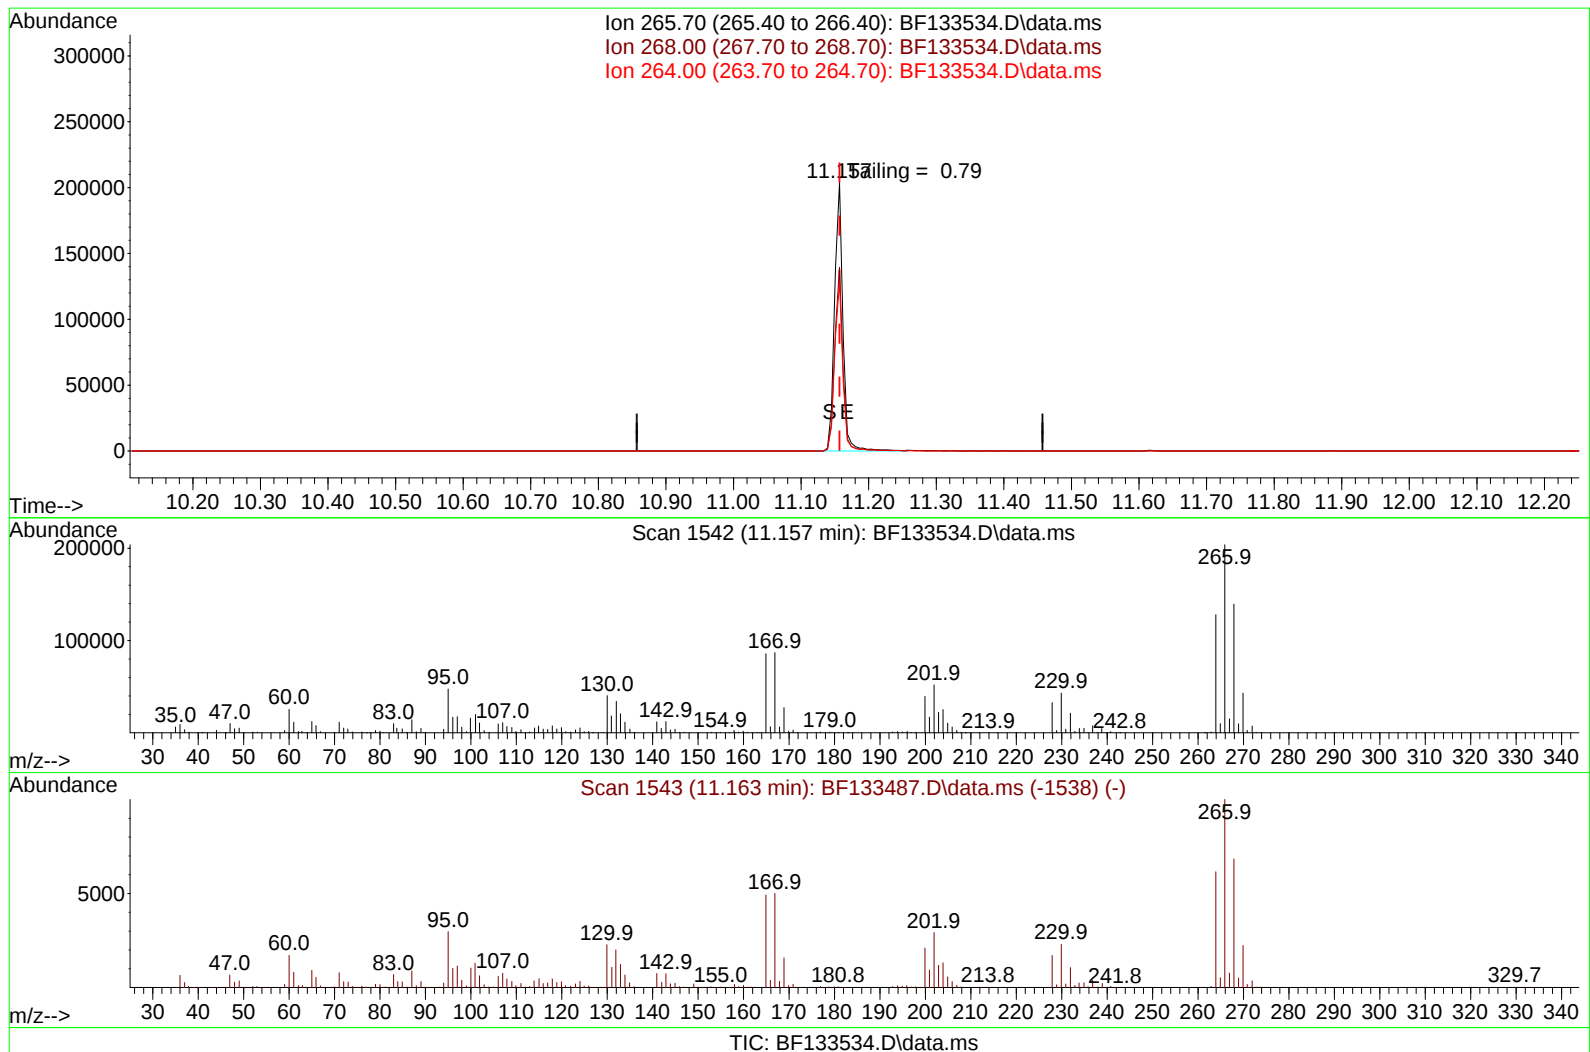

(70) Pentachlorophenol (C)

11.157min (-0.000) 471309.51 ng




response 175265

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	68.30	68.47
264.00	61.50	62.85
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF053123\
Data File : BF133534.D
Acq On : 31 May 2023 11:20
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: May 31 13:00:34 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052523.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 30 12:58:40 2023
Response via : Initial Calibration

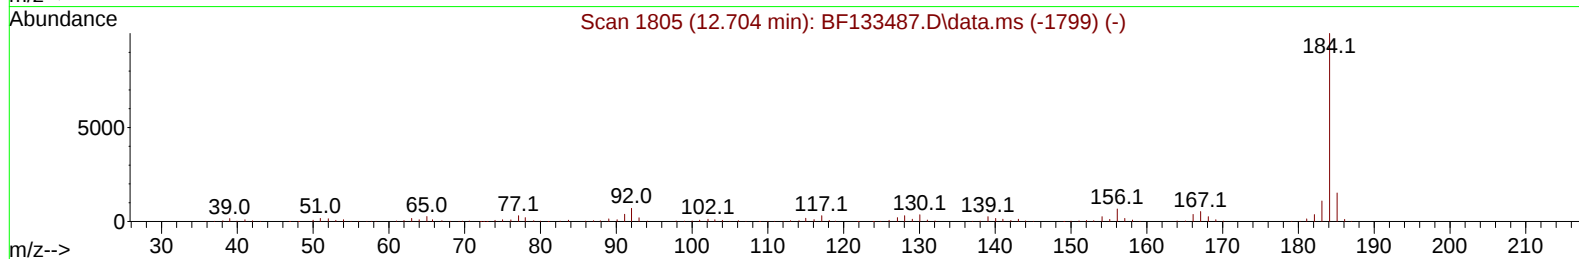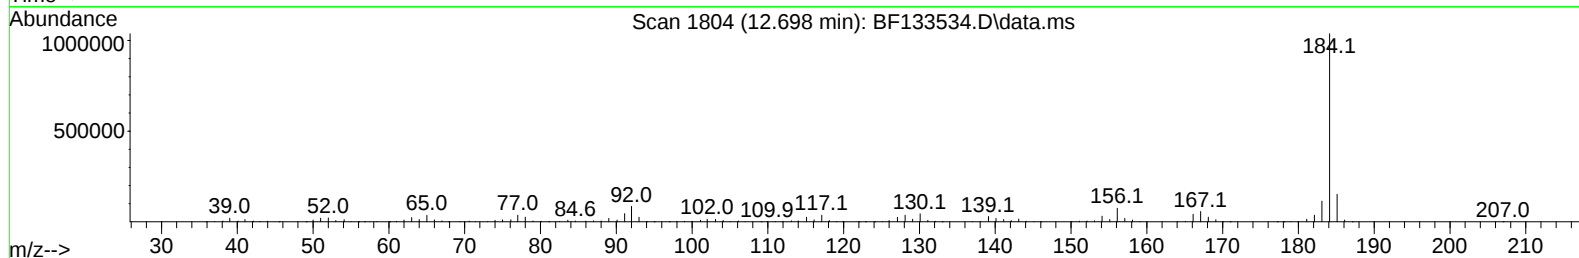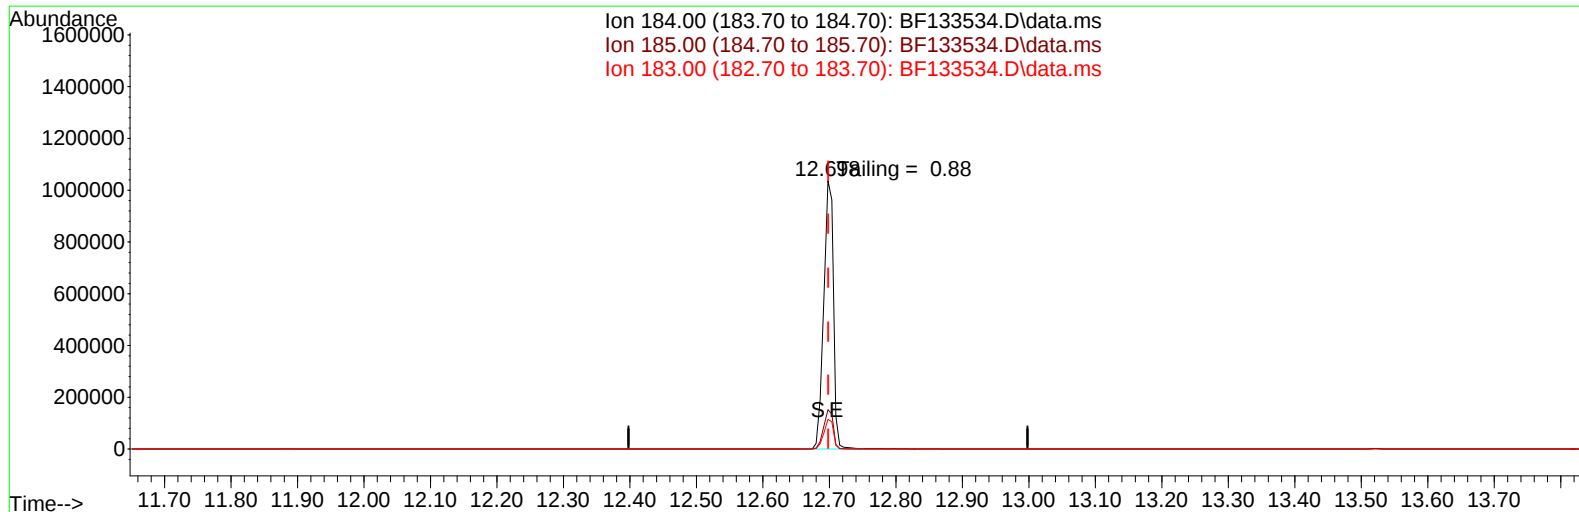

TIC: BF133534.D\data.ms

(77) Benzidine

12.698min (-0.000) 0.00 ng

response 1053506

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.20	14.66
183.00	10.90	11.03
0.00	0.00	0.00