
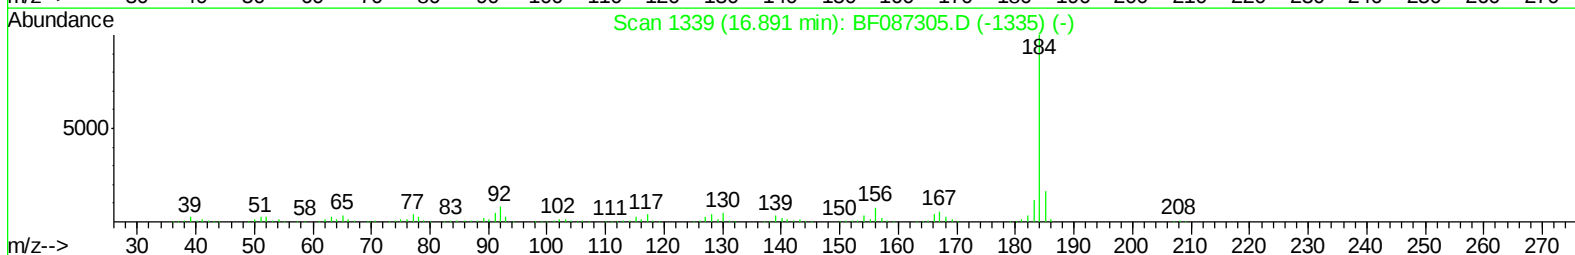
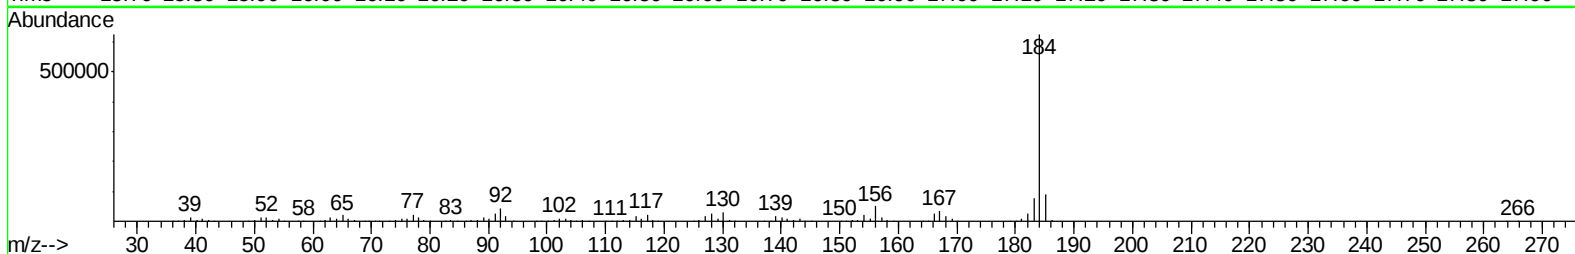


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF060116\
Data File : BF087641.D
Acq On : 2 Jun 2016 5:57
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 02 08:12:09 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF052316.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 02 02:13:57 2016
Response via : Initial Calibration

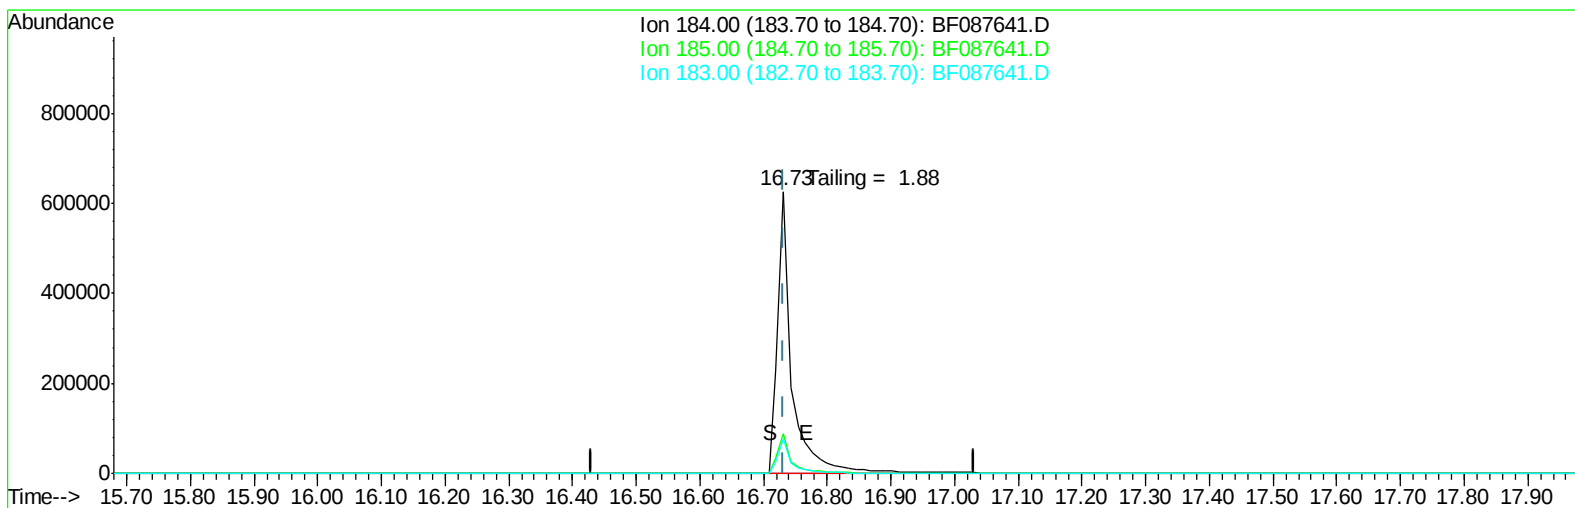

TIC: BF087641.D

(76) Benzidine




16.731min (+0.000) 0.00ng

response 975111

Ion	Exp%	Act%
184.00	100	100
185.00	17.00	14.25
183.00	12.20	12.12
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF060116\
Data File : BF087641.D
Acq On : 2 Jun 2016 5:57
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 02 08:12:09 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF052316.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 02 02:13:57 2016
Response via : Initial Calibration

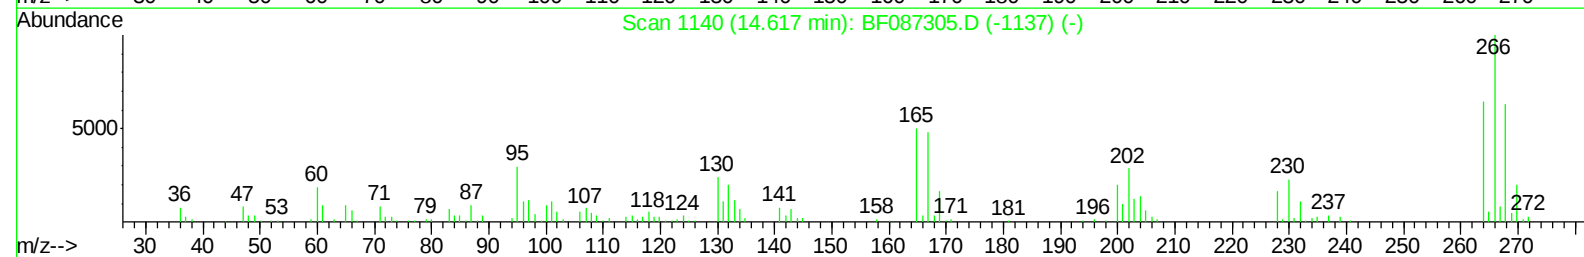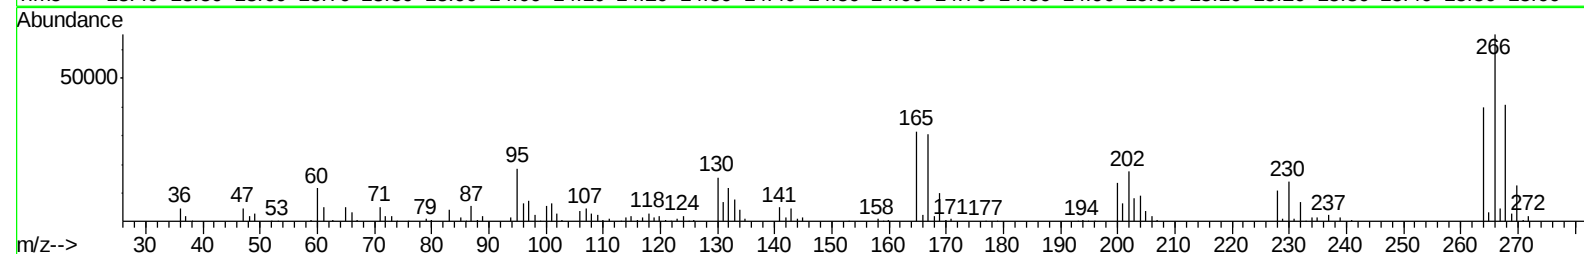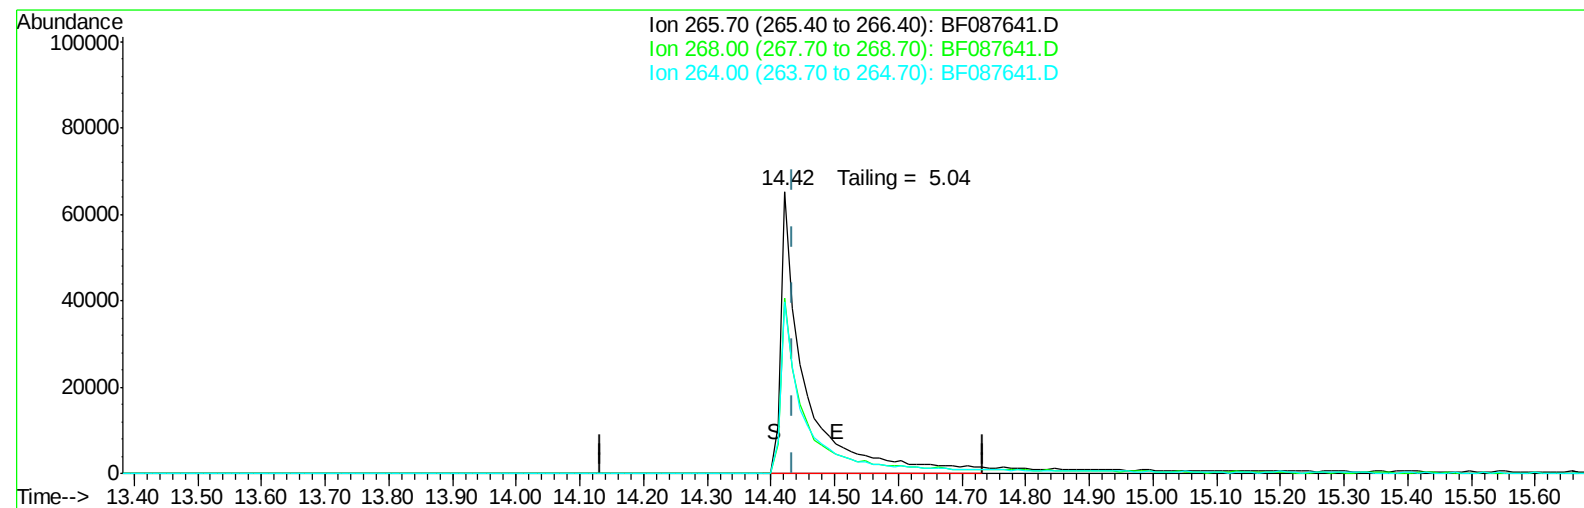

TIC: BF087641.D

(69) Pentachlorophenol (C)

14.423min (-0.011) 0.00ng

response 168156

Ion	Exp%	Act%
265.70	100	100
268.00	64.40	62.31
264.00	66.10	61.12
0.00	0.00	0.00