

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF060116\
 Data File : BF087640.D
 Acq On : 2 Jun 2016 4:20
 Operator : UM/SJ
 Sample : H3349-16
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 W-32

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF052316.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.370	328	331	354	rBV	145285	716893	33.42%	4.542%
2	7.027	474	476	480	rBV	150971	340851	15.89%	2.159%
3	7.084	480	481	501	rVB	743584	1876169	87.45%	11.886%
4	7.427	509	511	522	rBV	365857	704917	32.86%	4.466%
5	7.656	529	531	547	rVB	814702	1385615	64.59%	8.778%
6	8.342	589	591	617	rBV	399067	1264310	58.93%	8.010%
7	9.462	686	689	709	rBV	389290	913002	42.56%	5.784%
8	11.222	841	843	858	rBV	1531167	2145384	100.00%	13.592%
9	12.273	933	935	958	rBV	622532	940154	43.82%	5.956%
10	13.576	1047	1049	1068	rBV	632443	1280901	59.70%	8.115%
11	14.685	1144	1146	1163	rBV	512268	929196	43.31%	5.887%
12	17.040	1349	1352	1363	rBV	1558366	2070823	96.52%	13.119%
13	18.411	1470	1472	1487	rBV	342561	689081	32.12%	4.366%
14	20.091	1617	1619	1635	rBV	228048	527190	24.57%	3.340%


Sum of corrected areas: 15784486

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF060116\
Data File : BF087640.D
Acq On : 2 Jun 2016 4:20
Operator : UM/SJ
Sample : H3349-16
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
W-32

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF052316.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

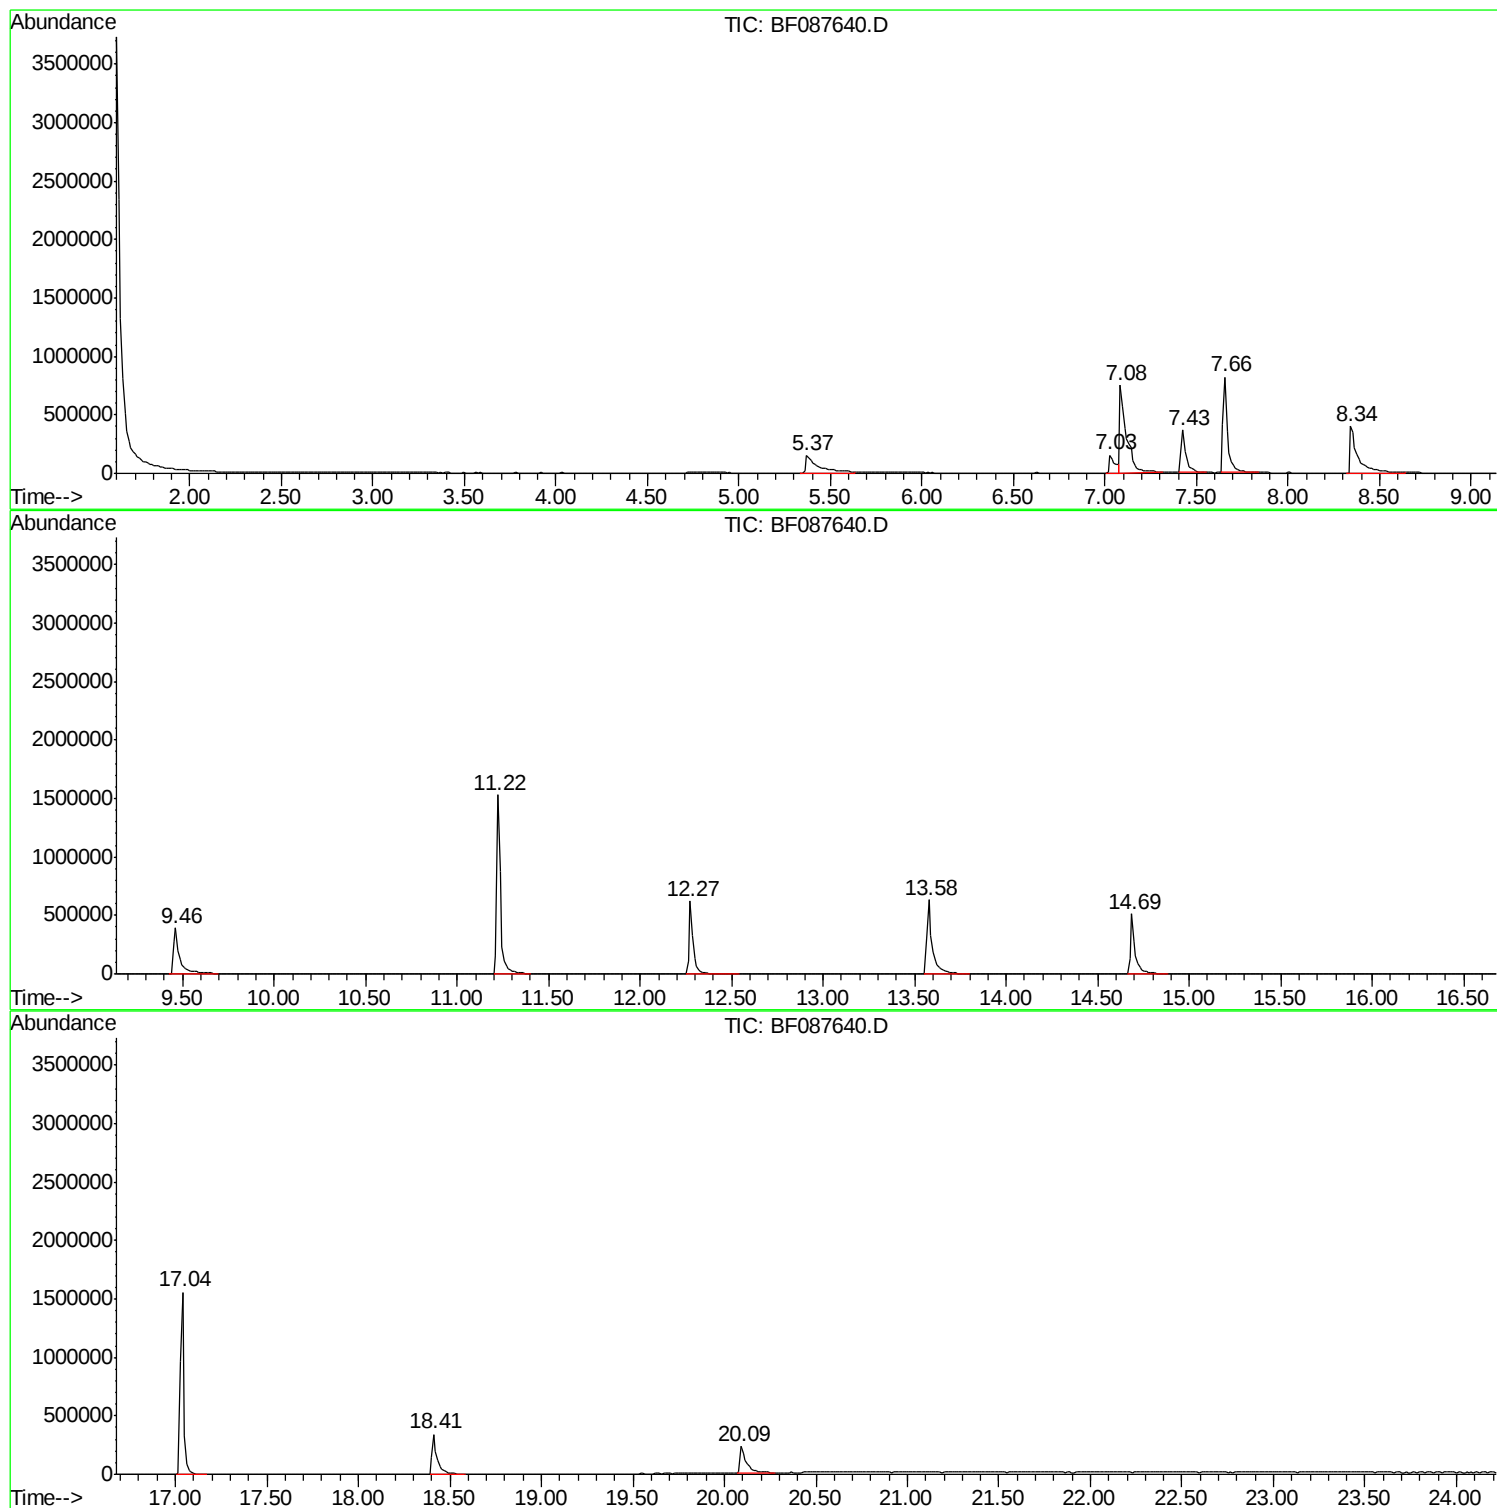

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF060116\
Data File : BF087640.D
Acq On : 2 Jun 2016 4:20
Operator : UM/SJ
Sample : H3349-16
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
W-32










Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF052316.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown7.08 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
7.08	53.23 ng	1876170	1,4-Dichlorobenzene-d4	7.43

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	27
2		Tranylcypromine-propionyl	189	C12H15NO	1000123-86-3	22
3		1H-Benzimidazole, 2-methyl-	132	C8H8N2	000615-15-6	22
4		5-Fluoro-2-chloropyrimidine	132	C4H2ClFN2	062802-42-0	12
5		Pyrazolo(2,3-a)pyridine, 7-methyl-	132	C8H8N2	034760-58-2	10

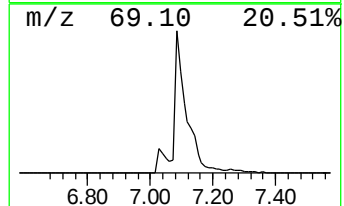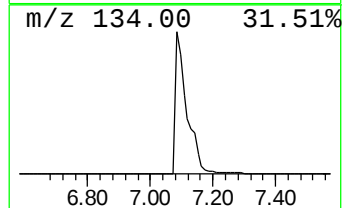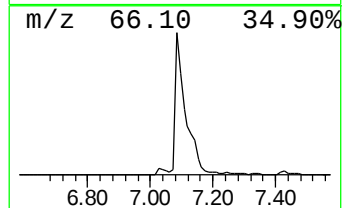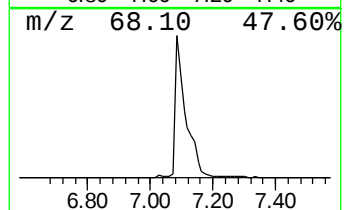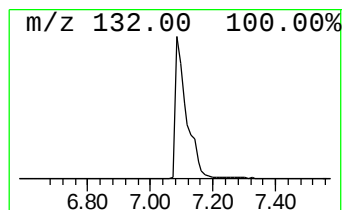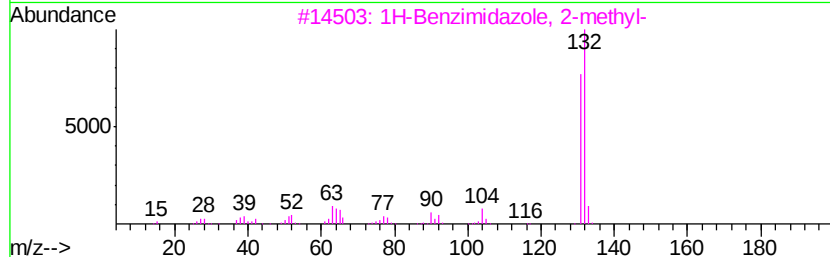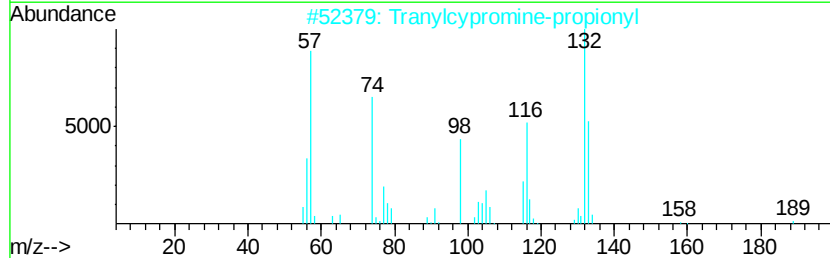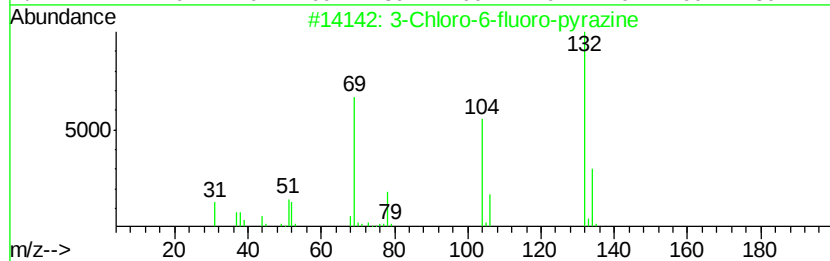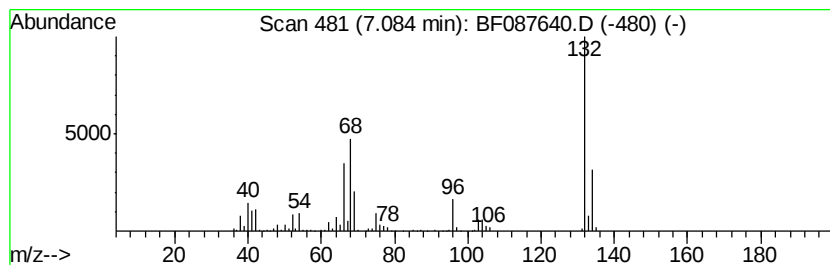

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF060116\
Data File : BF087640.D
Acq On : 2 Jun 2016 4:20
Operator : UM/SJ
Sample : H3349-16
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
W-32

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF052316.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown7.08	7.08	53.2	ng	1876170	1	7.43	704917	20.0