


Data Path : Z:\HPCHEM1\BNA F\DATA\BF060116\
 Data File : BF087641.D
 Acq On : 2 Jun 2016 5:57
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF052316.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed May 25 16:26:52 2016

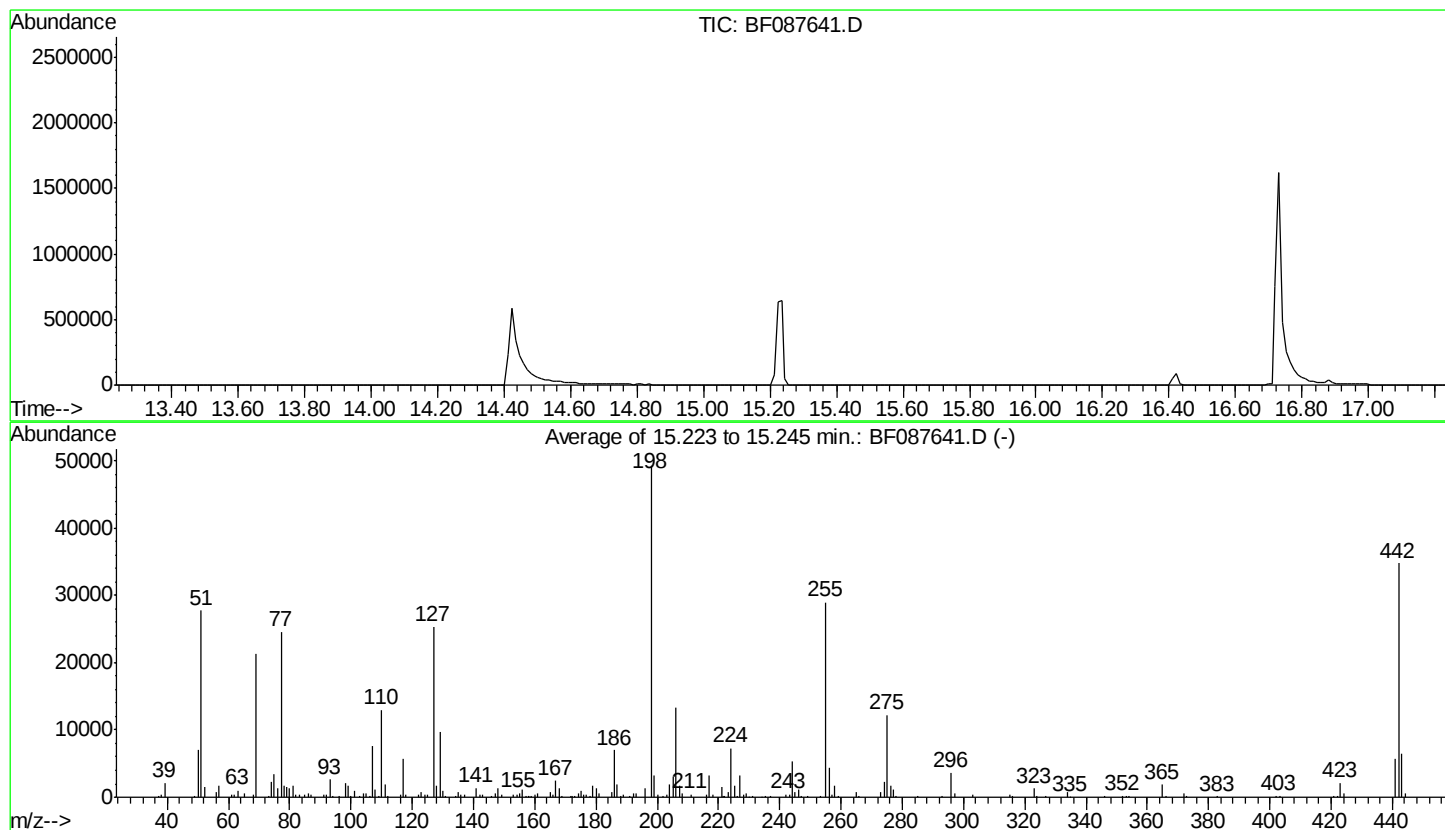

AutoFind: Scans 1193, 1194, 1195; Background Corrected with Scan 1189

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	56.3	27757	PASS
68	69	0.00	2	1.9	398	PASS
69	198	0.00	100	43.4	21397	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	51.4	25344	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	49264	PASS
199	198	5	9	6.5	3208	PASS
275	198	10	60	24.8	12220	PASS
365	198	1	100	3.8	1849	PASS
441	442	0.01	24	16.6	5782	PASS
442	198	50	100	70.5	34740	PASS
443	442	15	24	18.5	6423	PASS