
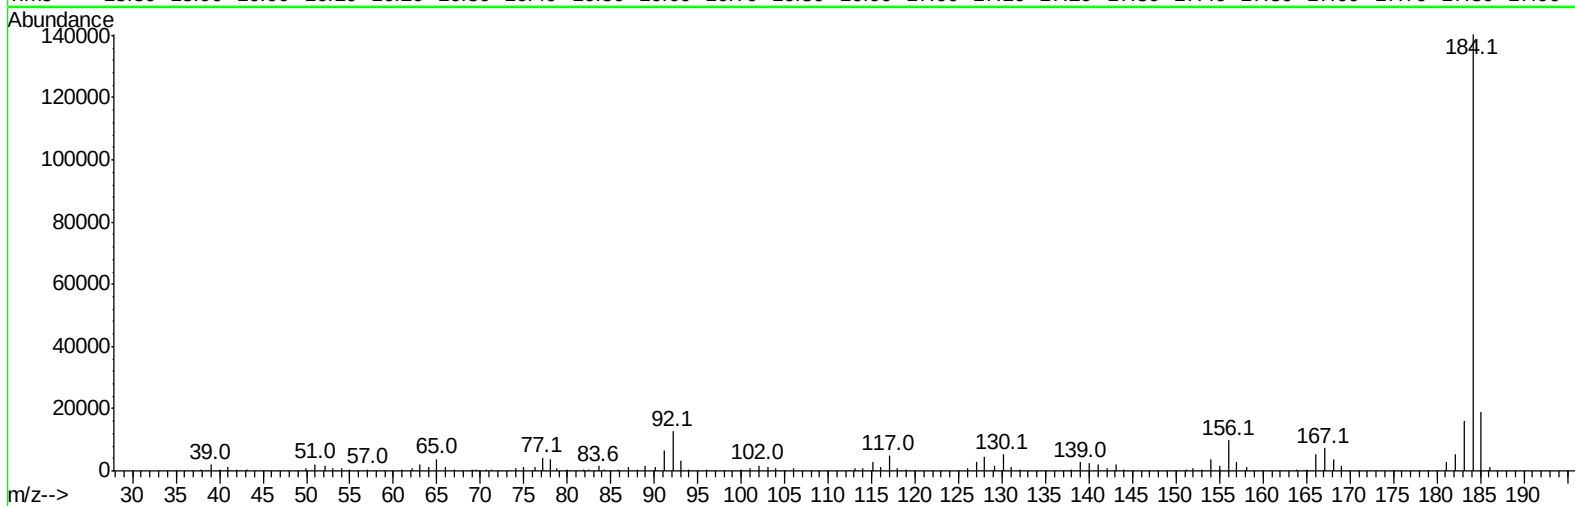


Data Path : Z:\HPCHEM1\BNA F\DATA\BF060117\
Data File : BF095592.D
Acq On : 1 Jun 2017 13:10
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 02 09:02:36 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF050217.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 01 18:51:16 2017
Response via : Initial Calibration

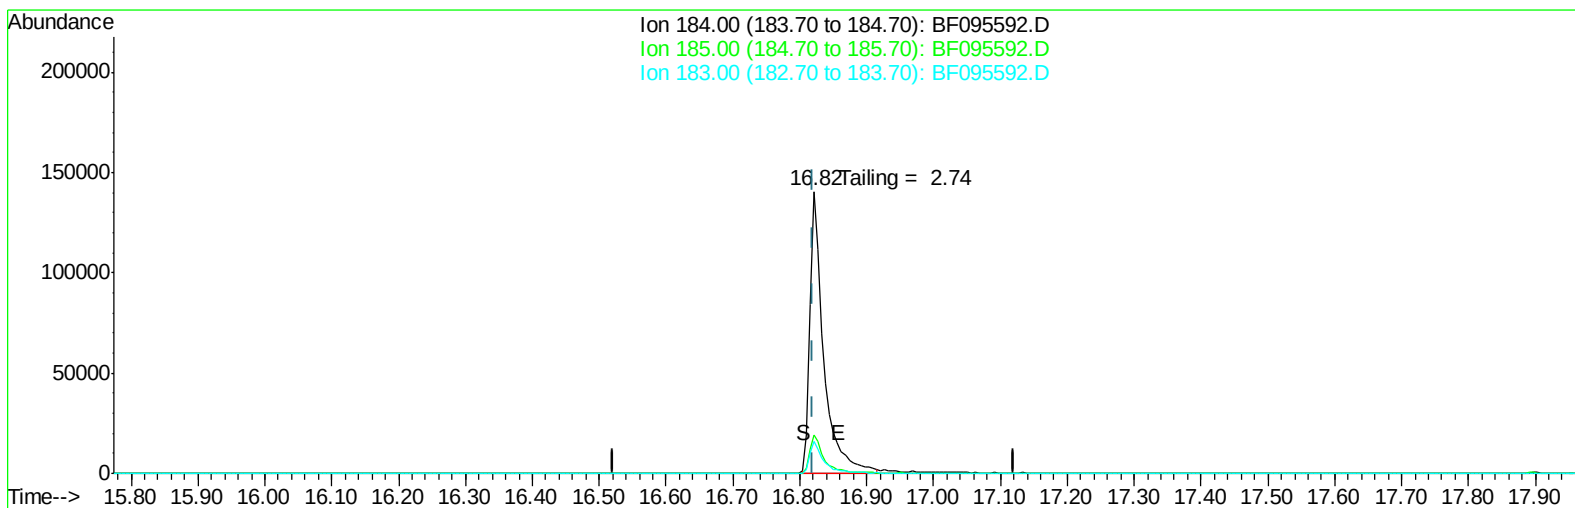

TIC: BF095592.D

(76) Benzidine




16.821min (-0.000) 0.00ng

response 210395

Ion	Exp%	Act%
184.00	100	100
185.00	19.40	13.50#
183.00	12.20	11.59
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\DATA\BF060117\
Data File : BF095592.D
Acq On : 1 Jun 2017 13:10
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 02 09:02:36 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF050217.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 01 18:51:16 2017
Response via : Initial Calibration

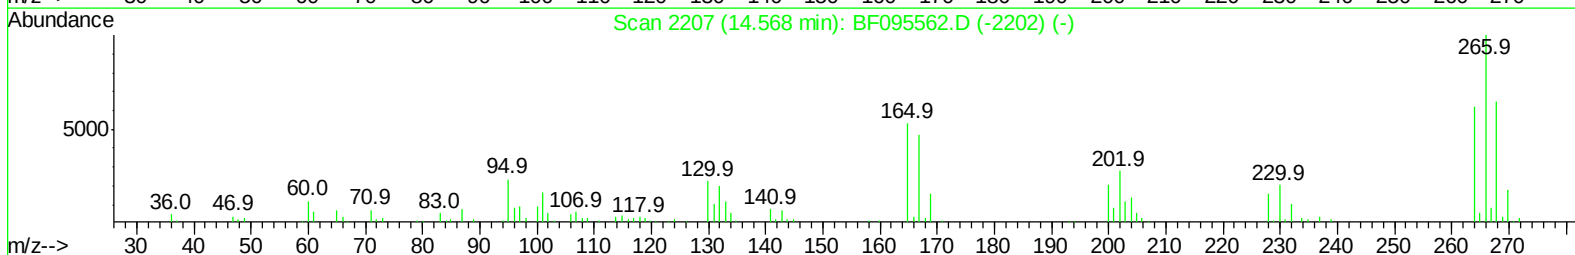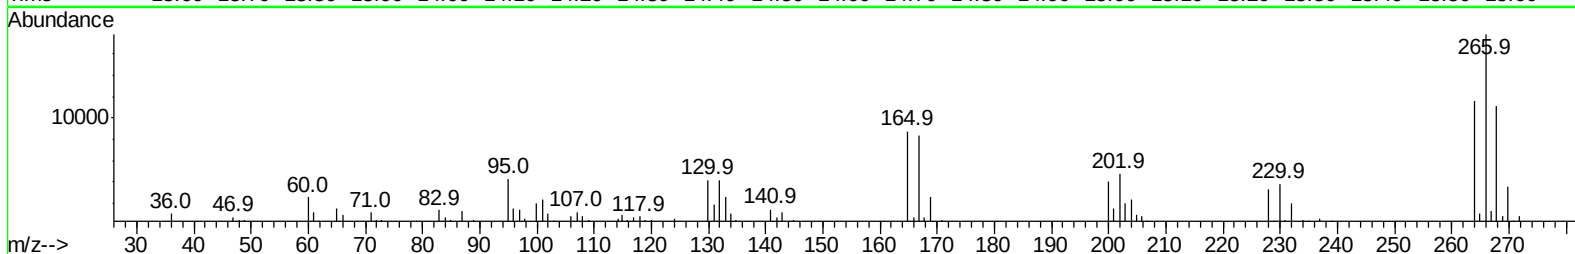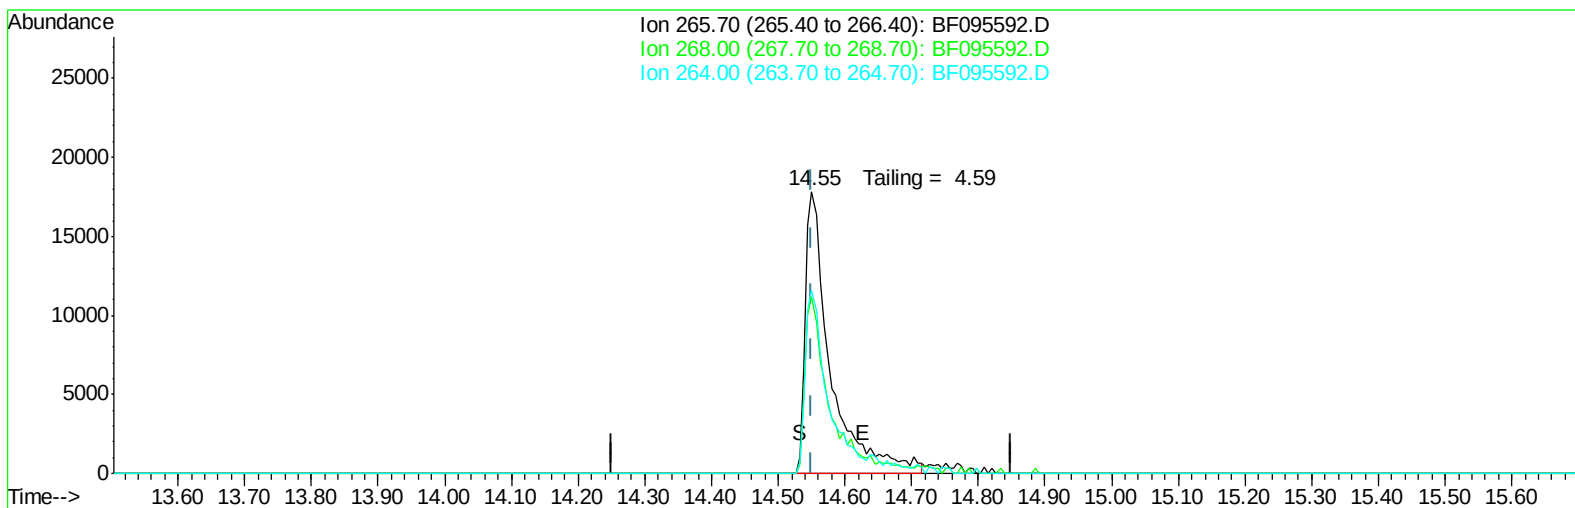

TIC: BF095592.D

(69) Pentachlorophenol (C)

14.551min (-0.000) 0.00ng

response 44847

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	62.52
264.00	64.60	65.19
0.00	0.00	0.00