
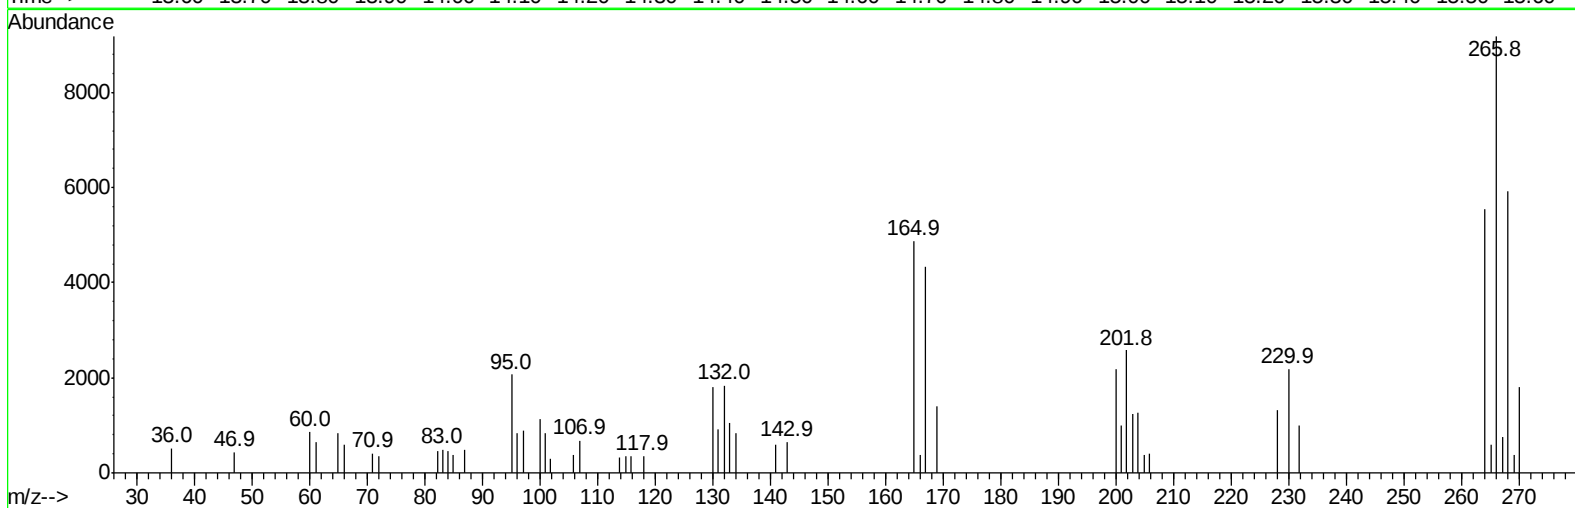


Data Path : Z:\HPCHEM1\BNA F\DATA\BF060117\
Data File : BF095611.D
Acq On : 2 Jun 2017 00:59
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 02 09:04:25 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF050217.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 01 18:51:16 2017
Response via : Initial Calibration

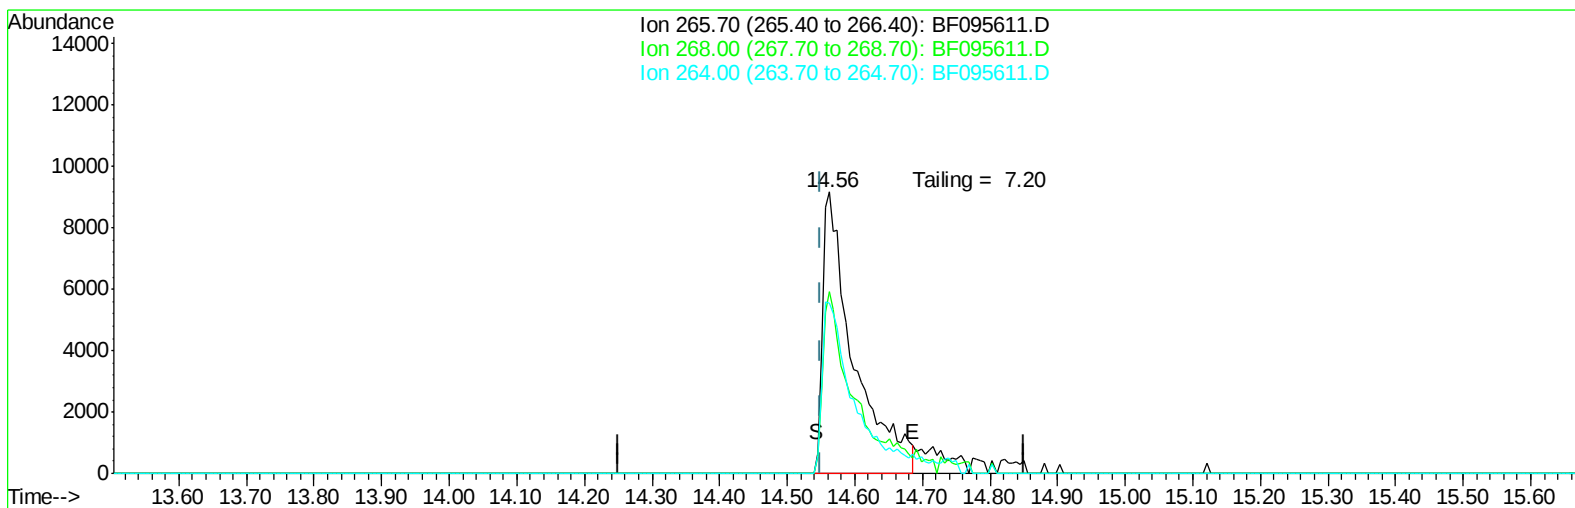

TIC: BF095611.D

(69) Pentachlorophenol (C)



14.562min (+0.012) 0.00ng

response 28048

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	64.55
264.00	64.60	60.54
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\DATA\BF060117\
Data File : BF095611.D
Acq On : 2 Jun 2017 00:59
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 02 09:04:25 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF050217.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 01 18:51:16 2017
Response via : Initial Calibration

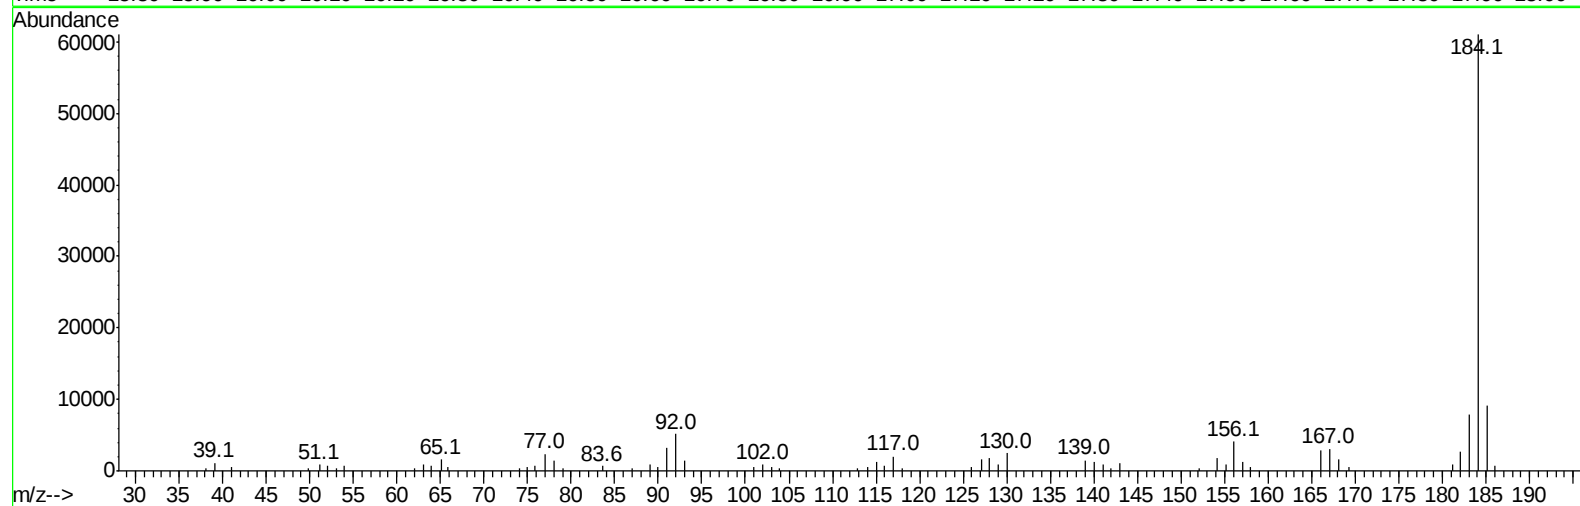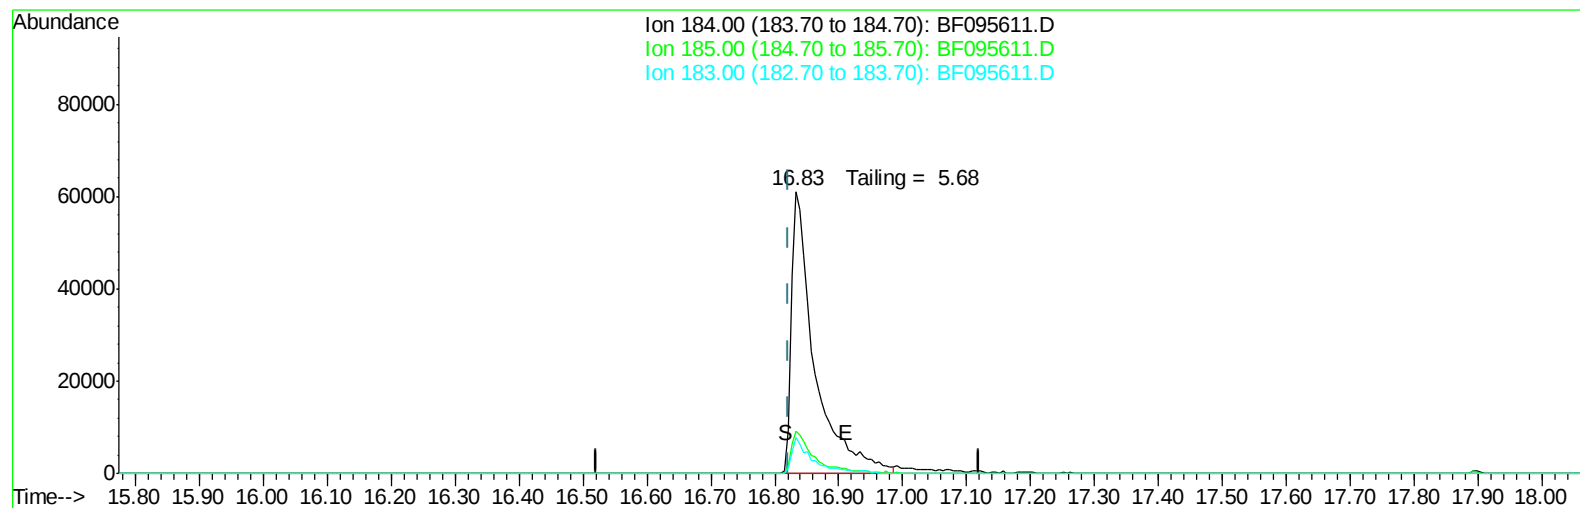

TIC: BF095611.D

(76) Benzidine

16.833min (+0.012) 10591.42ng

response 156950

Ion	Exp%	Act%
184.00	100	100
185.00	19.40	14.90#
183.00	12.20	12.97
0.00	0.00	0.00