

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF060117\
 Data File : BF095597.D
 Acq On : 1 Jun 2017 16:28
 Operator : SJ/MA
 Sample : I3379-01
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 S22-0022

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF050217.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.793	524	528	539	rBV2	19948	52792	1.81%	0.282%
2	5.457	638	641	672	rBV	365010	960066	32.86%	5.123%
3	7.104	917	921	932	rBV	204309	494689	16.93%	2.640%
4	7.192	932	936	955	rVB	1295520	2143001	73.34%	11.435%
5	7.534	990	994	1009	rVB	366240	508776	17.41%	2.715%
6	7.775	1029	1035	1050	rBV	1258513	1805623	61.79%	9.635%
7	8.451	1145	1150	1175	rBV	947622	1503692	51.46%	8.024%
8	9.569	1335	1340	1368	rBV	476218	709598	24.28%	3.787%
9	11.345	1635	1642	1663	rBV	2172707	2879758	98.55%	15.367%
10	12.045	1757	1761	1771	rBV	54294	80197	2.74%	0.428%
11	12.392	1815	1820	1832	rBV2	569509	791531	27.09%	4.224%
12	13.692	2036	2041	2064	rBV	1111568	1657832	56.74%	8.846%
13	14.798	2224	2229	2242	rBV	561876	820705	28.09%	4.379%
14	17.151	2623	2629	2632	rBV	2346579	2922060	100.00%	15.593%
15	18.386	2835	2839	2849	rVB3	40055	62887	2.15%	0.336%
16	18.492	2853	2857	2873	rVV	555891	781266	26.74%	4.169%
17	20.168	3137	3142	3153	rBV	372997	565602	19.36%	3.018%


Sum of corrected areas: 18740075

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF060117\
Data File : BF095597.D
Acq On : 1 Jun 2017 16:28
Operator : SJ/MA
Sample : I3379-01
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
S22-0022

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF050217.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

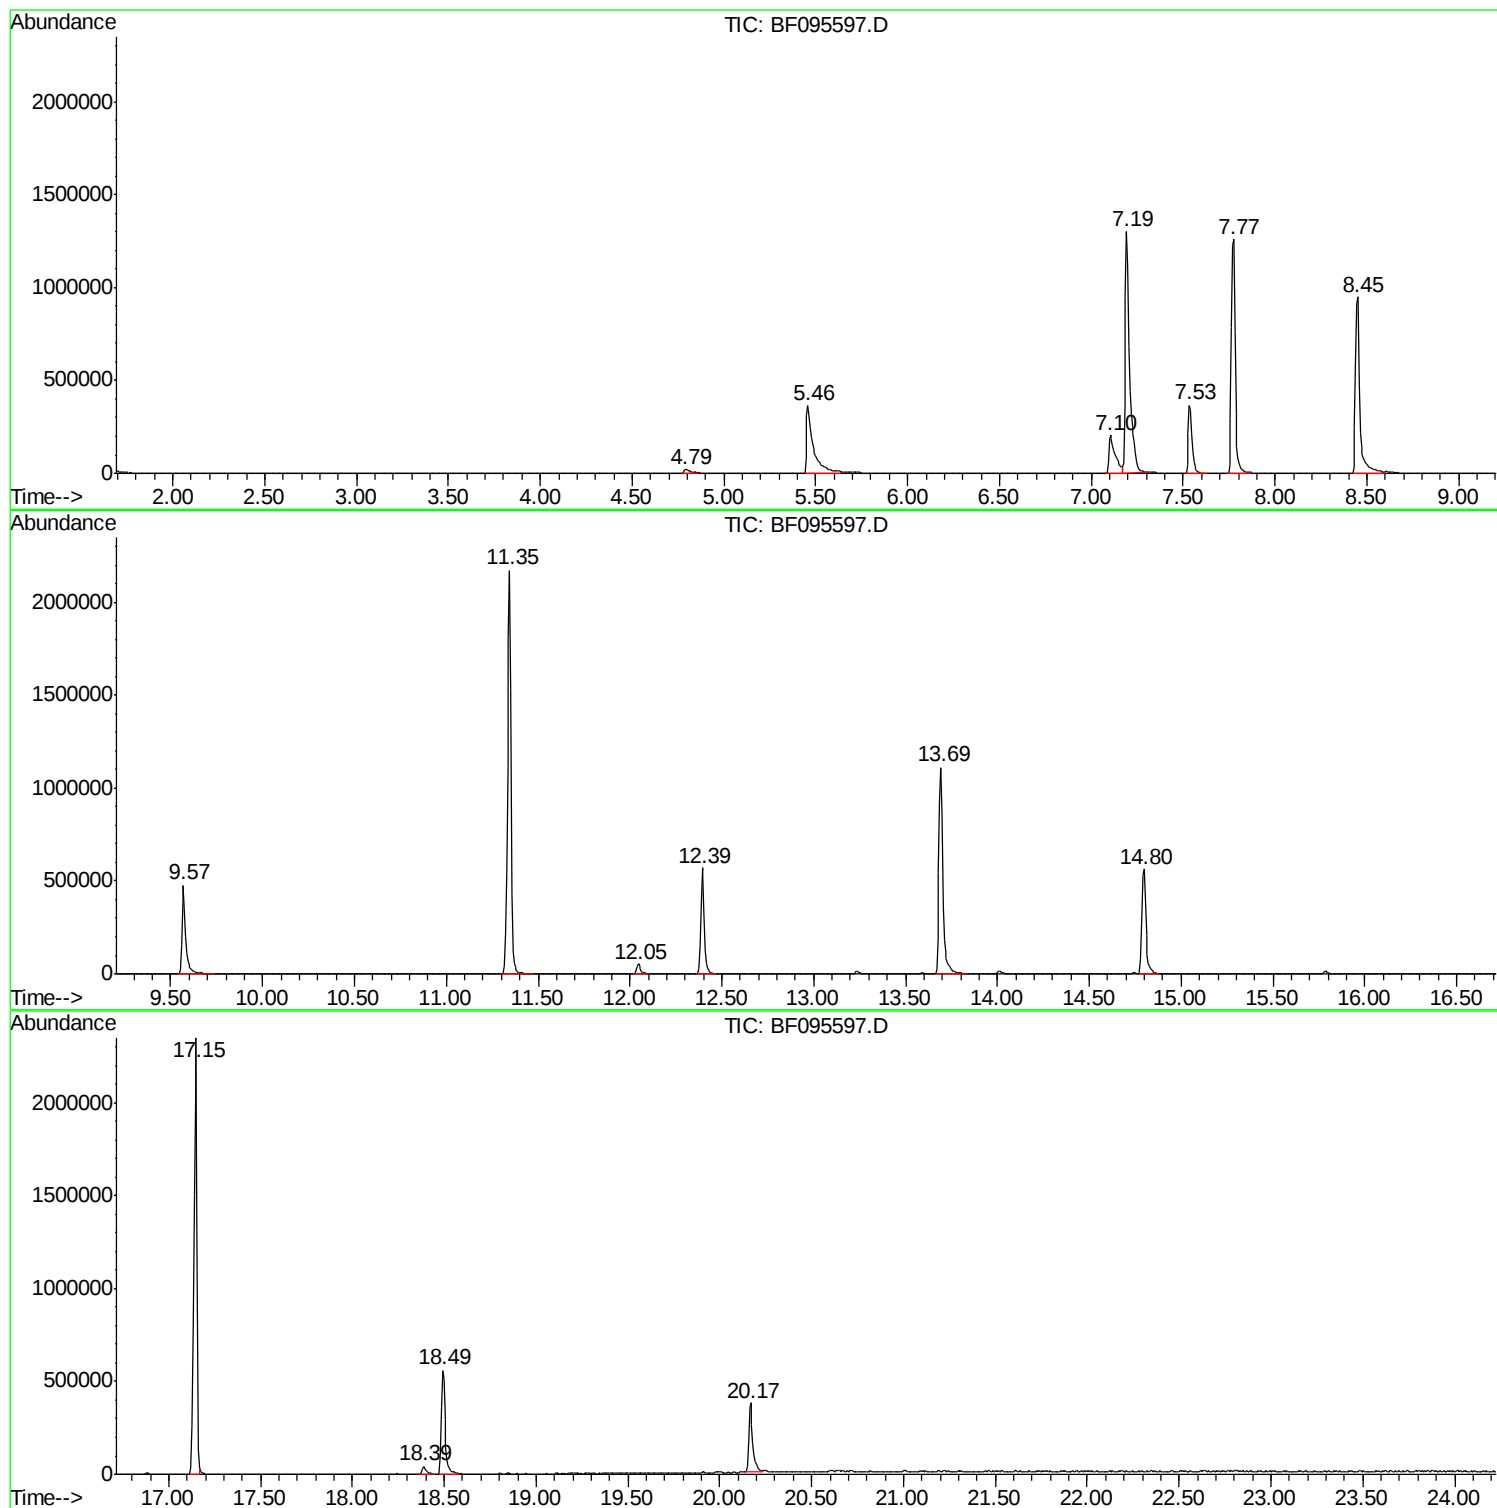

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF060117\
Data File : BF095597.D
Acq On : 1 Jun 2017 16:28
Operator : SJ/MA
Sample : I3379-01
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
S22-0022










Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF050217.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown4.79 Concentration Rank 3

R.T.	EstConc	Area	Relative to ISTD	R.T.
4.79	2.08 ng	52792	1,4-Dichlorobenzene-d4	7.53

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			3-Hexanol	102	C6H14O	000623-37-0	9
2			Propylamine	59	C3H9N	000107-10-8	5
3			Morpholine, 4-methyl-	101	C5H11NO	000109-02-4	5
4			Acetone	58	C3H6O	000067-64-1	4
5			2,3-Butanedione, monooxime	101	C4H7NO2	000057-71-6	4

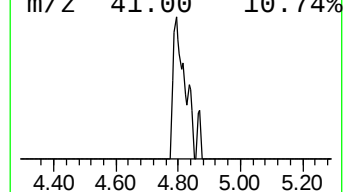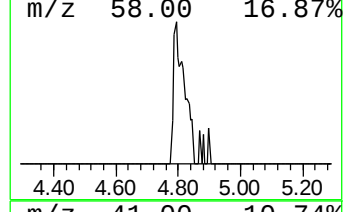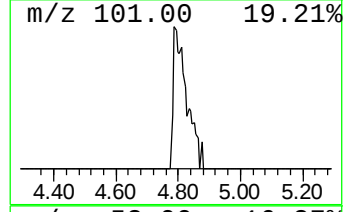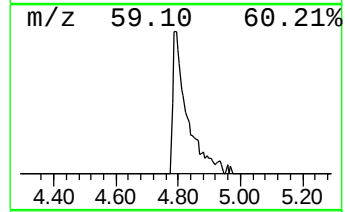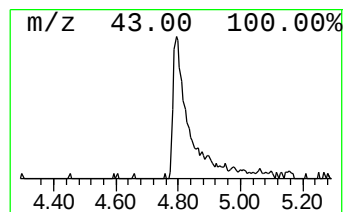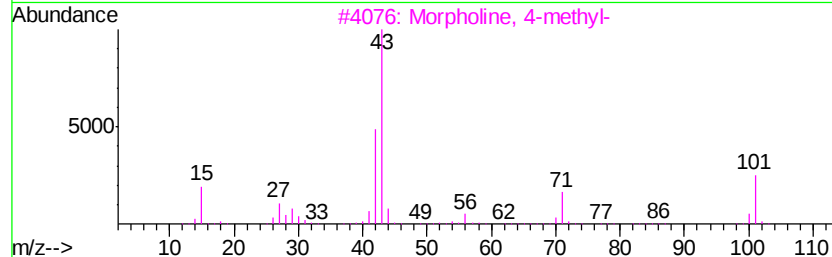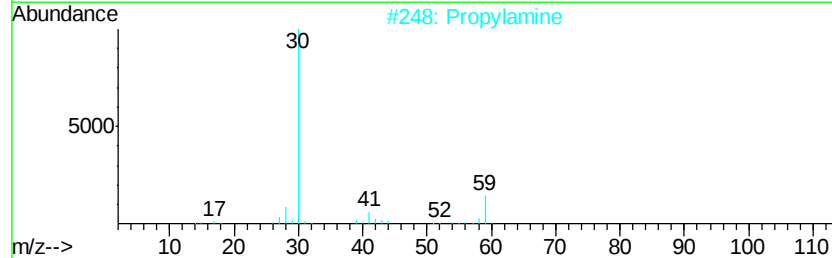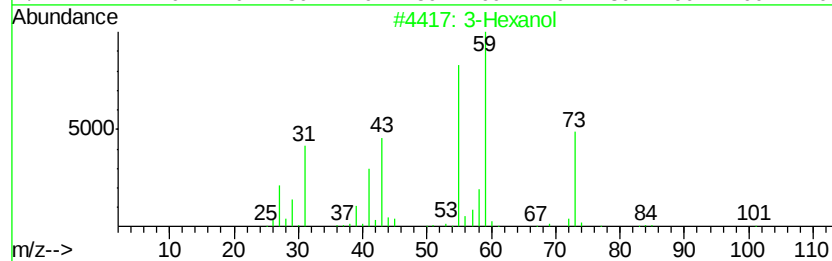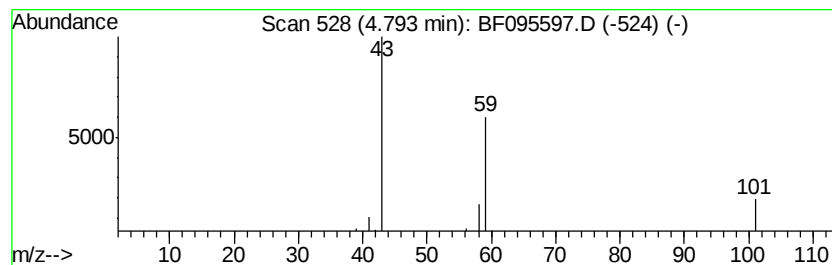

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF060117\
Data File : BF095597.D
Acq On : 1 Jun 2017 16:28
Operator : SJ/MA
Sample : I3379-01
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
S22-0022










Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF050217.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 unknown7.19 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
7.19	84.24 ng	2143000	1,4-Dichlorobenzene-d4	7.53

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	38
2		(E)-3-Chloro-2-methyl-2-pentenal	132	C6H9ClO	031357-76-3	35
3		Tranylcypromine-propionyl	189	C12H15NO	1000123-86-3	12
4		1H-Indazole, 7-methyl-	132	C8H8N2	1000316-00-7	10
5		2H-Cyclopenta[d]pyridazine, 2-me...	132	C8H8N2	022291-85-6	9

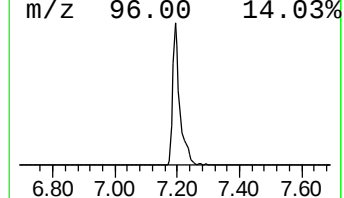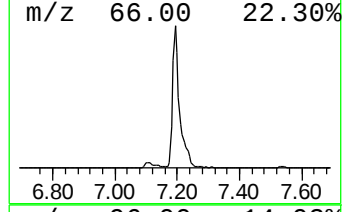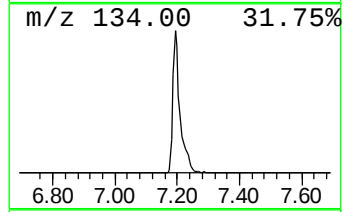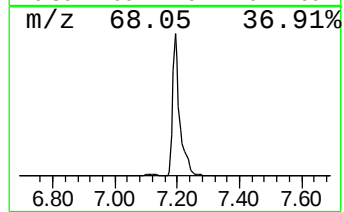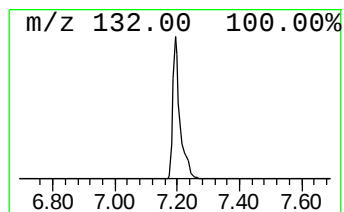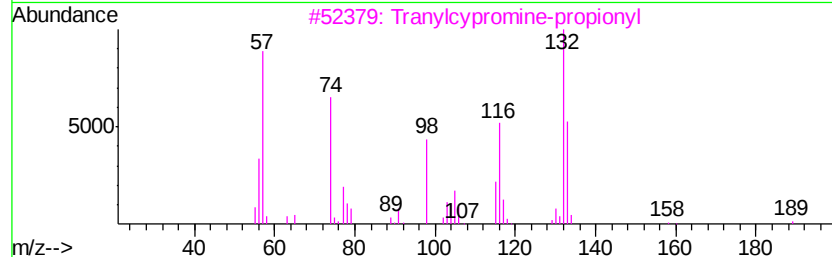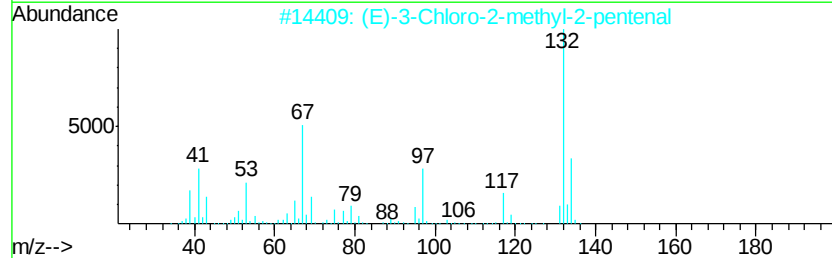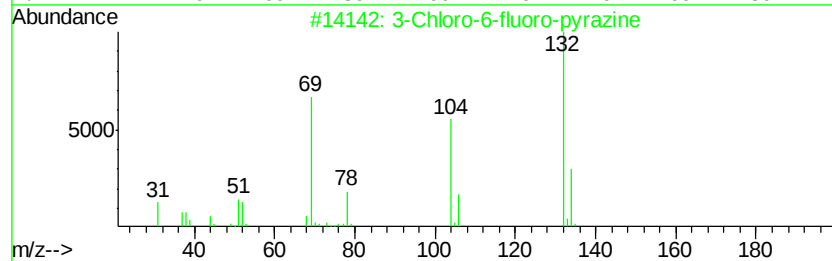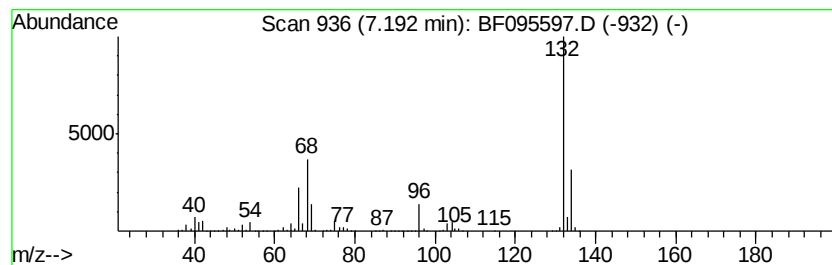

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF060117\
Data File : BF095597.D
Acq On : 1 Jun 2017 16:28
Operator : SJ/MA
Sample : I3379-01
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
S22-0022

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF050217.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown4.79	4.79	2.1	ng	52792	1	7.53	508776	20.0
unknown7.19	7.19	84.2	ng	2143000	1	7.53	508776	20.0