

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF060117\
 Data File : BF095604.D
 Acq On : 1 Jun 2017 20:12
 Operator : SJ/MA
 Sample : I3384-01
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 MW-1

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF050217.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.775	522	525	539	rBV	43418	110321	4.24%	0.763%
2	5.475	641	644	671	rBV	127320	413459	15.89%	2.859%
3	7.122	921	924	933	rBV	88501	218787	8.41%	1.513%
4	7.198	933	937	957	rVB	578871	1145814	44.03%	7.923%
5	7.534	991	994	1007	rBV	305480	428833	16.48%	2.965%
6	7.775	1030	1035	1057	rBV	1183473	1622631	62.36%	11.220%
7	8.451	1145	1150	1182	rBV	828250	1289619	49.56%	8.917%
8	9.569	1336	1340	1361	rBV	388364	589719	22.66%	4.078%
9	11.345	1636	1642	1655	rBV	1961078	2599927	99.92%	17.978%
10	12.051	1758	1762	1773	rBV	21560	37290	1.43%	0.258%
11	12.392	1816	1820	1835	rBV2	501236	683027	26.25%	4.723%
12	13.692	2036	2041	2059	rBV	529458	821133	31.56%	5.678%
13	14.798	2224	2229	2241	rBV	475447	693124	26.64%	4.793%
14	17.151	2623	2629	2632	rBV	2157887	2602104	100.00%	17.993%
15	18.386	2836	2839	2850	rVB4	37191	56075	2.15%	0.388%
16	18.498	2853	2858	2872	rBV	472065	672593	25.85%	4.651%
17	20.168	3138	3142	3154	rBV	316927	477487	18.35%	3.302%


Sum of corrected areas: 14461943

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF060117\
Data File : BF095604.D
Acq On : 1 Jun 2017 20:12
Operator : SJ/MA
Sample : I3384-01
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
MW-1

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF050217.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

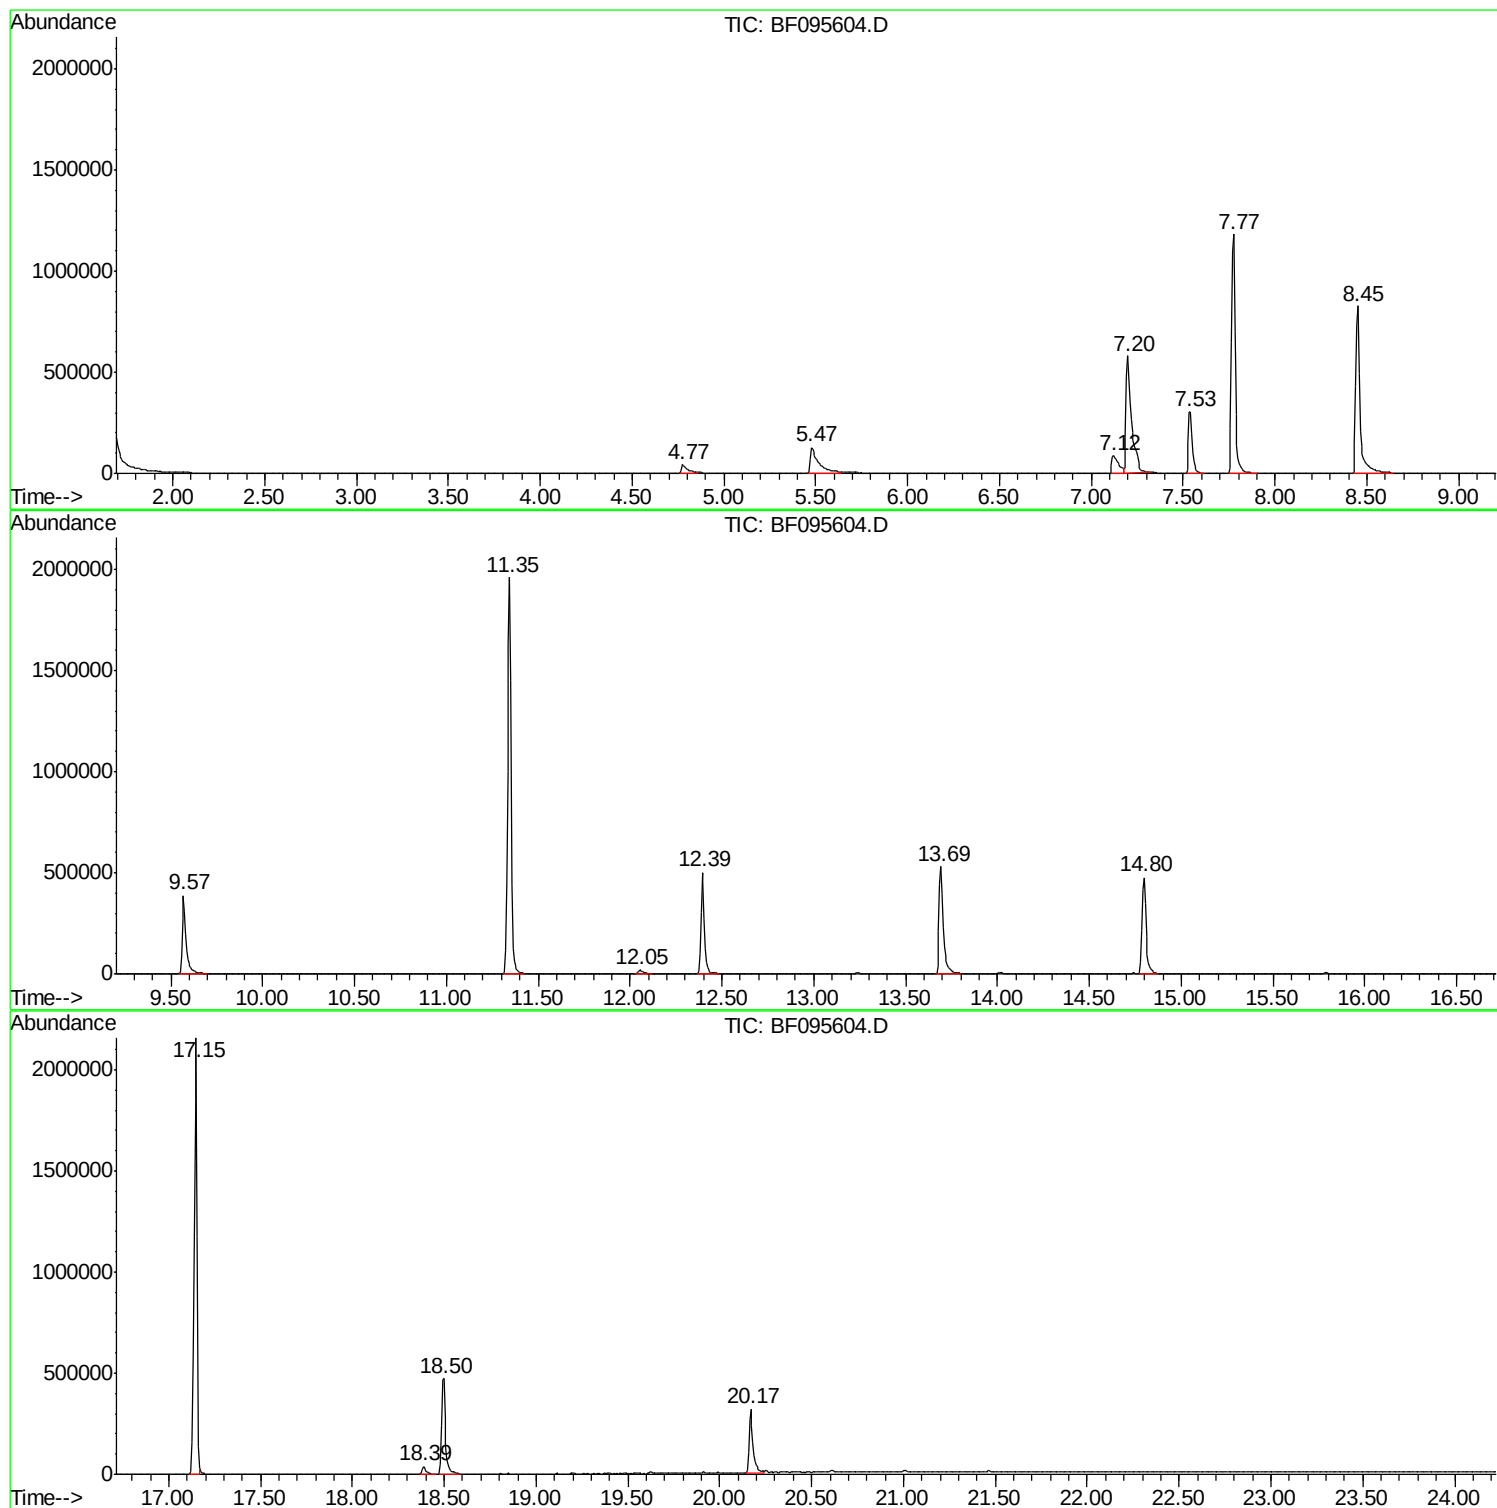

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF060117\
Data File : BF095604.D
Acq On : 1 Jun 2017 20:12
Operator : SJ/MA
Sample : I3384-01
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
MW-1










Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF050217.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 2-Pentanone, 4-hydroxy-4-me... Concentration Rank 3

R.T.	EstConc	Area	Relative to ISTD	R.T.
4.77	5.15 ng	110321	1,4-Dichlorobenzene-d4	7.54

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	42
2			Acetic acid, 1,1-dimethylethyl e...	116	C6H12O2	000540-88-5	39
3			Propane, 2-ethoxy-2-methyl-	102	C6H14O	000637-92-3	9
4			3-Hexanol, 4-methyl-	116	C7H16O	000615-29-2	9
5			3-Octanol	130	C8H18O	000589-98-0	9

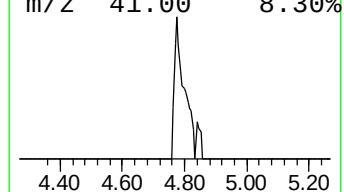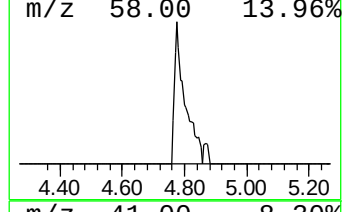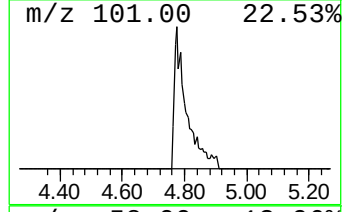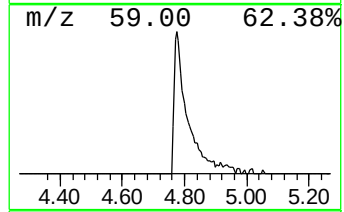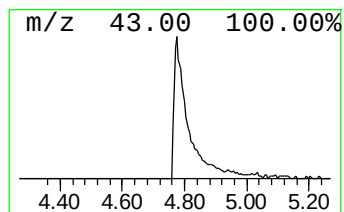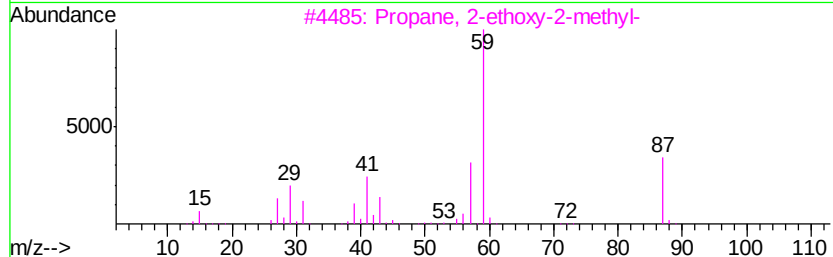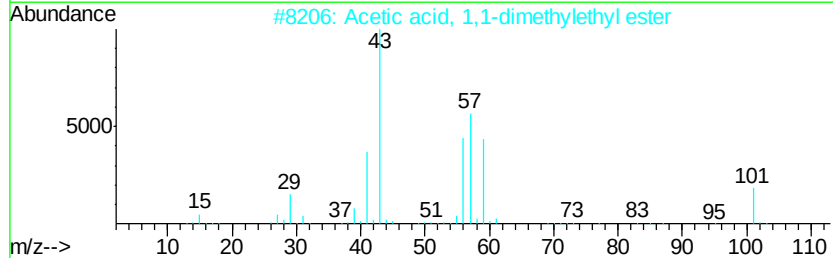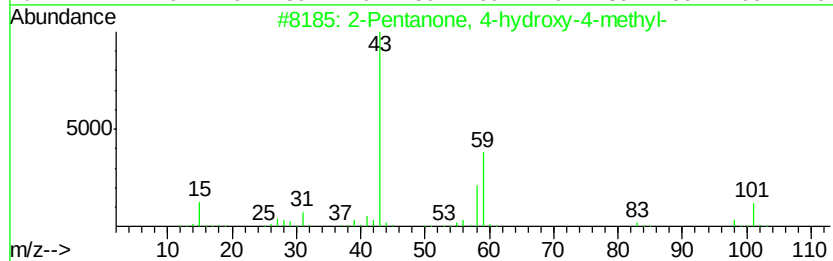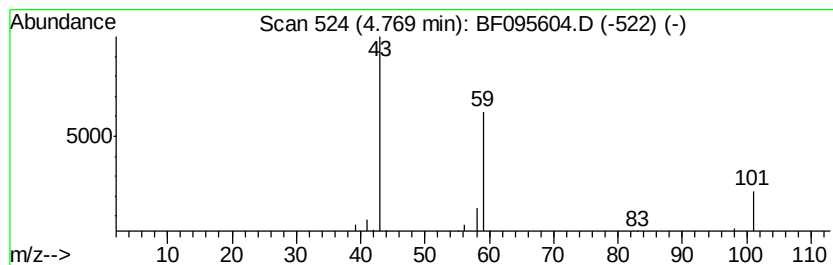

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF060117\
Data File : BF095604.D
Acq On : 1 Jun 2017 20:12
Operator : SJ/MA
Sample : I3384-01
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
MW-1










Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF050217.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 unknown7.20 Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
7.20	53.44 ng	1145810	1,4-Dichlorobenzene-d4	7.54

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	38
2		(E)-3-Chloro-2-methyl-2-pentenal	132	C6H9ClO	031357-76-3	25
3		Tranylcypromine-propionyl	189	C12H15NO	1000123-86-3	12
4		1H-Indazole, 7-methyl-	132	C8H8N2	1000316-00-7	10
5		4-Chloro-6-fluoro-pyrimidine	132	C4H2ClFN2	051422-01-6	9

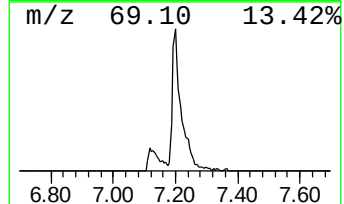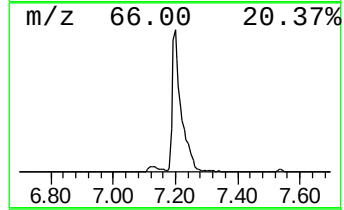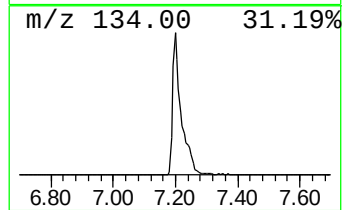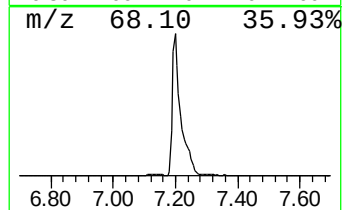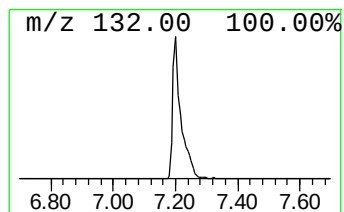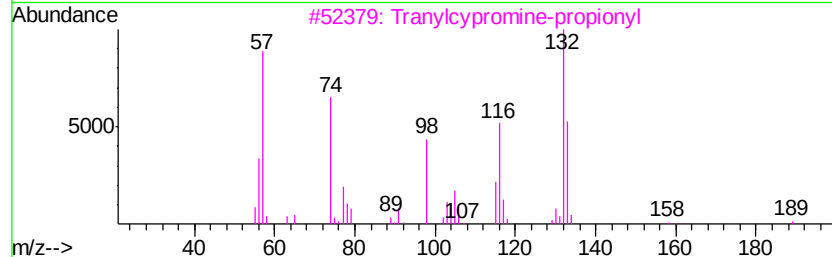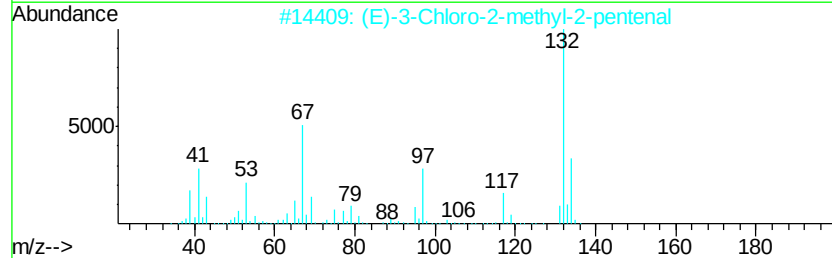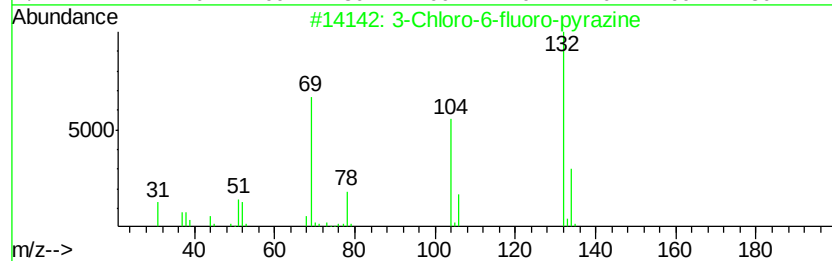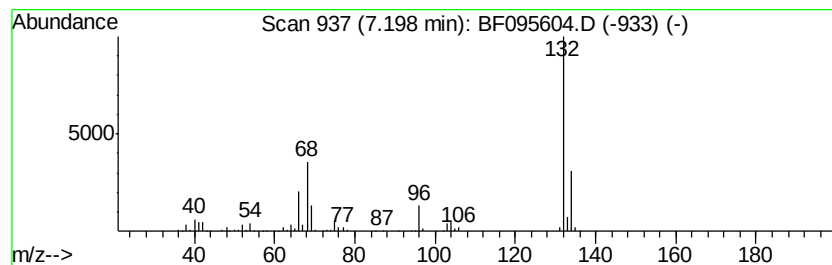

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF060117\
Data File : BF095604.D
Acq On : 1 Jun 2017 20:12
Operator : SJ/MA
Sample : I3384-01
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
MW-1

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF050217.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
2-Pentanone, 4-hy...	4.77	5.2	ng	110321	1	7.54	428833	20.0
unknown7.20	7.20	53.4	ng	1145810	1	7.54	428833	20.0