

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF060117\
Data File : BF095607.D
Acq On : 1 Jun 2017 21:48
Operator : SJ/MA
Sample : I3384-02
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
MW-2

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF050217.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.798	525	529	543	rBV	20944	58123	2.04%	0.333%
2	5.457	638	641	676	rBV	362040	967556	34.03%	5.547%
3	7.098	917	920	932	rBV	218053	508113	17.87%	2.913%
4	7.192	932	936	951	rVB	1270177	2031521	71.46%	11.646%
5	7.539	991	995	1010	rVB	296174	420837	14.80%	2.413%
6	7.775	1030	1035	1055	rBV	1264143	1752019	61.63%	10.044%
7	8.451	1145	1150	1174	rBV	945684	1387132	48.79%	7.952%
8	9.569	1336	1340	1361	rBV	373518	588109	20.69%	3.372%
9	11.345	1636	1642	1659	rBV	2077823	2842869	100.00%	16.298%
10	12.392	1816	1820	1834	rBV2	481572	684158	24.07%	3.922%
11	13.692	2036	2041	2064	rBV	1075190	1617367	56.89%	9.272%
12	14.798	2224	2229	2253	rBV	429185	689736	24.26%	3.954%
13	17.151	2623	2629	2632	rBV	2170278	2723483	95.80%	15.613%
14	18.498	2853	2858	2875	rBV	406133	637931	22.44%	3.657%
15	20.168	3138	3142	3153	rBV	284683	436030	15.34%	2.500%
16	20.250	3153	3156	3162	rVB	28985	35459	1.25%	0.203%
17	20.603	3210	3216	3222	rBV	21216	33898	1.19%	0.194%
18	21.009	3280	3285	3289	rBV2	19264	29137	1.02%	0.167%


Sum of corrected areas: 17443478

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF060117\
Data File : BF095607.D
Acq On : 1 Jun 2017 21:48
Operator : SJ/MA
Sample : I3384-02
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
MW-2

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF050217.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

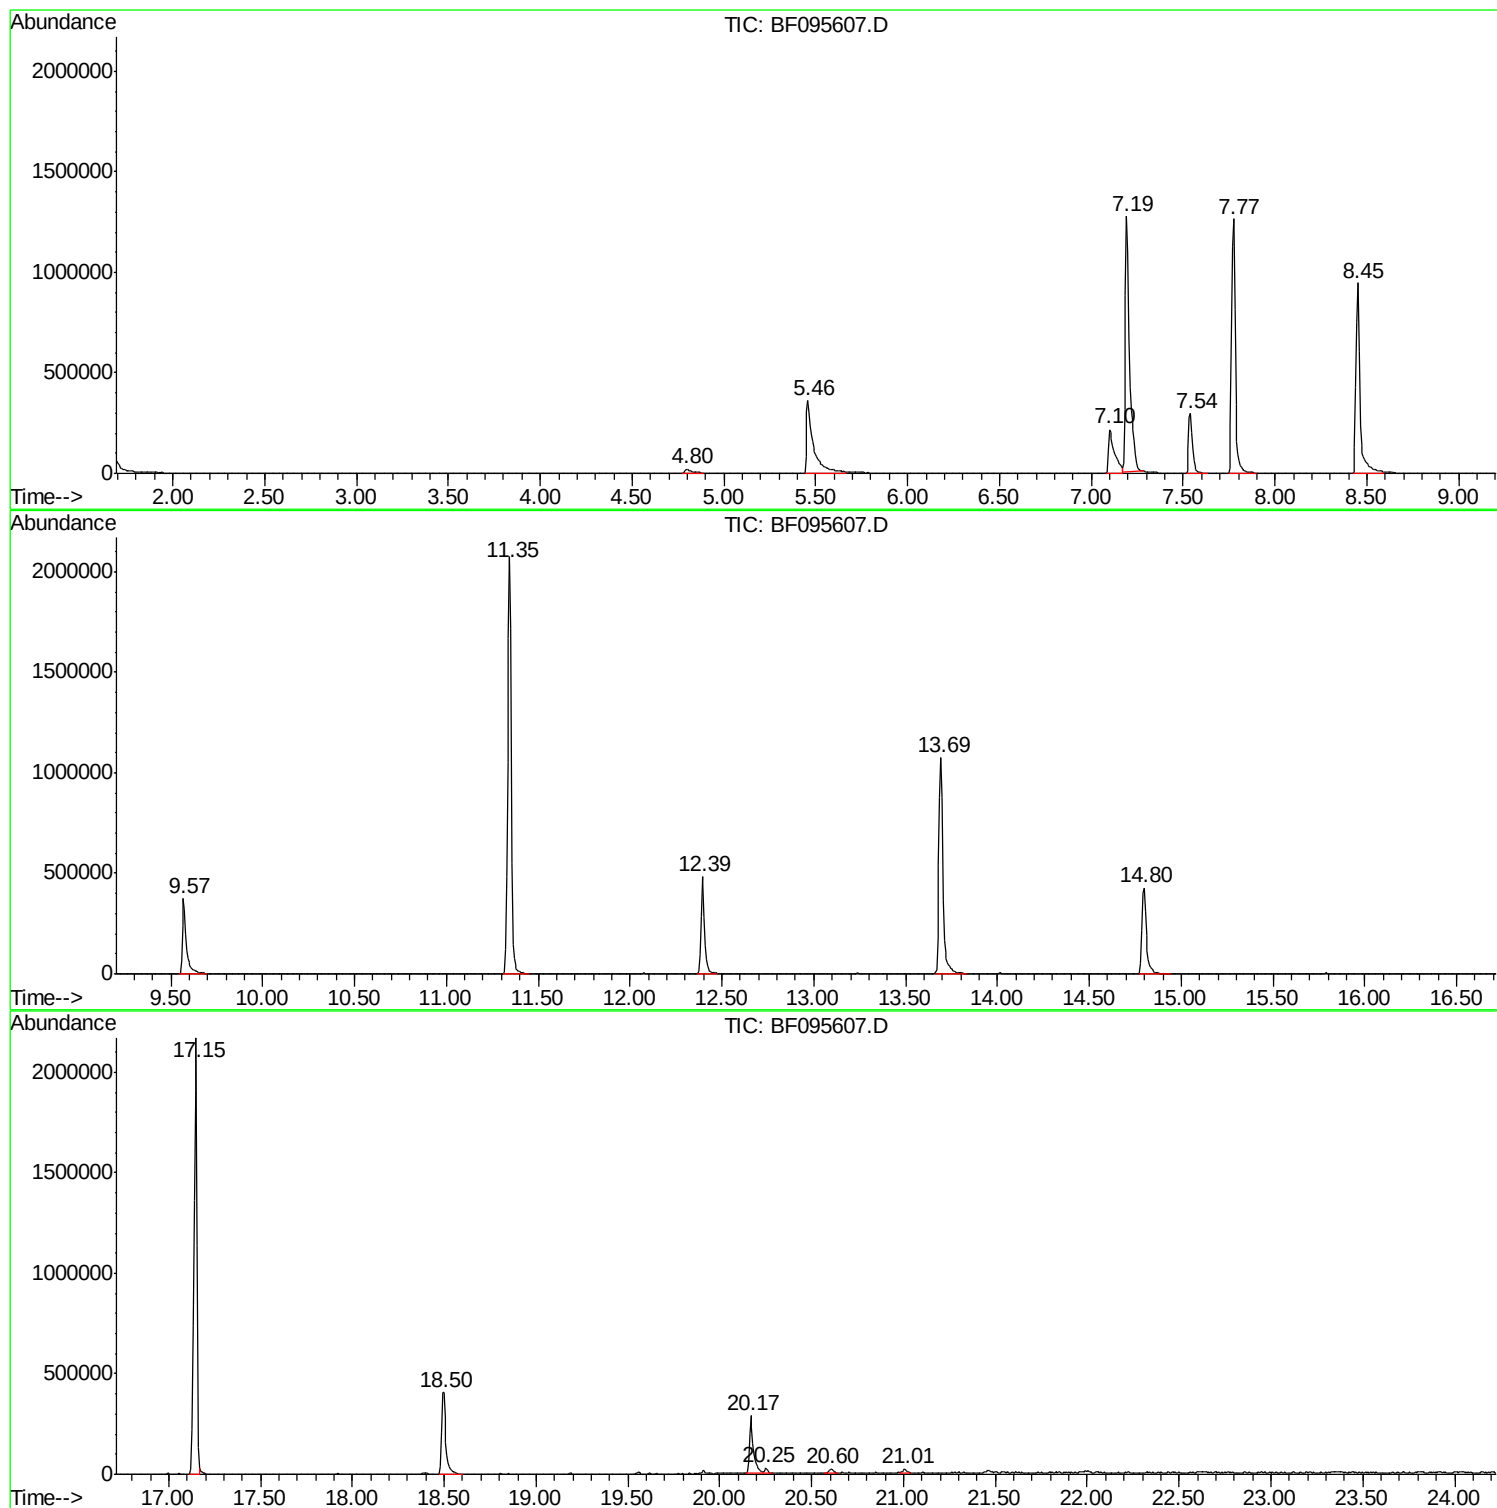

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF060117\
Data File : BF095607.D
Acq On : 1 Jun 2017 21:48
Operator : SJ/MA
Sample : I3384-02
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
MW-2










Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF050217.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Oxirane, [(1-methylethoxy)m... Concentration Rank 3

R.T.	EstConc	Area	Relative to ISTD	R.T.
4.80	2.76 ng	58123	1,4-Dichlorobenzene-d4	7.54

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	Oxirane, [(1-methylethoxy)methyl]-	116	C6H12O2	004016-14-2	64
2		5-Hexen-2-one	98	C6H10O	000109-49-9	5
3		Morpholine, 4-methyl-	101	C5H11NO	000109-02-4	5
4		Acetone	58	C3H6O	000067-64-1	5
5		Guanidine	59	CH5N3	000113-00-8	4

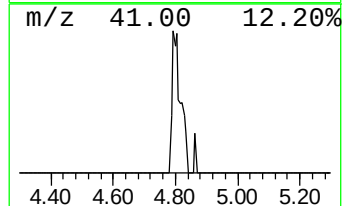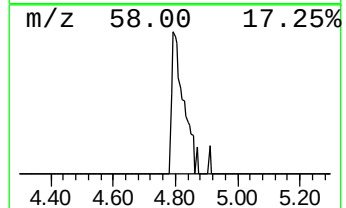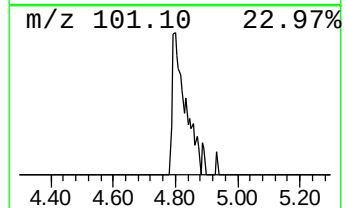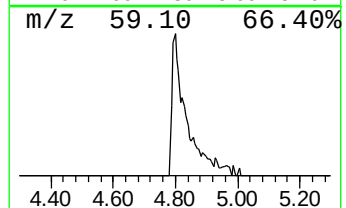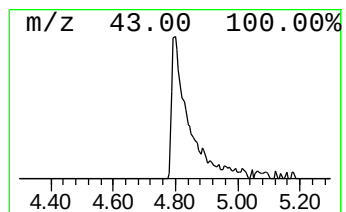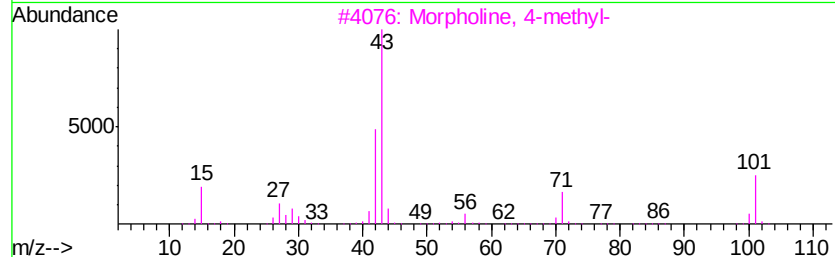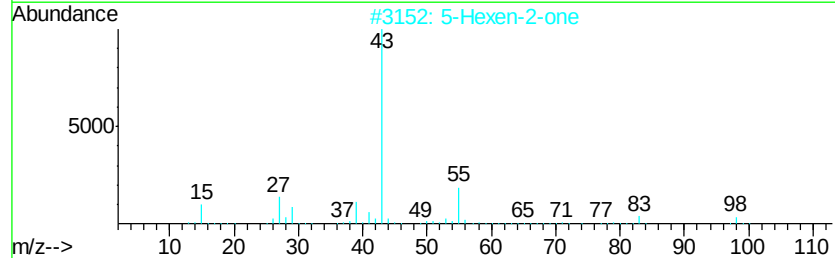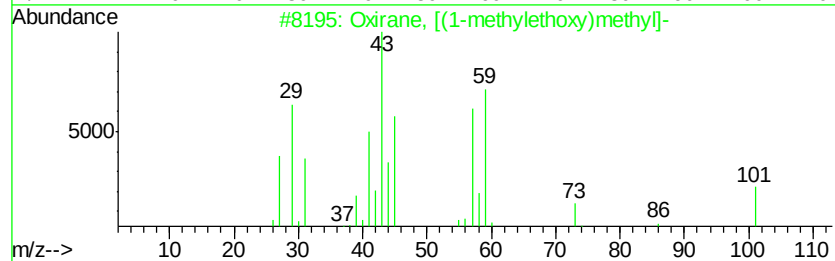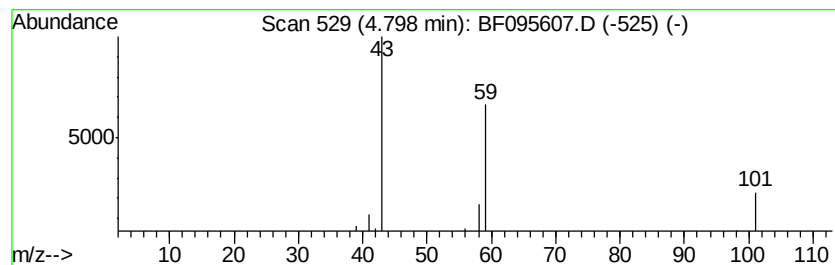

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF060117\
Data File : BF095607.D
Acq On : 1 Jun 2017 21:48
Operator : SJ/MA
Sample : I3384-02
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
MW-2










Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF050217.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 unknown7.19 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
7.19	96.55 ng	2031520	1,4-Dichlorobenzene-d4	7.54

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	(E)-3-Chloro-2-methyl-2-pentenal	132	C6H9ClO	031357-76-3	35
2		3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	25
3		5-Aminoindole	132	C8H8N2	005192-03-0	12
4		1H-Benzimidazole, 2-methyl-	132	C8H8N2	000615-15-6	10
5		5-Fluoro-2-chloropyrimidine	132	C4H2ClFN2	062802-42-0	9

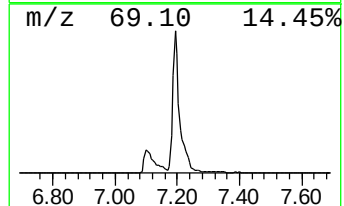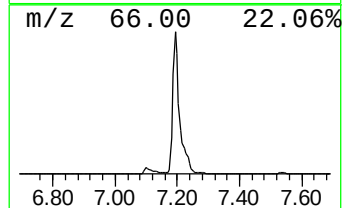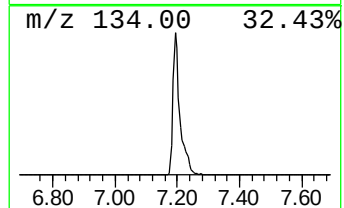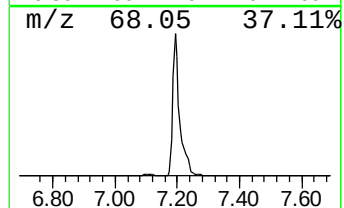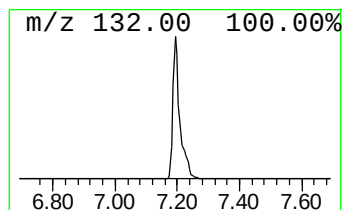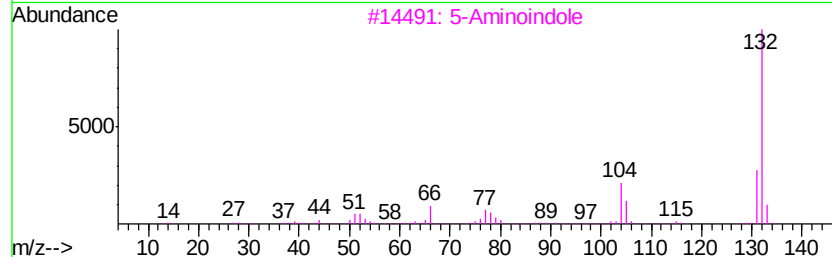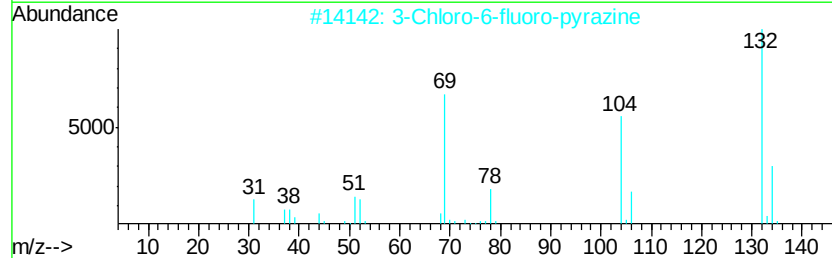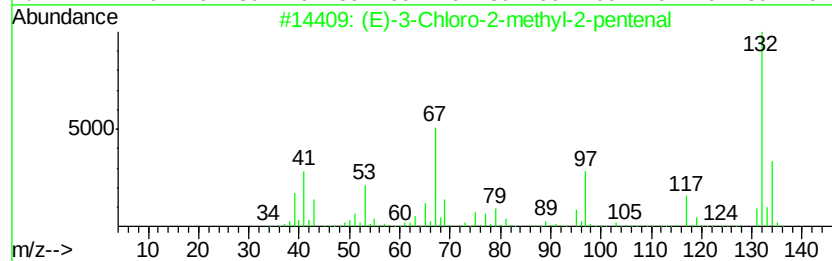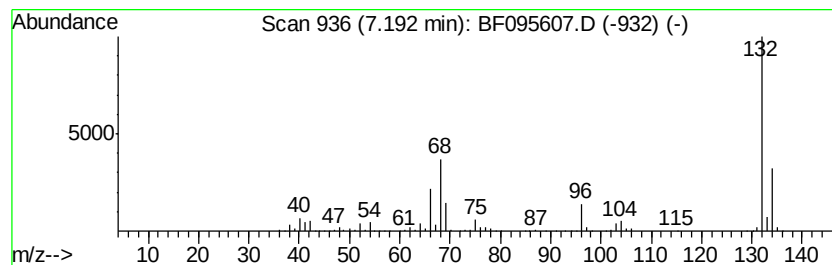

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF060117\
Data File : BF095607.D
Acq On : 1 Jun 2017 21:48
Operator : SJ/MA
Sample : I3384-02
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
MW-2

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF050217.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Oxirane, [(1-meth...	4.80	2.8	ng	58123	1	7.54	420837	20.0
unknown7.19	7.19	96.5	ng	2031520	1	7.54	420837	20.0