

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF060117\
 Data File : BF095624.D
 Acq On : 2 Jun 2017 8:09
 Operator : SJ/MA
 Sample : I3329-09 10X
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 B-17(0-5)

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF050217.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.545	653	656	661	rBV2	23526	52466	6.08%	0.914%
2	7.169	928	932	933	rBV	30945	37838	4.38%	0.659%
3	7.239	940	944	963	rVB	101311	297996	34.53%	5.189%
4	7.539	991	995	1010	rBV	406788	591909	68.58%	10.307%
5	7.786	1034	1037	1056	rBV	95576	191995	22.25%	3.343%
6	8.516	1158	1161	1184	rBV2	25879	122016	14.14%	2.125%
7	9.569	1336	1340	1364	rBV	458697	839868	97.31%	14.625%
8	11.357	1640	1644	1666	rBV	150660	274562	31.81%	4.781%
9	12.063	1760	1764	1783	rBV	28859	65539	7.59%	1.141%
10	12.398	1816	1821	1834	rBV2	596987	863059	100.00%	15.029%
11	13.727	2044	2047	2062	rBV3	29990	73506	8.52%	1.280%
12	14.798	2225	2229	2248	rBV2	432405	776937	90.02%	13.529%
13	16.492	2513	2517	2526	rBV	34162	54770	6.35%	0.954%
14	16.639	2538	2542	2550	rBV2	10646	18577	2.15%	0.323%
15	16.945	2590	2594	2600	rBV	10534	15872	1.84%	0.276%
16	17.145	2625	2628	2642	rBB	144685	185444	21.49%	3.229%
17	18.403	2836	2842	2845	rBV3	7232	13392	1.55%	0.233%
18	18.498	2854	2858	2876	rBV	371264	602417	69.80%	10.490%
19	19.621	3046	3049	3053	rBV3	10807	12162	1.41%	0.212%
20	19.803	3076	3080	3083	rBV3	7448	10789	1.25%	0.188%
21	19.909	3093	3098	3103	rBV6	6592	13044	1.51%	0.227%
22	20.074	3124	3126	3132	rBV6	10638	11768	1.36%	0.205%
23	20.168	3138	3142	3153	rBV	337780	538584	62.40%	9.379%
24	20.603	3211	3216	3222	rVB10	11292	23452	2.72%	0.408%
25	20.703	3230	3233	3239	rVB7	12970	20311	2.35%	0.354%
26	21.003	3280	3284	3289	rBV8	6617	14384	1.67%	0.250%
27	21.050	3289	3292	3298	rVB7	13458	20080	2.33%	0.350%


Sum of corrected areas: 5742737

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF060117\
Data File : BF095624.D
Acq On : 2 Jun 2017 8:09
Operator : SJ/MA
Sample : I3329-09 10X
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
B-17(0-5)

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF050217.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

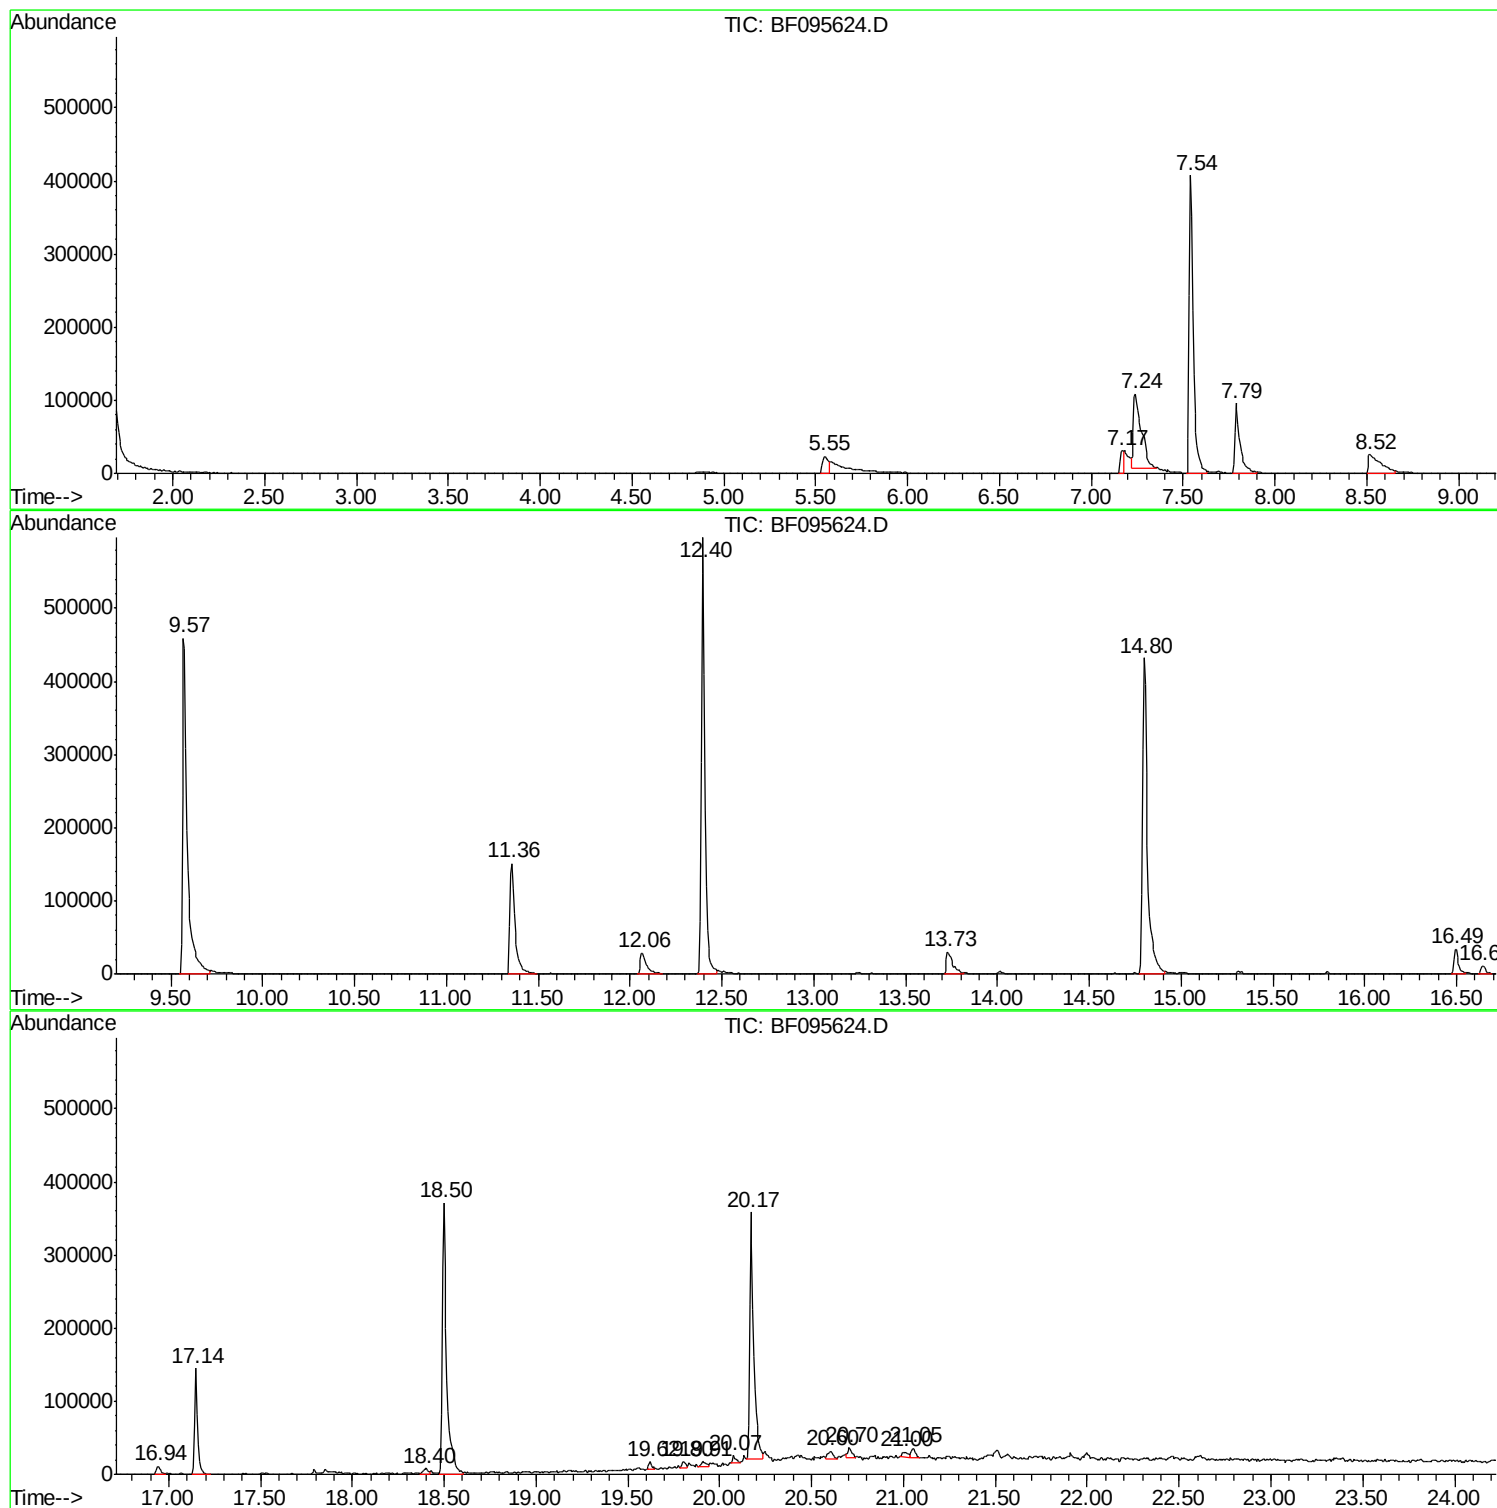

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF060117\
Data File : BF095624.D
Acq On : 2 Jun 2017 8:09
Operator : SJ/MA
Sample : I3329-09 10X
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
B-17(0-5)










Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF050217.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown7.24 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
7.24	10.07 ng	297996	1,4-Dichlorobenzene-d4	7.54

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	35
2		5-Fluoro-2-chloropyrimidine	132	C4H2ClFN2	062802-42-0	17
3		1,3,5-Trifluorobenzene	132	C6H3F3	000372-38-3	9
4		1,2,4-Trifluorobenzene	132	C6H3F3	000367-23-7	9
5		4-Chloro-6-fluoro-pyrimidine	132	C4H2ClFN2	051422-01-6	9

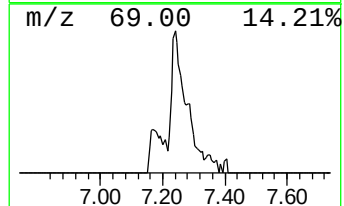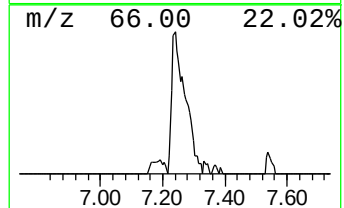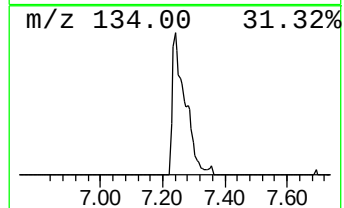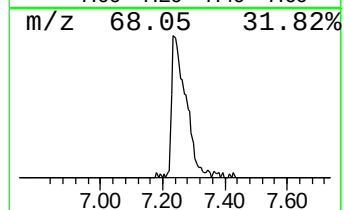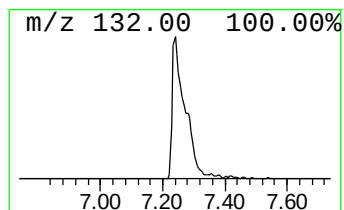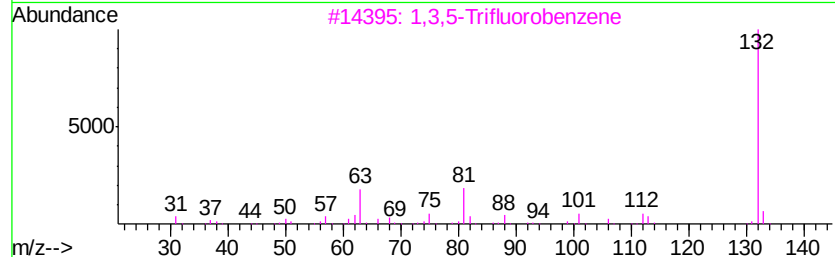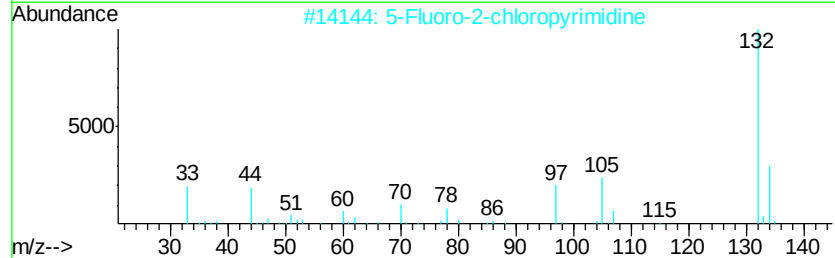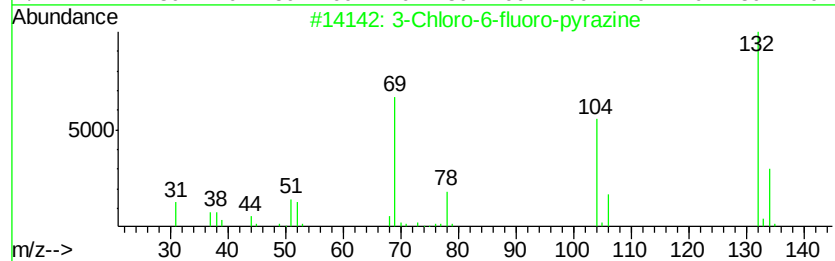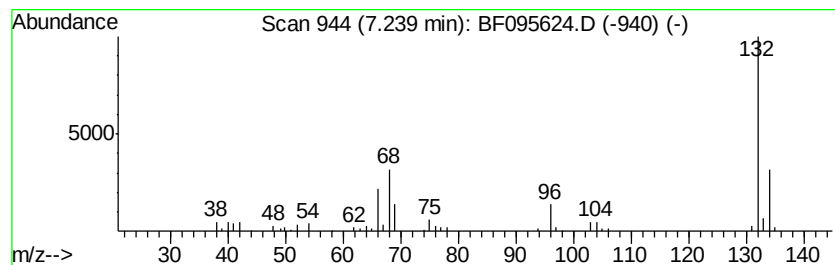

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF060117\
Data File : BF095624.D
Acq On : 2 Jun 2017 8:09
Operator : SJ/MA
Sample : I3329-09 10X
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
B-17(0-5)

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF050217.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown7.24	7.24	10.1	ng	297996	1	7.54	591909	20.0