

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF060117\
 Data File : BF095625.D
 Acq On : 2 Jun 2017 8:41
 Operator : SJ/MA
 Sample : I3329-05 10X
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 B-11(0-3)

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF050217.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.998	218	223	226	rBV2	5702	10770	1.24%	0.190%
2	5.545	652	656	657	rBV2	22261	33651	3.88%	0.594%
3	7.169	929	932	933	rBV2	29580	32209	3.71%	0.569%
4	7.239	940	944	961	rVB	97712	278755	32.11%	4.923%
5	7.539	991	995	1010	rBV	391163	590144	67.97%	10.422%
6	7.786	1033	1037	1053	rBV	93776	179221	20.64%	3.165%
7	8.522	1157	1162	1172	rBV4	23558	83987	9.67%	1.483%
8	9.569	1336	1340	1364	rBV	468224	837288	96.44%	14.787%
9	11.351	1639	1643	1655	rBV	181042	257976	29.71%	4.556%
10	12.063	1760	1764	1778	rBV	25836	54901	6.32%	0.970%
11	12.398	1816	1821	1842	rBV2	586614	868212	100.00%	15.333%
12	13.721	2042	2046	2062	rBV3	38359	85810	9.88%	1.515%
13	14.798	2224	2229	2249	rBV	448332	748992	86.27%	13.227%
14	16.621	2536	2539	2549	rBV	33403	48661	5.60%	0.859%
15	16.927	2586	2591	2599	rBV	30279	47939	5.52%	0.847%
16	17.145	2624	2628	2637	rVB	133604	154340	17.78%	2.726%
17	18.409	2836	2843	2847	rBV5	5660	14444	1.66%	0.255%
18	18.497	2854	2858	2872	rBV	386420	578871	66.67%	10.223%
19	19.791	3075	3078	3082	rBV	21067	33309	3.84%	0.588%
20	19.909	3094	3098	3100	rBV4	11409	16957	1.95%	0.299%
21	20.074	3123	3126	3131	rBV	20316	30347	3.50%	0.536%
22	20.127	3131	3135	3138	rVV	23569	27808	3.20%	0.491%
23	20.168	3138	3142	3152	rVV	349372	541363	62.35%	9.561%
24	20.250	3154	3156	3159	rVB4	12979	12647	1.46%	0.223%
25	20.597	3213	3215	3219	rVB5	9262	12310	1.42%	0.217%
26	20.703	3230	3233	3241	rVB9	23233	41627	4.79%	0.735%
27	21.003	3281	3284	3288	rBV6	11811	17307	1.99%	0.306%
28	21.556	3376	3378	3386	rBV8	7430	13591	1.57%	0.240%
29	21.827	3421	3424	3425	rBV3	9546	8990	1.04%	0.159%


Sum of corrected areas: 5662427

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF060117\
Data File : BF095625.D
Acq On : 2 Jun 2017 8:41
Operator : SJ/MA
Sample : I3329-05 10X
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
B-11(0-3)

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF050217.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

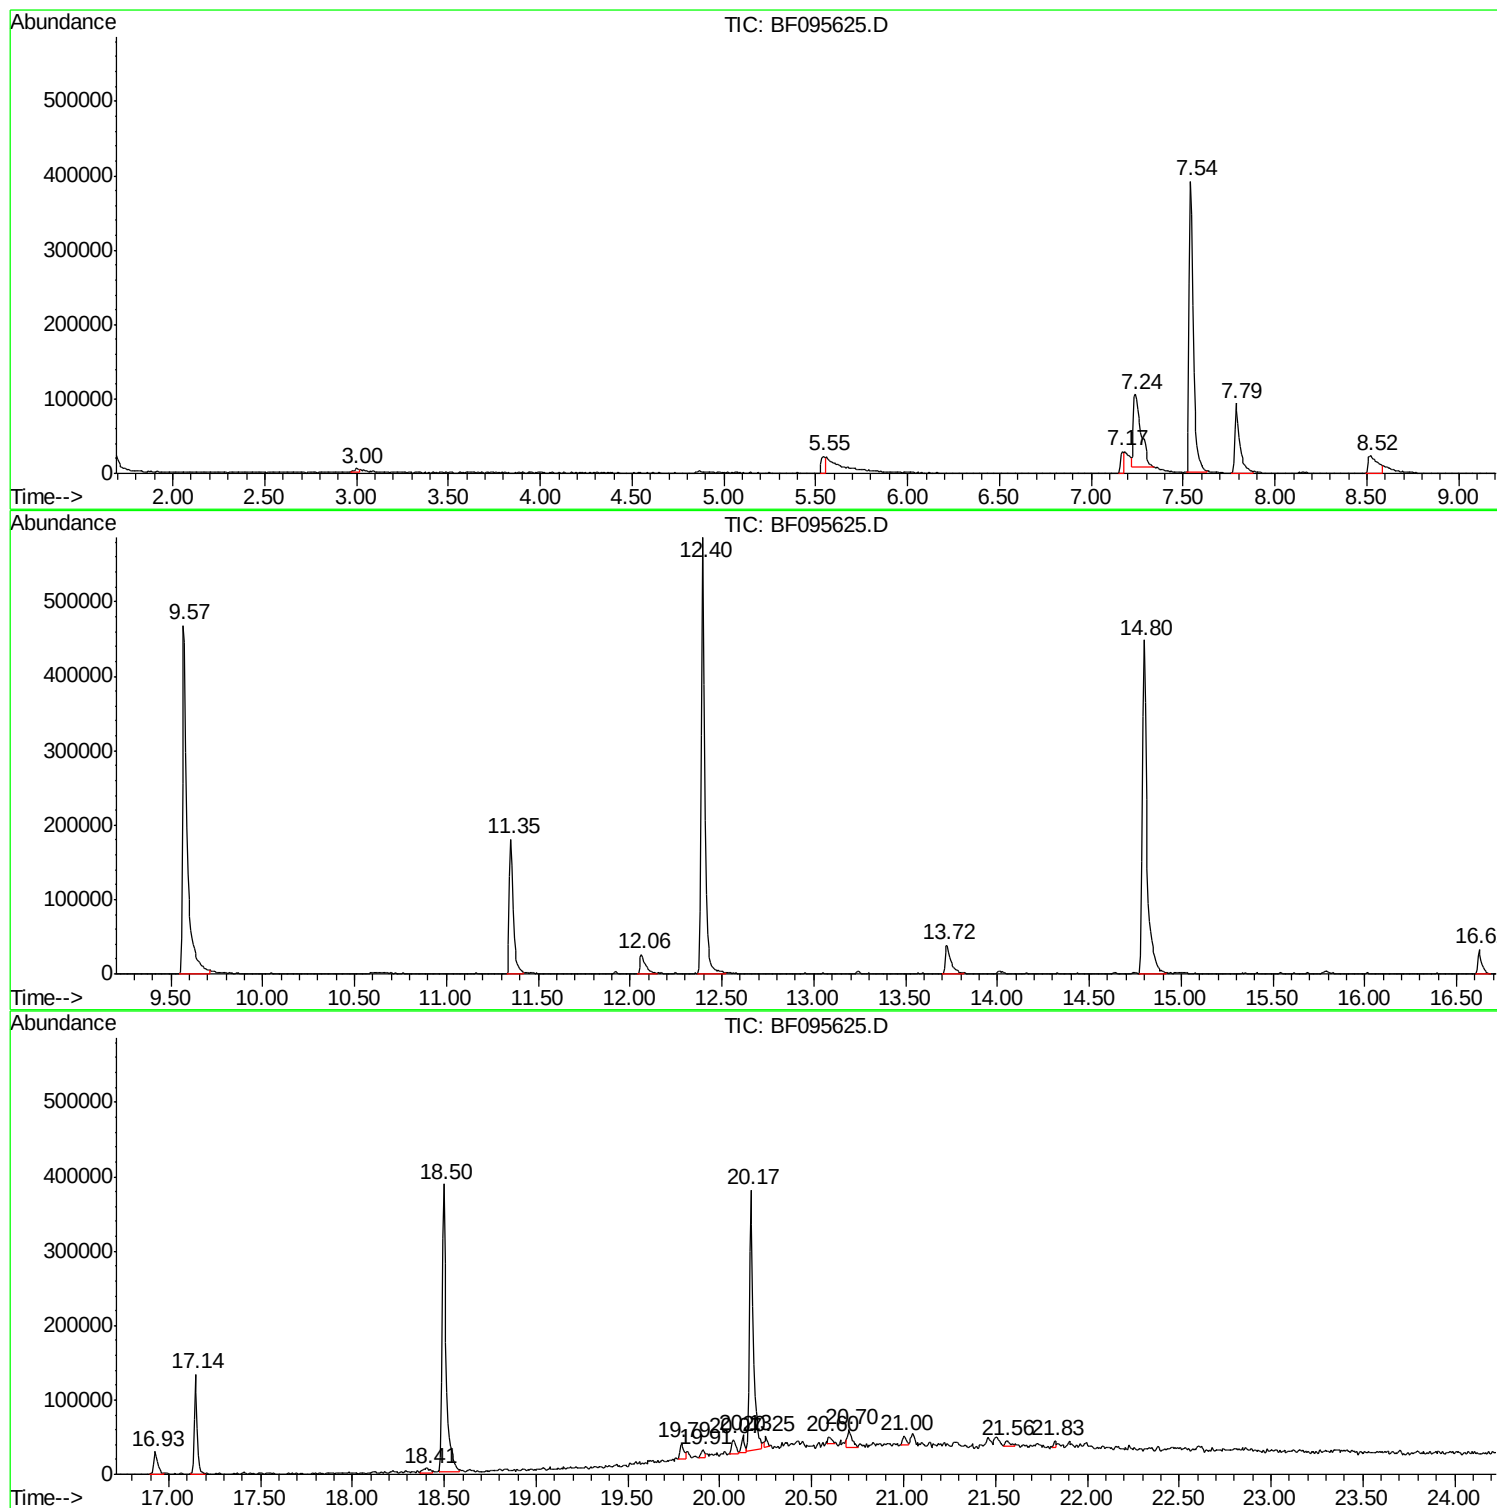

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF060117\
Data File : BF095625.D
Acq On : 2 Jun 2017 8:41
Operator : SJ/MA
Sample : I3329-05 10X
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
B-11(0-3)










Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF050217.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown7.24 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
7.24	9.45 ng	278755	1,4-Dichlorobenzene-d4	7.54

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	25
2		(E)-3-Chloro-2-methyl-2-pentenal	132	C6H9ClO	031357-76-3	25
3		1,3-Cyclopentanedione, 2-chloro-	132	C5H5ClO2	014203-19-1	23
4		4-Chloro-6-fluoro-pyrimidine	132	C4H2ClFN2	051422-01-6	9
5		(5-Methyl-2-pyridyl)acetonitrile	132	C8H8N2	1000241-93-9	9

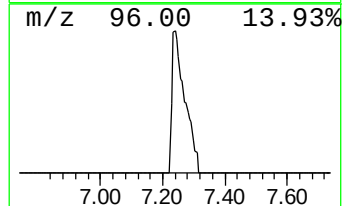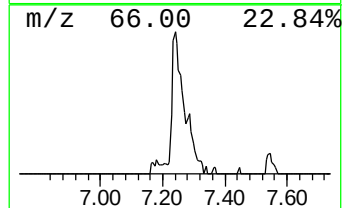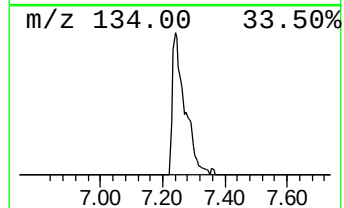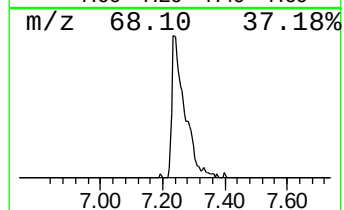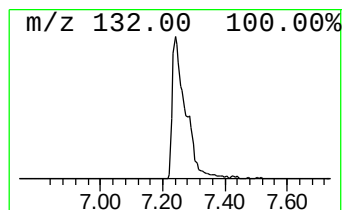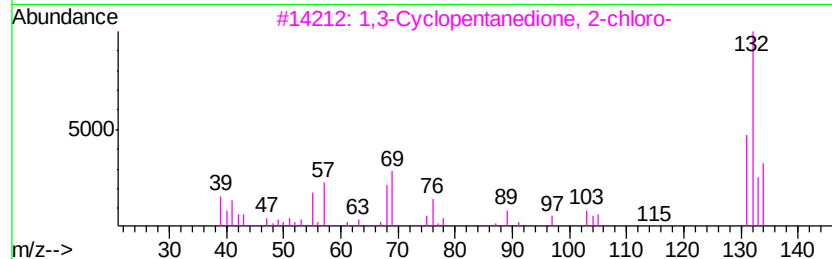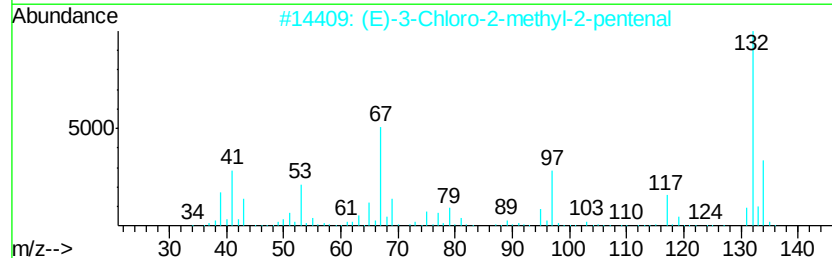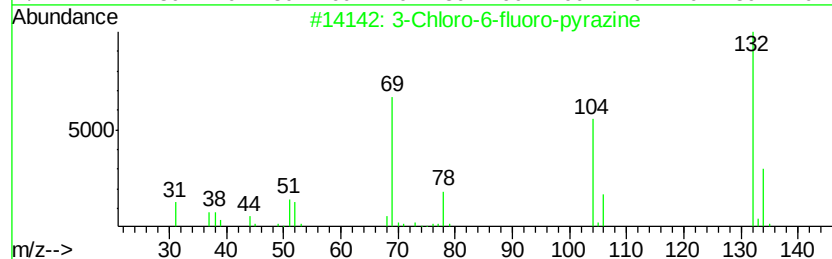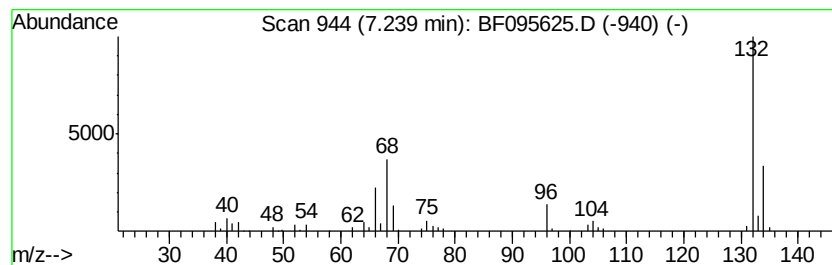

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF060117\
Data File : BF095625.D
Acq On : 2 Jun 2017 8:41
Operator : SJ/MA
Sample : I3329-05 10X
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
B-11(0-3)

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF050217.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown7.24	7.24	9.4	ng	278755	1	7.54	590144	20.0