

Data Path : Z:\HPCHEM1\BNA\_F\DATA\BF060117\  
 Data File : BF095626.D  
 Acq On : 2 Jun 2017 9:14  
 Operator : SJ/MA  
 Sample : I3415-02 5X  
 Misc :  
 ALS Vial : 32 Sample Multiplier: 1

Instrument :  
 BNA\_F  
 ClientSampleId :  
 E2-T6-BASE

Integration Parameters: rteint.p  
 Integrator: RTE  
 Smoothing : ON  
 Sampling : 1  
 Start Thrs: 0.2  
 Stop Thrs : 0  
 Filtering: 5  
 Min Area: 3 % of largest Peak  
 Max Peaks: 100  
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >  
 Peak separation: 5

Method : Z:\HPCHEM1\BNA\_F\METHODS\8270-BF050217.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

| peak<br># | R.T.<br>min | first<br>scan | max<br>scan | last<br>scan | PK<br>TY | peak<br>height | corr.<br>area | corr.<br>% max. | % of<br>total |
|-----------|-------------|---------------|-------------|--------------|----------|----------------|---------------|-----------------|---------------|
| 1         | 3.287       | 266           | 272         | 279          | rBV2     | 11897          | 25790         | 3.10%           | 0.274%        |
| 2         | 3.810       | 355           | 361         | 365          | rBV3     | 9897           | 18951         | 2.28%           | 0.201%        |
| 3         | 4.492       | 472           | 477         | 486          | rBV3     | 10283          | 20737         | 2.50%           | 0.220%        |
| 4         | 4.610       | 492           | 497         | 504          | rVB4     | 22892          | 40122         | 4.83%           | 0.426%        |
| 5         | 4.687       | 506           | 510         | 517          | rVB2     | 17914          | 27289         | 3.28%           | 0.290%        |
| 6         | 4.804       | 527           | 530         | 536          | rBV3     | 7978           | 20840         | 2.51%           | 0.221%        |
| 7         | 5.016       | 561           | 566         | 568          | rBV3     | 13189          | 20190         | 2.43%           | 0.215%        |
| 8         | 5.045       | 568           | 571         | 575          | rVB      | 7352           | 12006         | 1.44%           | 0.128%        |
| 9         | 5.351       | 618           | 623         | 628          | rVB      | 7855           | 11570         | 1.39%           | 0.123%        |
| 10        | 5.481       | 642           | 645         | 659          | rBV      | 101286         | 322689        | 38.83%          | 3.429%        |
| 11        | 5.651       | 670           | 674         | 680          | rVB      | 25883          | 38394         | 4.62%           | 0.408%        |
| 12        | 5.716       | 680           | 685         | 690          | rVB3     | 15407          | 24582         | 2.96%           | 0.261%        |
| 13        | 5.969       | 724           | 728         | 736          | rVB6     | 12225          | 24508         | 2.95%           | 0.260%        |
| 14        | 6.116       | 745           | 753         | 761          | rBV3     | 10177          | 24777         | 2.98%           | 0.263%        |
| 15        | 6.181       | 761           | 764         | 769          | rVV5     | 7470           | 12518         | 1.51%           | 0.133%        |
| 16        | 6.234       | 769           | 773         | 778          | rVB      | 14972          | 20301         | 2.44%           | 0.216%        |
| 17        | 6.322       | 778           | 788         | 790          | rBV6     | 9741           | 23291         | 2.80%           | 0.247%        |
| 18        | 6.345       | 790           | 792         | 795          | rVV      | 15354          | 19897         | 2.39%           | 0.211%        |
| 19        | 6.386       | 795           | 799         | 806          | rVB3     | 23343          | 43592         | 5.25%           | 0.463%        |
| 20        | 6.469       | 806           | 813         | 818          | rBV5     | 14889          | 30213         | 3.64%           | 0.321%        |
| 21        | 6.692       | 844           | 851         | 856          | rBV3     | 24859          | 41020         | 4.94%           | 0.436%        |
| 22        | 6.769       | 860           | 864         | 867          | rBV2     | 10189          | 16010         | 1.93%           | 0.170%        |
| 23        | 6.804       | 867           | 870         | 873          | rVB2     | 11150          | 14040         | 1.69%           | 0.149%        |
| 24        | 6.986       | 896           | 901         | 905          | rBV4     | 7226           | 14239         | 1.71%           | 0.151%        |
| 25        | 7.116       | 920           | 923         | 936          | rBV      | 118979         | 407307        | 49.01%          | 4.328%        |
| 26        | 7.210       | 936           | 939         | 955          | rVB      | 268632         | 622981        | 74.97%          | 6.619%        |
| 27        | 7.539       | 991           | 995         | 1006         | rVV      | 391376         | 572058        | 68.84%          | 6.078%        |
| 28        | 7.622       | 1006          | 1009        | 1014         | rVV3     | 27826          | 37014         | 4.45%           | 0.393%        |
| 29        | 7.686       | 1014          | 1020        | 1026         | rVB5     | 10451          | 18167         | 2.19%           | 0.193%        |
| 30        | 7.781       | 1032          | 1036        | 1052         | rBV      | 241320         | 415755        | 50.03%          | 4.418%        |
| 31        | 8.428       | 1139          | 1146        | 1150         | rBV3     | 16633          | 25648         | 3.09%           | 0.273%        |
| 32        | 8.475       | 1150          | 1154        | 1166         | rBV      | 82555          | 248240        | 29.87%          | 2.638%        |
| 33        | 8.557       | 1166          | 1168        | 1172         | rVB3     | 8689           | 14192         | 1.71%           | 0.151%        |
| 34        | 8.745       | 1194          | 1200        | 1206         | rVB6     | 10640          | 22995         | 2.77%           | 0.244%        |

Data Path : Z:\HPCHEM1\BNA\_F\DATA\BF060117\  
 Data File : BF095626.D  
 Acq On : 2 Jun 2017 9:14  
 Operator : SJ/MA  
 Sample : I3415-02 5X  
 Misc :  
 ALS Vial : 32 Sample Multiplier: 1

Instrument :  
 BNA\_F  
 ClientSampleId :  
 E2-T6-BASE

Integration Parameters: rteint.p  
 Integrator: RTE  
 Smoothing : ON  
 Sampling : 1  
 Start Thrs: 0.2  
 Stop Thrs : 0

Filtering: 5  
 Min Area: 3 % of largest Peak  
 Max Peaks: 100  
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >  
 Peak separation: 5

Method : Z:\HPCHEM1\BNA\_F\METHODS\8270-BF050217.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

|    |        |      |      |      |      |        |        |         |        |
|----|--------|------|------|------|------|--------|--------|---------|--------|
| 35 | 8.804  | 1206 | 1210 | 1215 | rBV5 | 14157  | 21702  | 2.61%   | 0.231% |
| 36 | 9.004  | 1242 | 1244 | 1248 | rVV2 | 15344  | 20189  | 2.43%   | 0.215% |
| 37 | 9.163  | 1264 | 1271 | 1277 | rBV4 | 16211  | 29646  | 3.57%   | 0.315% |
| 38 | 9.345  | 1296 | 1302 | 1305 | rBV3 | 8722   | 12638  | 1.52%   | 0.134% |
| 39 | 9.569  | 1336 | 1340 | 1354 | rBV  | 519406 | 786509 | 94.65%  | 8.357% |
| 40 | 9.780  | 1369 | 1376 | 1380 | rVB  | 47033  | 61610  | 7.41%   | 0.655% |
| 41 | 9.857  | 1386 | 1389 | 1396 | rVB4 | 11405  | 17957  | 2.16%   | 0.191% |
| 42 | 9.933  | 1396 | 1402 | 1406 | rBV3 | 15396  | 20527  | 2.47%   | 0.218% |
| 43 | 10.016 | 1409 | 1416 | 1419 | rBV6 | 5581   | 11744  | 1.41%   | 0.125% |
| 44 | 10.051 | 1419 | 1422 | 1426 | rVB3 | 9487   | 11432  | 1.38%   | 0.121% |
| 45 | 10.104 | 1426 | 1431 | 1438 | rBV2 | 23632  | 36313  | 4.37%   | 0.386% |
| 46 | 10.192 | 1438 | 1446 | 1451 | rBV3 | 15509  | 28974  | 3.49%   | 0.308% |
| 47 | 10.239 | 1451 | 1454 | 1458 | rVV3 | 10808  | 14099  | 1.70%   | 0.150% |
| 48 | 10.363 | 1471 | 1475 | 1479 | rVV  | 44780  | 61775  | 7.43%   | 0.656% |
| 49 | 10.422 | 1483 | 1485 | 1493 | rVB6 | 8498   | 13667  | 1.64%   | 0.145% |
| 50 | 10.598 | 1508 | 1515 | 1517 | rBV2 | 10180  | 19125  | 2.30%   | 0.203% |
| 51 | 10.739 | 1534 | 1539 | 1542 | rVV5 | 9548   | 19850  | 2.39%   | 0.211% |
| 52 | 10.798 | 1545 | 1549 | 1555 | rVB4 | 17395  | 26961  | 3.24%   | 0.286% |
| 53 | 10.957 | 1569 | 1576 | 1579 | rBV6 | 11188  | 25076  | 3.02%   | 0.266% |
| 54 | 11.104 | 1597 | 1601 | 1604 | rBV2 | 26875  | 33243  | 4.00%   | 0.353% |
| 55 | 11.345 | 1637 | 1642 | 1653 | rVB  | 312356 | 462886 | 55.70%  | 4.918% |
| 56 | 11.551 | 1674 | 1677 | 1678 | rBV  | 12039  | 11678  | 1.41%   | 0.124% |
| 57 | 11.574 | 1679 | 1681 | 1686 | rVB4 | 19944  | 24033  | 2.89%   | 0.255% |
| 58 | 11.633 | 1686 | 1691 | 1696 | rBV6 | 13992  | 29115  | 3.50%   | 0.309% |
| 59 | 11.686 | 1696 | 1700 | 1707 | rVB5 | 9508   | 18362  | 2.21%   | 0.195% |
| 60 | 12.045 | 1756 | 1761 | 1764 | rBV2 | 45989  | 78008  | 9.39%   | 0.829% |
| 61 | 12.080 | 1764 | 1767 | 1771 | rVV  | 71409  | 89407  | 10.76%  | 0.950% |
| 62 | 12.121 | 1771 | 1774 | 1780 | rVB4 | 10571  | 18308  | 2.20%   | 0.195% |
| 63 | 12.392 | 1815 | 1820 | 1827 | rBV2 | 633351 | 830988 | 100.00% | 8.830% |
| 64 | 12.445 | 1827 | 1829 | 1839 | rVV7 | 21457  | 42103  | 5.07%   | 0.447% |
| 65 | 12.845 | 1894 | 1897 | 1901 | rVB4 | 12088  | 14145  | 1.70%   | 0.150% |
| 66 | 12.945 | 1911 | 1914 | 1919 | rVB3 | 13731  | 18489  | 2.22%   | 0.196% |
| 67 | 13.151 | 1947 | 1949 | 1953 | rVB3 | 8547   | 11853  | 1.43%   | 0.126% |
| 68 | 13.292 | 1969 | 1973 | 1975 | rBV3 | 10946  | 16864  | 2.03%   | 0.179% |
| 69 | 13.598 | 2019 | 2025 | 2030 | rVB  | 56989  | 81511  | 9.81%   | 0.866% |
| 70 | 13.704 | 2039 | 2043 | 2056 | rBV2 | 125142 | 248106 | 29.86%  | 2.636% |
| 71 | 13.898 | 2073 | 2076 | 2085 | rVB8 | 9290   | 15901  | 1.91%   | 0.169% |

Data Path : Z:\HPCHEM1\BNA\_F\DATA\BF060117\  
 Data File : BF095626.D  
 Acq On : 2 Jun 2017 9:14  
 Operator : SJ/MA  
 Sample : I3415-02 5X  
 Misc :  
 ALS Vial : 32 Sample Multiplier: 1

Instrument :  
 BNA\_F  
 ClientSampleId :  
 E2-T6-BASE

Integration Parameters: rteint.p  
 Integrator: RTE  
 Smoothing : ON  
 Sampling : 1  
 Start Thrs: 0.2  
 Stop Thrs : 0  
 Filtering: 5  
 Min Area: 3 % of largest Peak  
 Max Peaks: 100  
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >  
 Peak separation: 5

Method : Z:\HPCHEM1\BNA\_F\METHODS\8270-BF050217.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

|     |        |      |      |      |      |        |        |        |        |
|-----|--------|------|------|------|------|--------|--------|--------|--------|
| 72  | 14.033 | 2092 | 2099 | 2104 | rBV  | 71477  | 107789 | 12.97% | 1.145% |
| 73  | 14.380 | 2154 | 2158 | 2162 | rVB4 | 12229  | 15923  | 1.92%  | 0.169% |
| 74  | 14.798 | 2222 | 2229 | 2243 | rBV2 | 507506 | 827022 | 99.52% | 8.787% |
| 75  | 14.968 | 2255 | 2258 | 2263 | rVB6 | 12401  | 17779  | 2.14%  | 0.189% |
| 76  | 15.339 | 2318 | 2321 | 2327 | rVB5 | 12020  | 16069  | 1.93%  | 0.171% |
| 77  | 15.521 | 2348 | 2352 | 2358 | rBV6 | 7810   | 15404  | 1.85%  | 0.164% |
| 78  | 15.609 | 2365 | 2367 | 2373 | rBV5 | 6793   | 12401  | 1.49%  | 0.132% |
| 79  | 15.804 | 2398 | 2400 | 2405 | rVB6 | 11027  | 13104  | 1.58%  | 0.139% |
| 80  | 15.851 | 2405 | 2408 | 2411 | rBV3 | 8983   | 12810  | 1.54%  | 0.136% |
| 81  | 16.015 | 2433 | 2436 | 2441 | rBV5 | 8719   | 13352  | 1.61%  | 0.142% |
| 82  | 16.415 | 2501 | 2504 | 2508 | rVB6 | 14118  | 19638  | 2.36%  | 0.209% |
| 83  | 16.474 | 2510 | 2514 | 2516 | rBV4 | 8739   | 11574  | 1.39%  | 0.123% |
| 84  | 16.568 | 2526 | 2530 | 2535 | rVB7 | 9782   | 15314  | 1.84%  | 0.163% |
| 85  | 16.621 | 2535 | 2539 | 2546 | rBV2 | 24316  | 46087  | 5.55%  | 0.490% |
| 86  | 16.756 | 2558 | 2562 | 2564 | rBV4 | 8615   | 12155  | 1.46%  | 0.129% |
| 87  | 16.921 | 2587 | 2590 | 2599 | rVB3 | 26068  | 46947  | 5.65%  | 0.499% |
| 88  | 17.103 | 2617 | 2621 | 2624 | rBV4 | 11740  | 21268  | 2.56%  | 0.226% |
| 89  | 17.145 | 2624 | 2628 | 2634 | rVB  | 230734 | 270722 | 32.58% | 2.877% |
| 90  | 18.397 | 2836 | 2841 | 2846 | rBV5 | 13490  | 25341  | 3.05%  | 0.269% |
| 91  | 18.497 | 2853 | 2858 | 2871 | rBV  | 388497 | 580653 | 69.88% | 6.170% |
| 92  | 19.792 | 3074 | 3078 | 3080 | rBV  | 12785  | 16873  | 2.03%  | 0.179% |
| 93  | 19.903 | 3093 | 3097 | 3102 | rBV6 | 14696  | 21072  | 2.54%  | 0.224% |
| 94  | 20.074 | 3122 | 3126 | 3129 | rBV4 | 9823   | 11949  | 1.44%  | 0.127% |
| 95  | 20.127 | 3132 | 3135 | 3138 | rBV  | 12912  | 16953  | 2.04%  | 0.180% |
| 96  | 20.168 | 3138 | 3142 | 3153 | rVV  | 349005 | 529470 | 63.72% | 5.626% |
| 97  | 20.250 | 3153 | 3156 | 3160 | rVB5 | 15722  | 17844  | 2.15%  | 0.190% |
| 98  | 20.603 | 3212 | 3216 | 3221 | rBV4 | 12599  | 19231  | 2.31%  | 0.204% |
| 99  | 20.997 | 3279 | 3283 | 3289 | rBV7 | 11992  | 18272  | 2.20%  | 0.194% |
| 100 | 23.368 | 3677 | 3686 | 3696 | rVB8 | 44108  | 121649 | 14.64% | 1.293% |


Sum of corrected areas: 9411382

Data Path : Z:\HPCHEM1\BNA\_F\DATA\BF060117\  
Data File : BF095626.D  
Acq On : 2 Jun 2017 9:14  
Operator : SJ/MA  
Sample : I3415-02 5X  
Misc :  
ALS Vial : 32 Sample Multiplier: 1

Instrument :  
BNA\_F  
ClientSampleId :  
E2-T6-BASE

Quant Method : Z:\HPCHEM1\BNA\_F\METHODS\8270-BF050217.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L  
TIC Integration Parameters: LSCINT.P

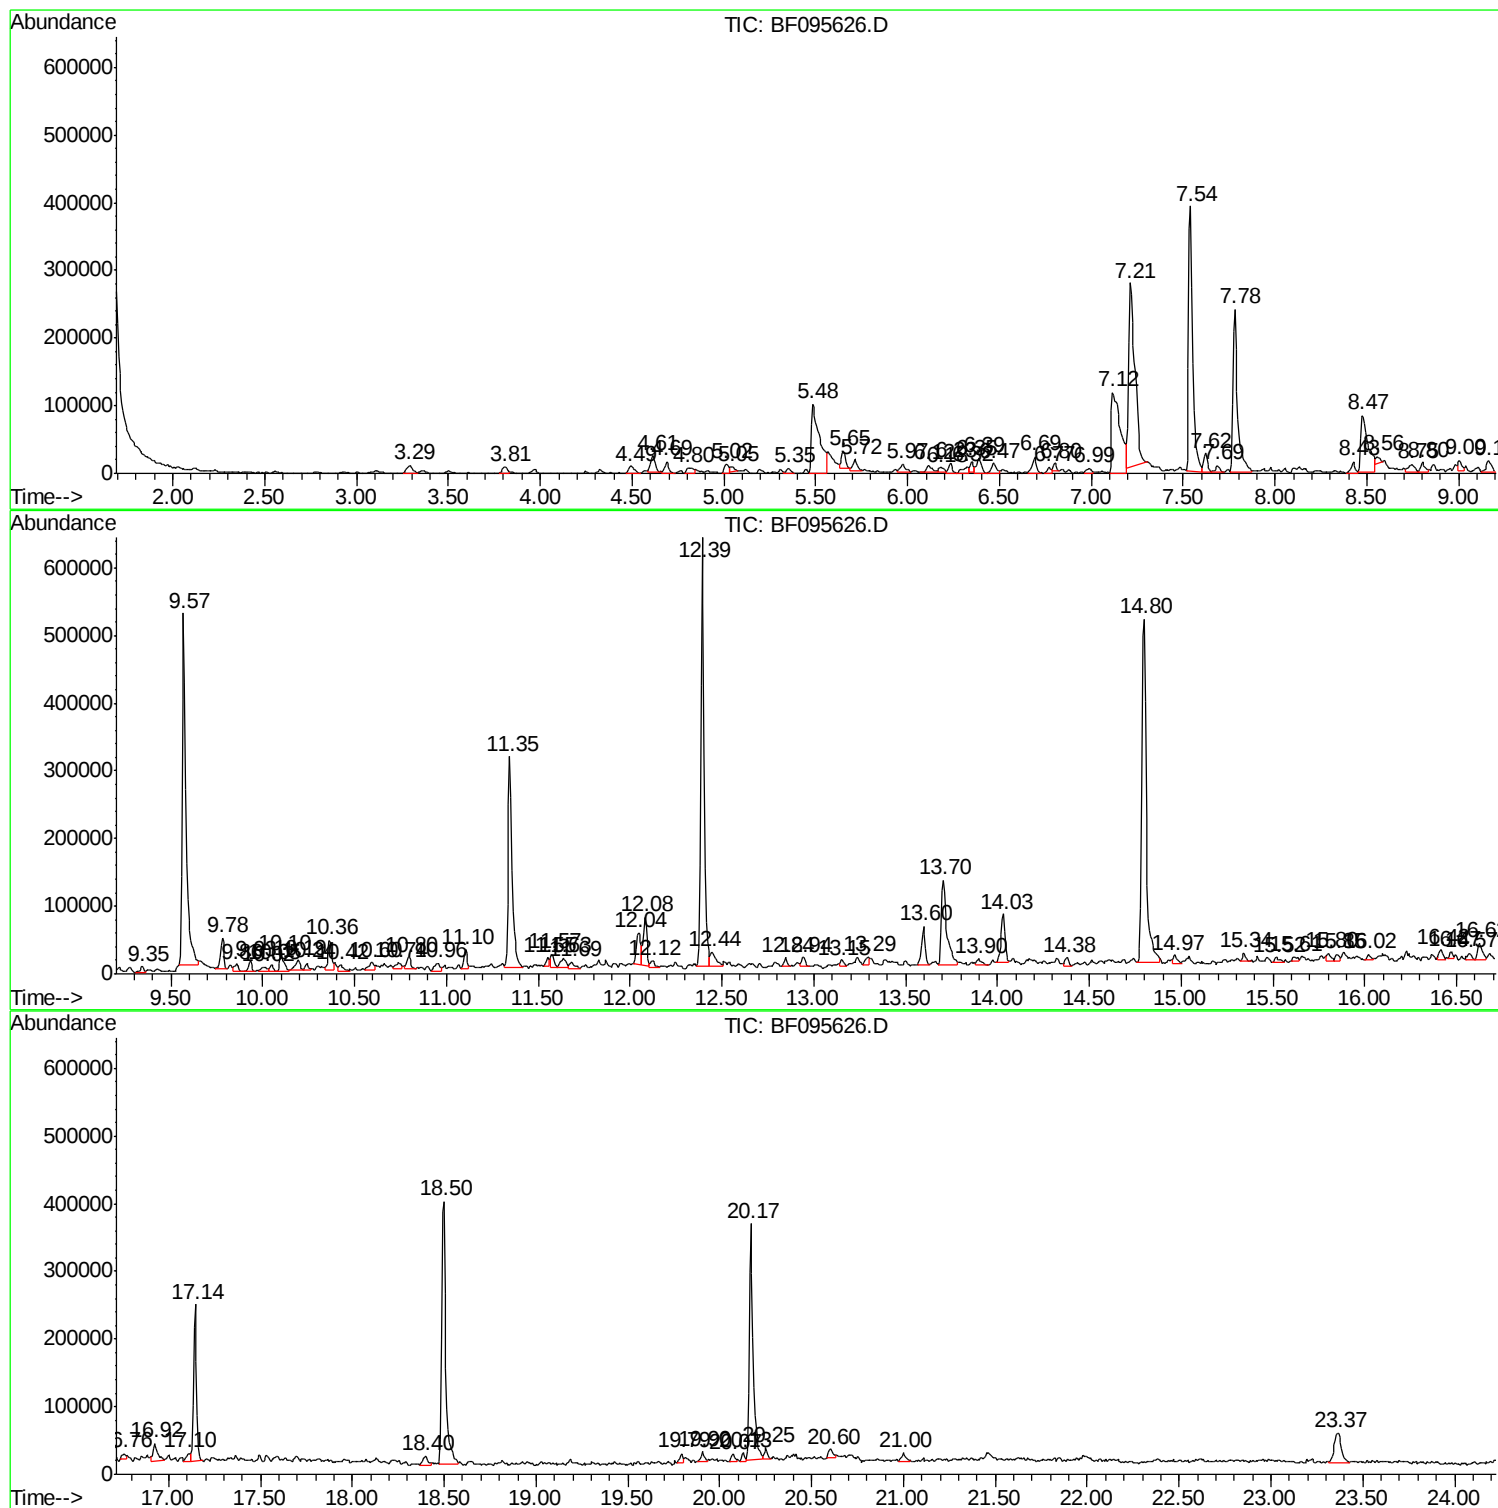

Data Path : Z:\HPCHEM1\BNA\_F\DATA\BF060117\  
Data File : BF095626.D  
Acq On : 2 Jun 2017 9:14  
Operator : SJ/MA  
Sample : I3415-02 5X  
Misc :  
ALS Vial : 32 Sample Multiplier: 1

Instrument :  
BNA\_F  
ClientSampleId :  
E2-T6-BASE

Quant Method : Z:\HPCHEM1\BNA\_F\METHODS\8270-BF050217.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION










TIC Library : C:\DATABASE\NIST11.L  
TIC Integration Parameters: LSCINT.P

\*\*\*\*\*  
Peak Number 1 unknown7.21 Concentration Rank 1

| R.T. | EstConc  | Area   | Relative to ISTD       | R.T. |
|------|----------|--------|------------------------|------|
| 7.21 | 21.78 ng | 622981 | 1,4-Dichlorobenzene-d4 | 7.54 |

| Hit# | of | Tentative ID                     | MW  | MolForm   | CAS#         | Qual |
|------|----|----------------------------------|-----|-----------|--------------|------|
| 1    | 5  | 3-Chloro-6-fluoro-pyrazine       | 132 | C4H2ClFN2 | 1000146-10-7 | 38   |
| 2    |    | (E)-3-Chloro-2-methyl-2-pentenal | 132 | C6H9ClO   | 031357-76-3  | 12   |
| 3    |    | Xenon                            | 132 | Xe        | 007440-63-3  | 9    |
| 4    |    | 4-Chloro-6-fluoro-pyrimidine     | 132 | C4H2ClFN2 | 051422-01-6  | 9    |
| 5    |    | 4-Methylpyrrolo[1,2-a]pyrazine   | 132 | C8H8N2    | 064608-60-2  | 9    |

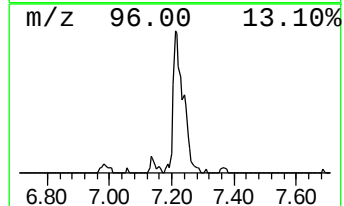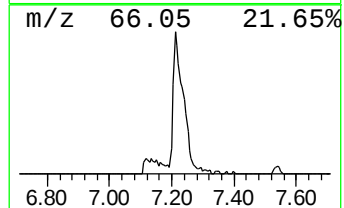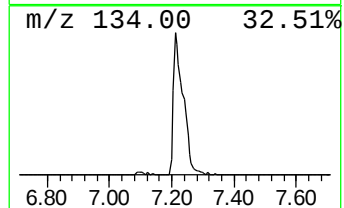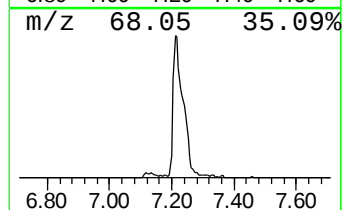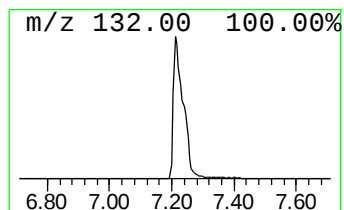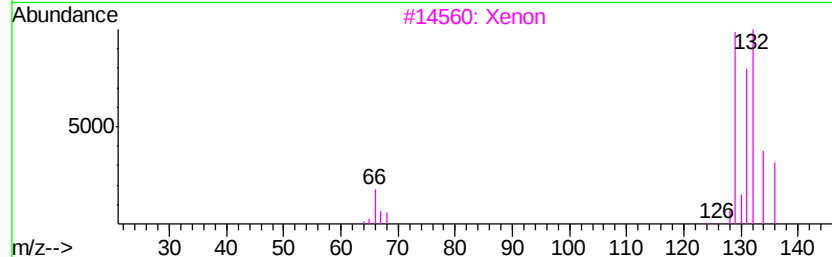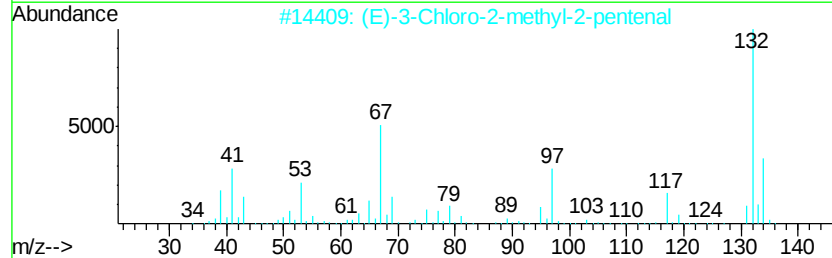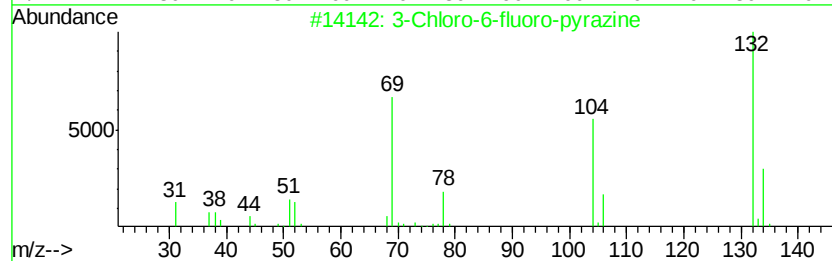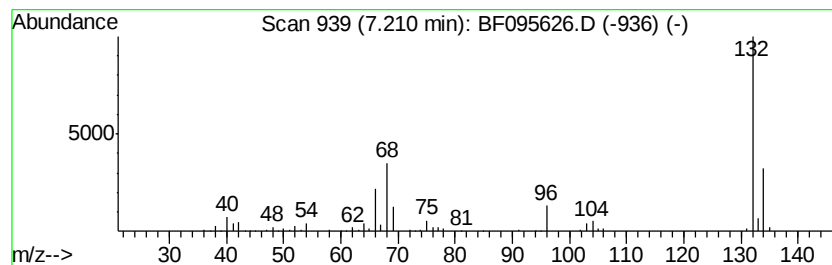

Data Path : Z:\HPCHEM1\BNA\_F\DATA\BF060117\  
Data File : BF095626.D  
Acq On : 2 Jun 2017 9:14  
Operator : SJ/MA  
Sample : I3415-02 5X  
Misc :  
ALS Vial : 32 Sample Multiplier: 1

Instrument :  
BNA\_F  
ClientSampleId :  
E2-T6-BASE

Quant Method : Z:\HPCHEM1\BNA\_F\METHODS\8270-BF050217.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION










TIC Library : C:\DATABASE\NIST11.L  
TIC Integration Parameters: LSCINT.P

\*\*\*\*\*  
Peak Number 3 Dodecane, 2,6,11-trimethyl- Concentration Rank 4

| R.T.  | EstConc | Area   | Relative to ISTD | R.T.  |
|-------|---------|--------|------------------|-------|
| 14.03 | 2.61 ng | 107789 | Phenanthrene-d10 | 14.80 |

| Hit# | of | Tentative ID                        | MW  | MolForm   | CAS#         | Qual |
|------|----|-------------------------------------|-----|-----------|--------------|------|
| 1    | 5  | Dodecane, 2,6,11-trimethyl-         | 212 | C15H32    | 031295-56-4  | 80   |
| 2    |    | Dodecane, 2,7,10-trimethyl-         | 212 | C15H32    | 074645-98-0  | 64   |
| 3    |    | Octane, 2,6-dimethyl-               | 142 | C10H22    | 002051-30-1  | 64   |
| 4    |    | Sulfurous acid, dodecyl 2-ethylh... | 362 | C20H42O3S | 1000309-19-5 | 58   |
| 5    |    | Tridecane, 3-methyl-                | 198 | C14H30    | 006418-41-3  | 53   |

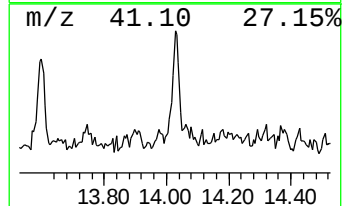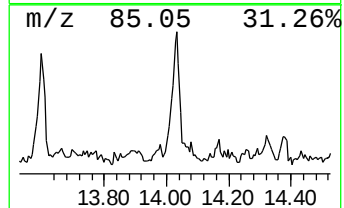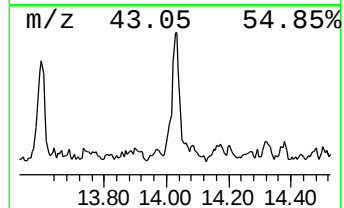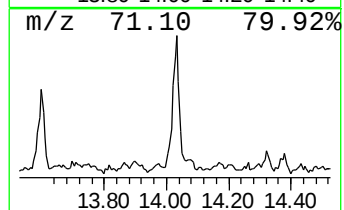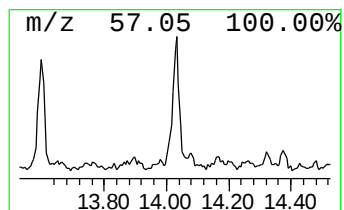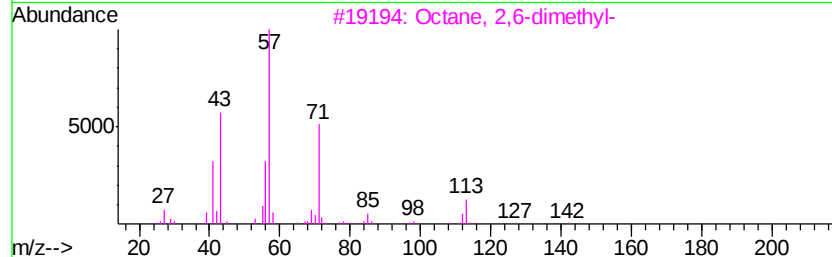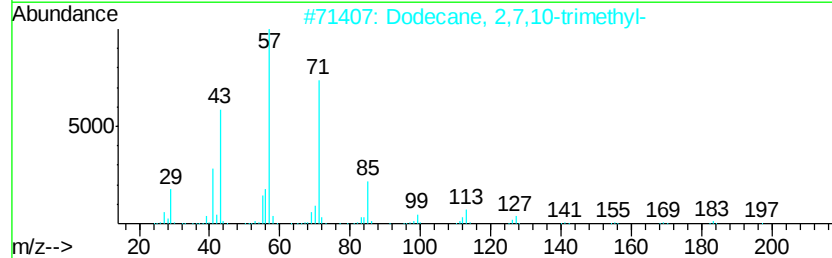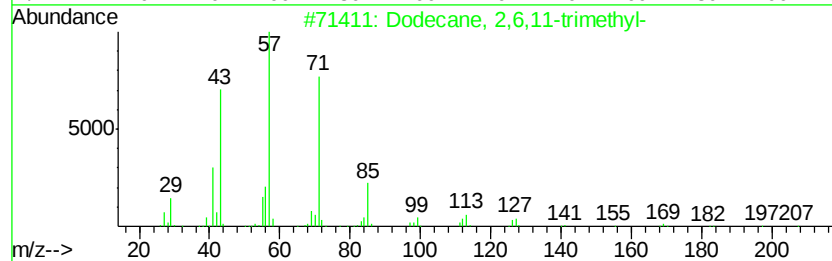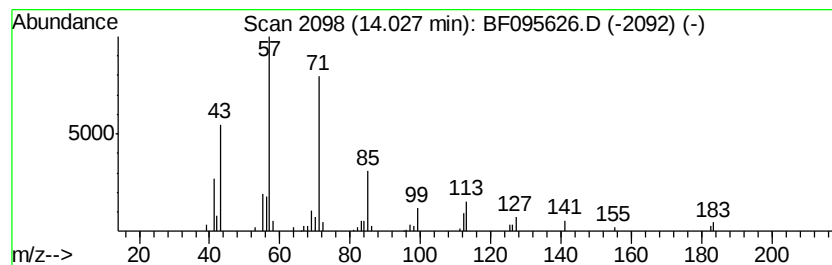

Data Path : Z:\HPCHEM1\BNA\_F\DATA\BF060117\  
Data File : BF095626.D  
Acq On : 2 Jun 2017 9:14  
Operator : SJ/MA  
Sample : I3415-02 5X  
Misc :  
ALS Vial : 32 Sample Multiplier: 1

Instrument :  
BNA\_F  
ClientSampleId :  
E2-T6-BASE

Quant Method : Z:\HPCHEM1\BNA\_F\METHODS\8270-BF050217.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION










TIC Library : C:\DATABASE\NIST11.L  
TIC Integration Parameters: LSCINT.P

\*\*\*\*\*  
Peak Number 4 unknown23.37 Concentration Rank 3

| R.T.  | EstConc | Area   | Relative to ISTD | R.T.  |
|-------|---------|--------|------------------|-------|
| 23.37 | 4.60 ng | 121649 | Perylene-d12     | 20.17 |

| Hit# | of | Tentative ID                        | MW  | MolForm  | CAS#         | Qual |
|------|----|-------------------------------------|-----|----------|--------------|------|
| 1    | 5  | Bicyclo[2.2.1]heptane, 2,2,3-tri... | 138 | C10H18   | 020536-40-7  | 35   |
| 2    |    | Bicyclo[2.2.1]heptane, 2,2,3-tri... | 138 | C10H18   | 020536-41-8  | 35   |
| 3    |    | 7-Heptadecyne, 17-chloro-           | 270 | C17H31Cl | 056554-75-7  | 27   |
| 4    |    | 9-Octadecyne                        | 250 | C18H34   | 035365-59-4  | 22   |
| 5    |    | Caparratriene                       | 206 | C15H26   | 1000374-08-7 | 22   |

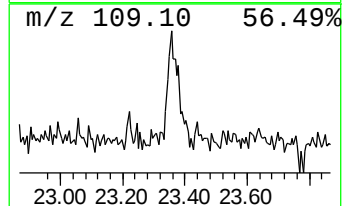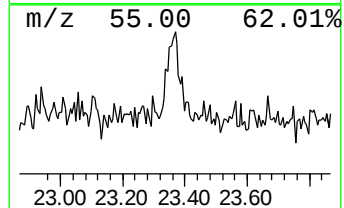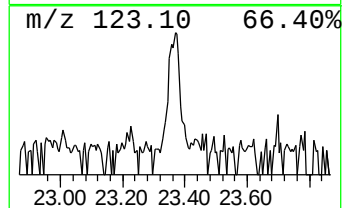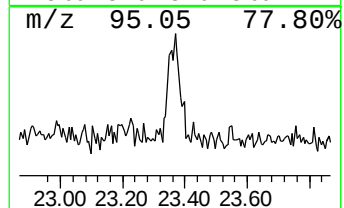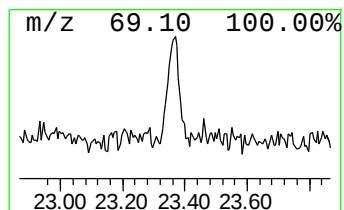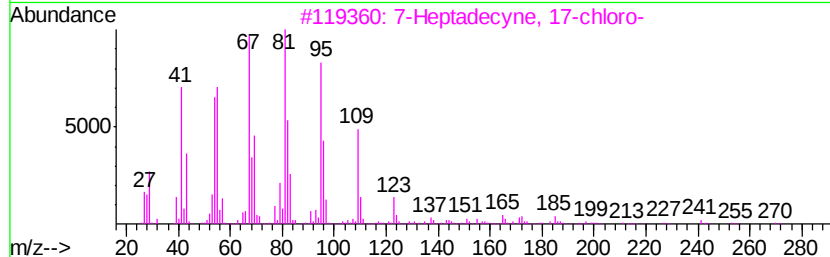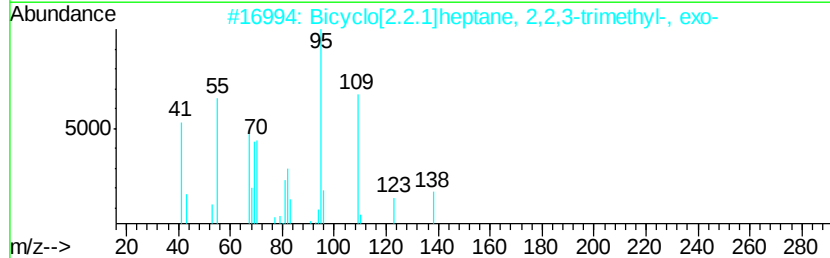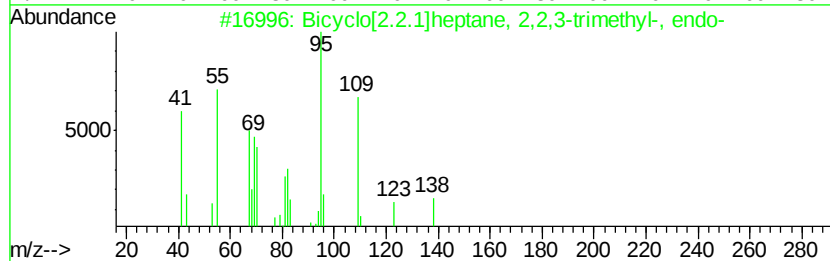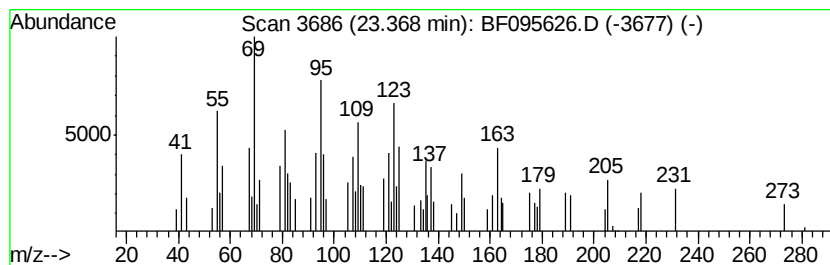

Data Path : Z:\HPCHEM1\BNA\_F\DATA\BF060117\  
Data File : BF095626.D  
Acq On : 2 Jun 2017 9:14  
Operator : SJ/MA  
Sample : I3415-02 5X  
Misc :  
ALS Vial : 32 Sample Multiplier: 1

Instrument :  
BNA\_F  
ClientSampleId :  
E2-T6-BASE

Quant Method : Z:\HPCHEM1\BNA\_F\METHODS\8270-BF050217.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L  
TIC Integration Parameters: LSCINT.P

| TIC Top Hit name     | RT    | EstConc | Units | Response | --Internal Standard-- |       |        |      |
|----------------------|-------|---------|-------|----------|-----------------------|-------|--------|------|
|                      |       |         |       |          | #                     | RT    | Resp   | Conc |
| unknown7.21          | 7.21  | 21.8    | ng    | 622981   | 1                     | 7.54  | 572058 | 20.0 |
| Dodecane, 2,6,11-... | 14.03 | 2.6     | ng    | 107789   | 4                     | 14.80 | 827022 | 20.0 |
| unknown23.37         | 23.37 | 4.6     | ng    | 121649   | 6                     | 20.17 | 529470 | 20.0 |