

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF060117\
 Data File : BF095628.D
 Acq On : 2 Jun 2017 10:18
 Operator : SJ/MA
 Sample : I3415-03 10X
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 E2-T6-ESW

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF050217.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.528	650	653	657	rBV3	23516	47767	5.71%	0.656%
2	5.710	680	684	696	rVB3	11266	26074	3.12%	0.358%
3	7.163	926	931	939	rBV2	34934	116203	13.89%	1.595%
4	7.234	939	943	960	rVV	106031	337278	40.31%	4.629%
5	7.345	960	962	970	rVB5	6692	11767	1.41%	0.161%
6	7.539	991	995	1015	rBV	436010	613073	73.27%	8.413%
7	7.787	1033	1037	1053	rBV	92583	178724	21.36%	2.453%
8	8.504	1155	1159	1177	rBV	27043	105961	12.66%	1.454%
9	9.569	1336	1340	1367	rBV	493957	801564	95.80%	11.000%
10	11.351	1639	1643	1665	rBV	154696	243207	29.07%	3.338%
11	12.057	1758	1763	1775	rBV	25842	49124	5.87%	0.674%
12	12.392	1816	1820	1828	rBV2	631987	836689	100.00%	11.482%
13	12.451	1828	1830	1837	rVB2	16736	26842	3.21%	0.368%
14	13.316	1974	1977	1988	rBB2	8302	14109	1.69%	0.194%
15	13.721	2042	2046	2062	rVB4	34782	70636	8.44%	0.969%
16	14.033	2091	2099	2105	rBV3	6551	15052	1.80%	0.207%
17	14.704	2209	2213	2218	rBV	62325	71974	8.60%	0.988%
18	14.798	2224	2229	2233	rBV	506794	722728	86.38%	9.918%
19	14.839	2233	2236	2247	rVV	112784	199445	23.84%	2.737%
20	14.951	2250	2255	2266	rVB	20614	39275	4.69%	0.539%
21	15.262	2304	2308	2312	rBV3	6902	11033	1.32%	0.151%
22	15.610	2364	2367	2371	rBV	10839	14181	1.69%	0.195%
23	15.657	2371	2375	2381	rVB2	12844	19314	2.31%	0.265%
24	15.757	2384	2392	2394	rBV2	18530	33527	4.01%	0.460%
25	15.780	2394	2396	2407	rVB	26566	42233	5.05%	0.580%
26	16.057	2439	2443	2447	rBV	8631	9817	1.17%	0.135%
27	16.604	2532	2536	2544	rBV	185821	237451	28.38%	3.259%
28	16.909	2583	2588	2600	rBV	158194	233585	27.92%	3.206%
29	17.115	2619	2623	2624	rBV	8812	8680	1.04%	0.119%
30	17.145	2624	2628	2633	rVB	146179	159184	19.03%	2.185%
31	17.239	2639	2644	2650	rVB3	8580	16855	2.01%	0.231%
32	17.345	2659	2662	2666	rBV4	6609	9815	1.17%	0.135%
33	17.386	2666	2669	2676	rVB2	14040	19387	2.32%	0.266%
34	17.474	2680	2684	2688	rBV3	8298	12028	1.44%	0.165%

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF060117\
Data File : BF095628.D
Acq On : 2 Jun 2017 10:18
Operator : SJ/MA
Sample : I3415-03 10X
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
E2-T6-ESW

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON
Sampling : 1
Start Thrs: 0.2
Stop Thrs : 0
Filtering: 5
Min Area: 3 % of largest Peak
Max Peaks: 100
Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF050217.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

35	17.527	2688	2693	2696	rBV4	14321	19482	2.33%	0.267%
36	18.209	2807	2809	2813	rVB4	8852	8931	1.07%	0.123%
37	18.256	2813	2817	2820	rVB	8465	12793	1.53%	0.176%
38	18.286	2820	2822	2826	rVB3	7226	8481	1.01%	0.116%
39	18.403	2839	2842	2848	rVB5	7733	11177	1.34%	0.153%
40	18.492	2852	2857	2862	rBV2	520149	694812	83.04%	9.535%
41	18.633	2878	2881	2884	rBV3	13221	15651	1.87%	0.215%
42	18.803	2906	2910	2913	rBV5	9235	12831	1.53%	0.176%
43	19.015	2943	2946	2951	rVB2	9708	12941	1.55%	0.178%
44	19.550	3035	3037	3040	rVB3	7932	8976	1.07%	0.123%
45	19.774	3071	3075	3079	rBV	68619	97818	11.69%	1.342%
46	19.903	3092	3097	3101	rBV5	22555	42361	5.06%	0.581%
47	20.062	3121	3124	3130	rBV	38351	51144	6.11%	0.702%
48	20.121	3130	3134	3138	rVV	65156	77111	9.22%	1.058%
49	20.168	3138	3142	3152	rVV	380717	578512	69.14%	7.939%
50	20.250	3152	3156	3161	rVB6	25392	39332	4.70%	0.540%
51	20.597	3213	3215	3221	rVB7	18034	28605	3.42%	0.393%
52	20.703	3231	3233	3240	rVB7	20302	30888	3.69%	0.424%
53	20.997	3281	3283	3287	rVV5	16238	21843	2.61%	0.300%
54	21.056	3289	3293	3299	rVB5	21529	39210	4.69%	0.538%
55	21.456	3357	3361	3366	rVB5	24307	41654	4.98%	0.572%
56	21.503	3368	3369	3373	rVB4	11578	12334	1.47%	0.169%
57	21.815	3418	3422	3430	rVB3	19103	45849	5.48%	0.629%
58	21.997	3449	3453	3458	rBV7	10017	19508	2.33%	0.268%


Sum of corrected areas: 7286826

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF060117\
Data File : BF095628.D
Acq On : 2 Jun 2017 10:18
Operator : SJ/MA
Sample : I3415-03 10X
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
E2-T6-ESW

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF050217.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

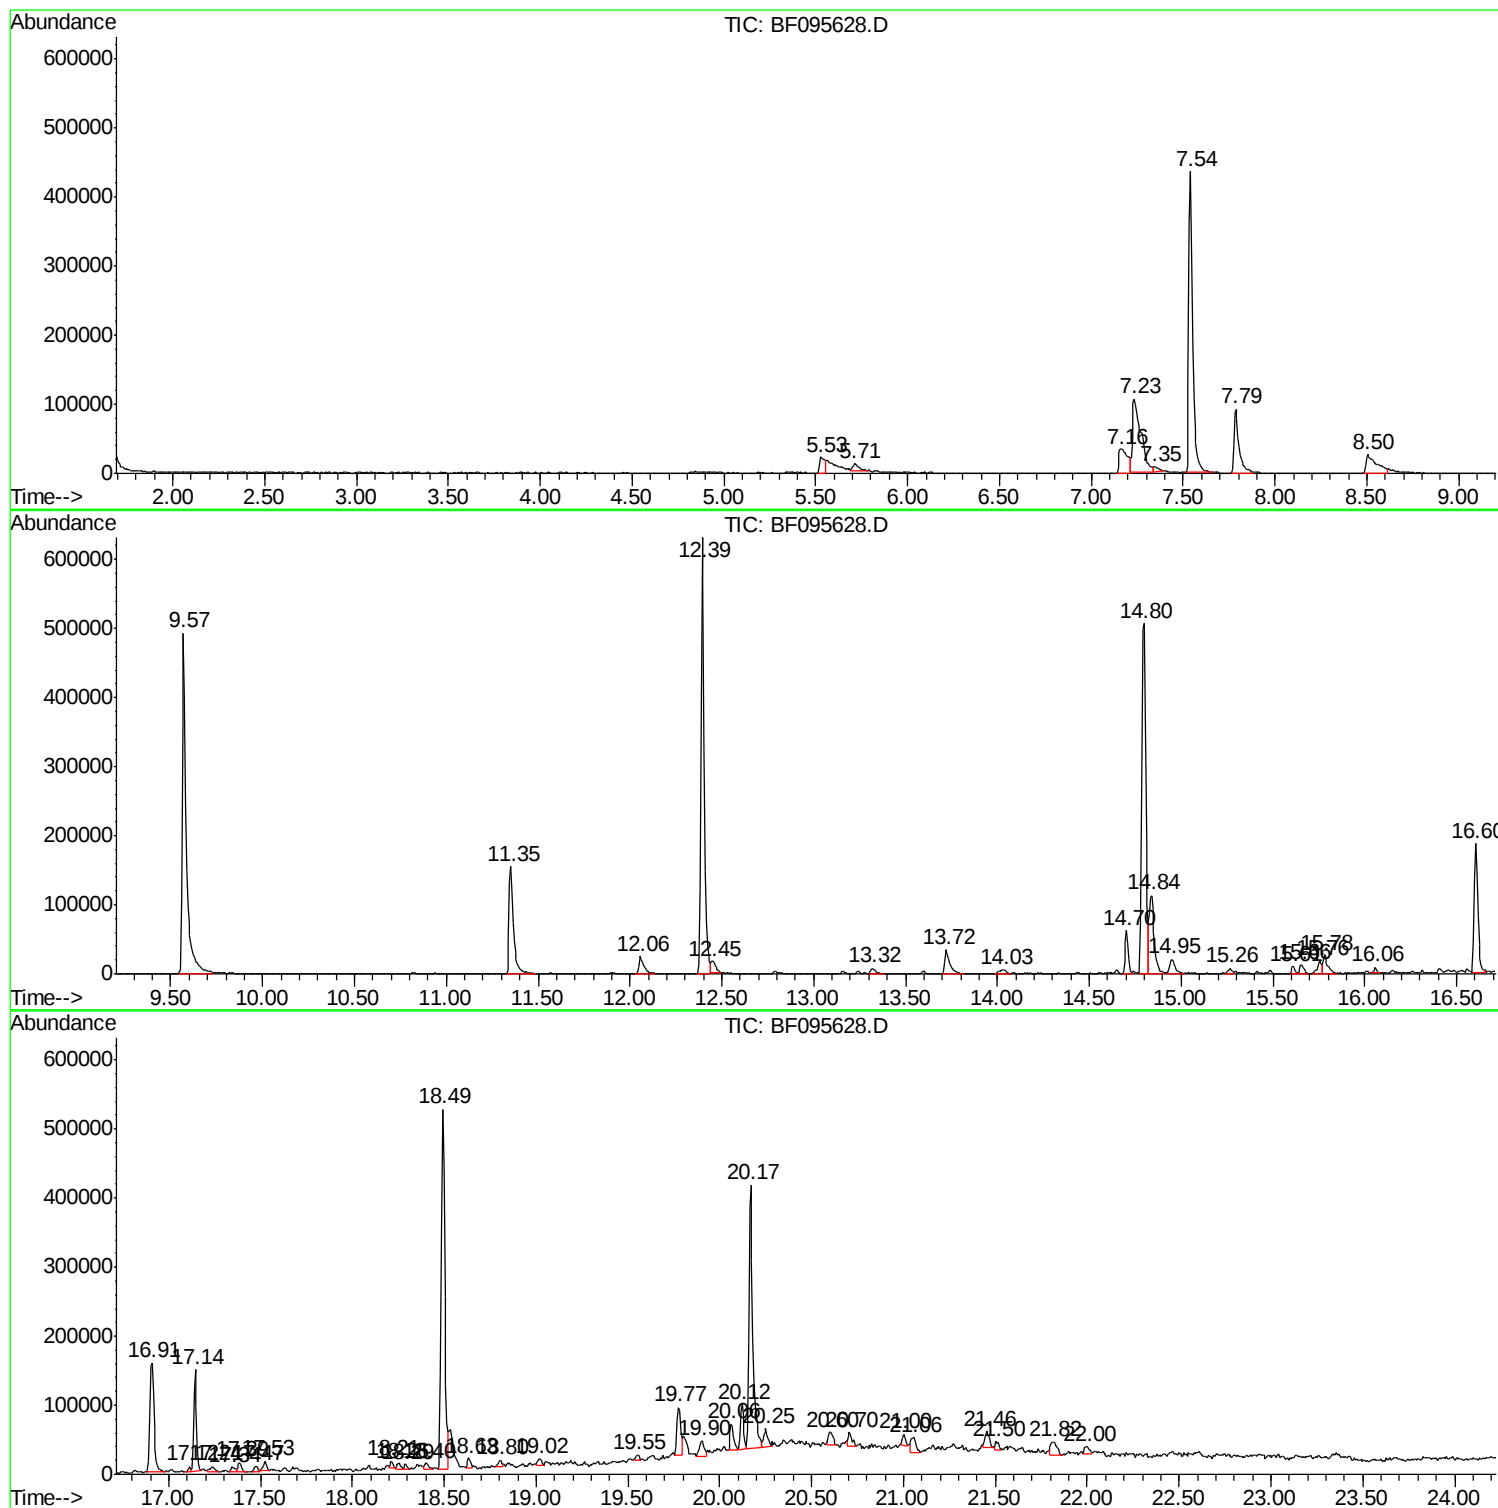

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF060117\
Data File : BF095628.D
Acq On : 2 Jun 2017 10:18
Operator : SJ/MA
Sample : I3415-03 10X
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
E2-T6-ESW










Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF050217.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown7.23 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
7.23	11.00 ng	337278	1,4-Dichlorobenzene-d4	7.54

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	35
2		(E)-3-Chloro-2-methyl-2-pentenal	132	C6H9ClO	031357-76-3	25
3		1,3,5-Trifluorobenzene	132	C6H3F3	000372-38-3	9
4		5-Fluoro-2-chloropyrimidine	132	C4H2ClFN2	062802-42-0	9
5		5-Aminoindole	132	C8H8N2	005192-03-0	9

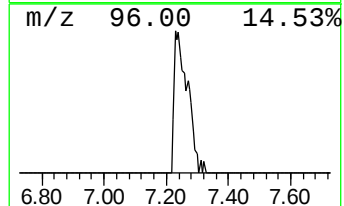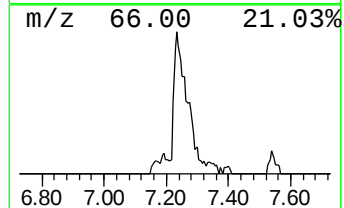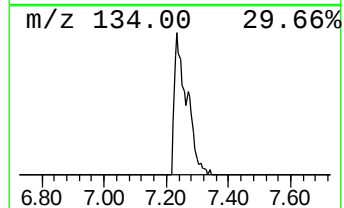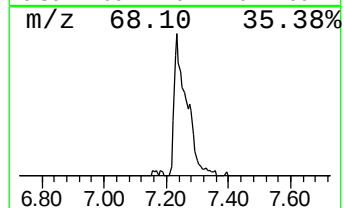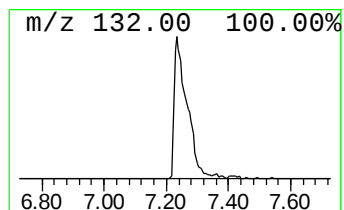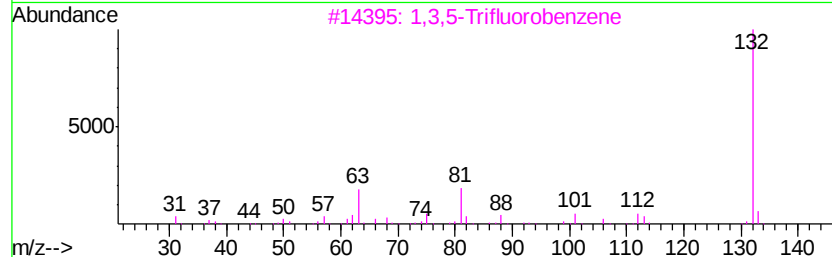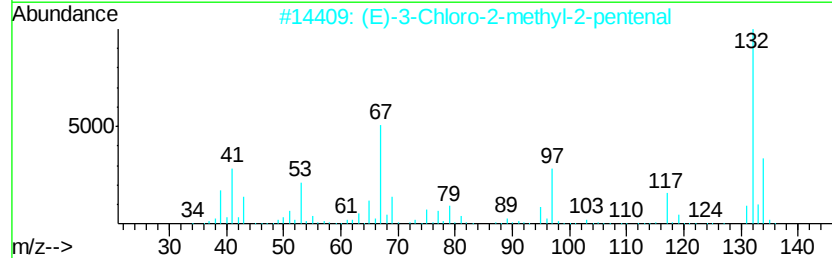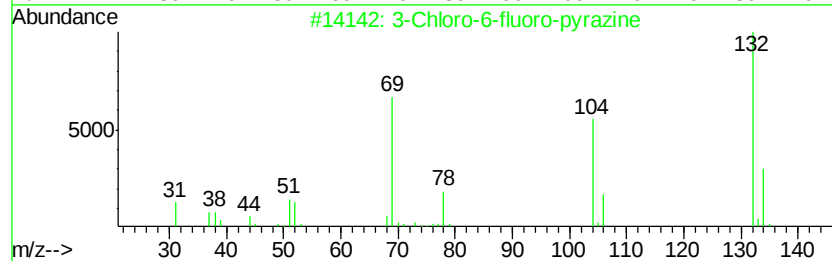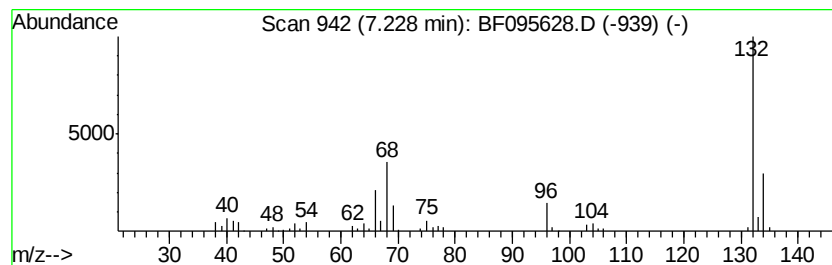

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF060117\
Data File : BF095628.D
Acq On : 2 Jun 2017 10:18
Operator : SJ/MA
Sample : I3415-03 10X
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
E2-T6-ESW

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF050217.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown7.23	7.23	11.0	ng	337278	1	7.54	613073	20.0