


Data Path : Z:\HPCHEM1\BNA_F\Data\BF060117\
 Data File : BF095592.D
 Acq On : 1 Jun 2017 13:10
 Operator : SJ/MA
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF050217.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Jun 01 18:51:16 2017

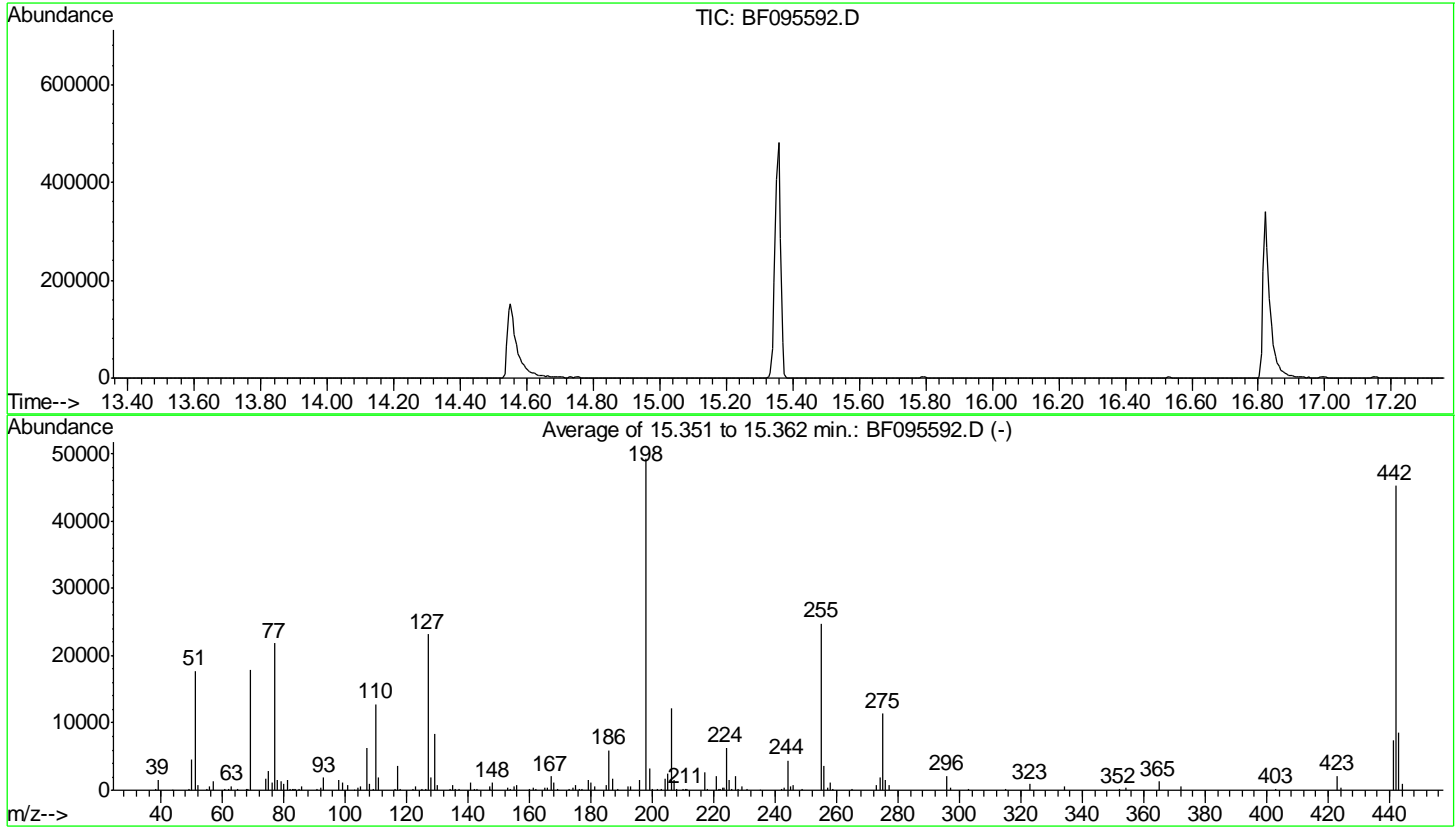

AutoFind: Scans 2323, 2324, 2325; Background Corrected with Scan 2316

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.0	17772	PASS
68	69	0.00	2	0.6	111	PASS
69	198	0.00	100	36.2	17861	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	47.1	23222	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	49309	PASS
199	198	5	9	6.7	3313	PASS
275	198	10	60	23.1	11383	PASS
365	198	1	100	2.5	1252	PASS
441	442	0.01	24	16.5	7464	PASS
442	198	50	100	91.7	45232	PASS
443	442	15	24	18.9	8566	PASS