


Data Path : Z:\HPCHEM1\BNA_F\Data\BF060117\
 Data File : BF095611.D
 Acq On : 2 Jun 2017 00:59
 Operator : SJ/MA
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF050217.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Jun 01 18:51:16 2017

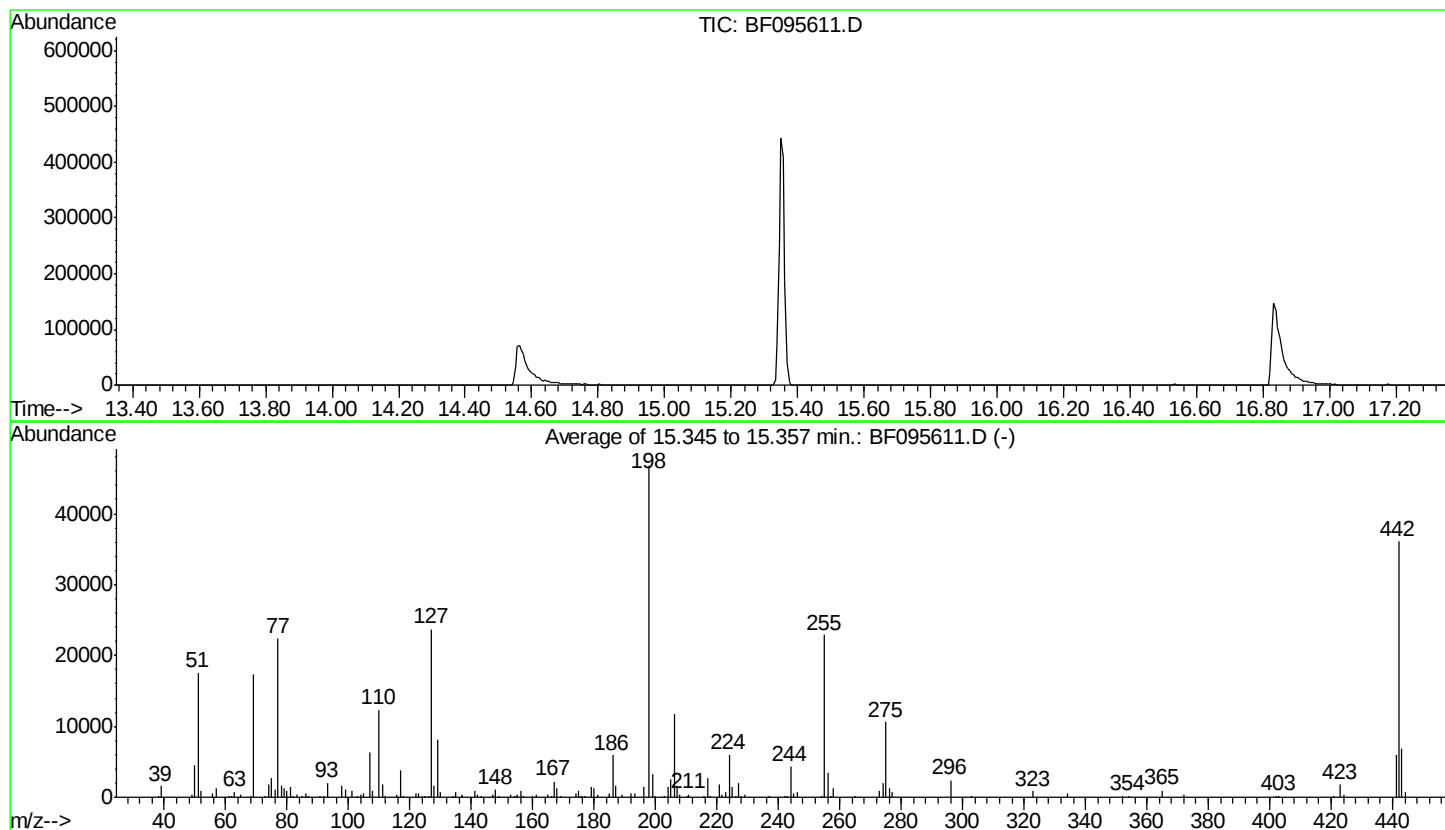

AutoFind: Scans 2322, 2323, 2324; Background Corrected with Scan 2317

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.6	17585	PASS
68	69	0.00	2	1.2	213	PASS
69	198	0.00	100	37.1	17334	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	50.8	23752	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	46784	PASS
199	198	5	9	6.9	3243	PASS
275	198	10	60	22.6	10582	PASS
365	198	1	100	2.1	973	PASS
441	442	0.01	24	16.7	6007	PASS
442	198	50	100	77.1	36058	PASS
443	442	15	24	18.8	6791	PASS