
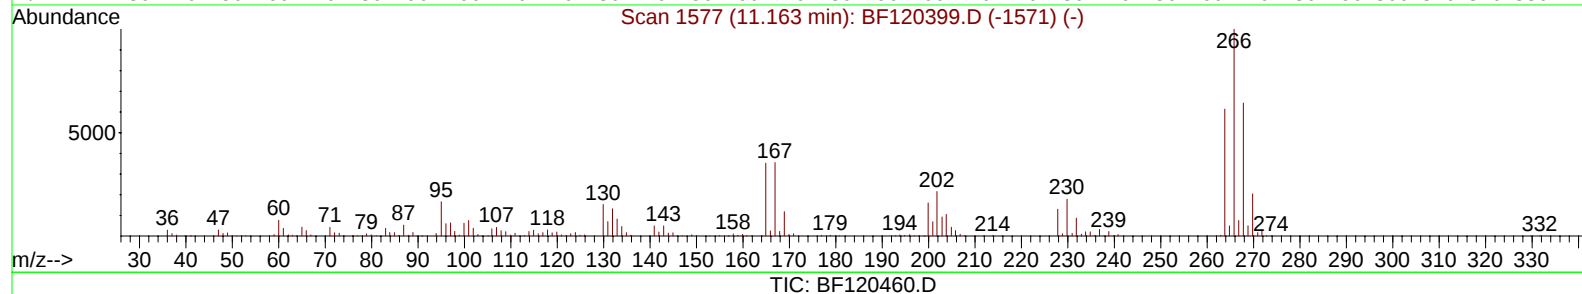
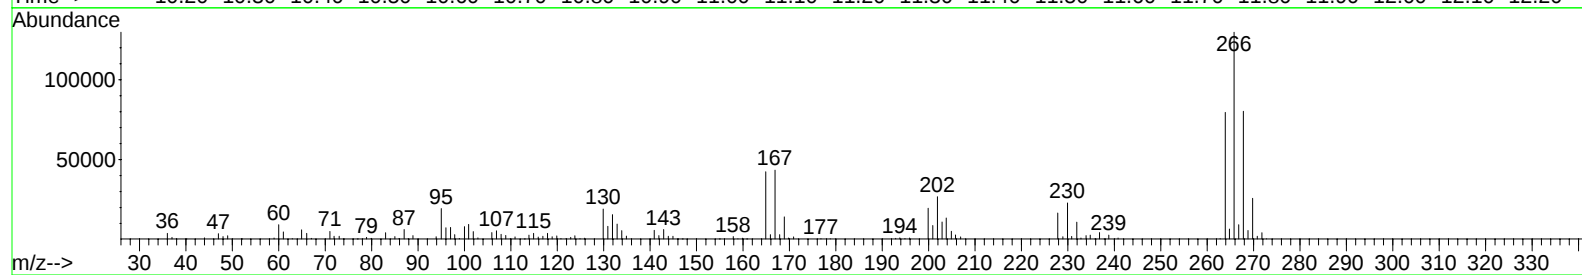


Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF060120\
 Data File : BF120460.D
 Acq On : 1 Jun 2020 9:49
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 01 17:05:18 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF052820.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri May 29 12:39:43 2020
 Response via : Initial Calibration

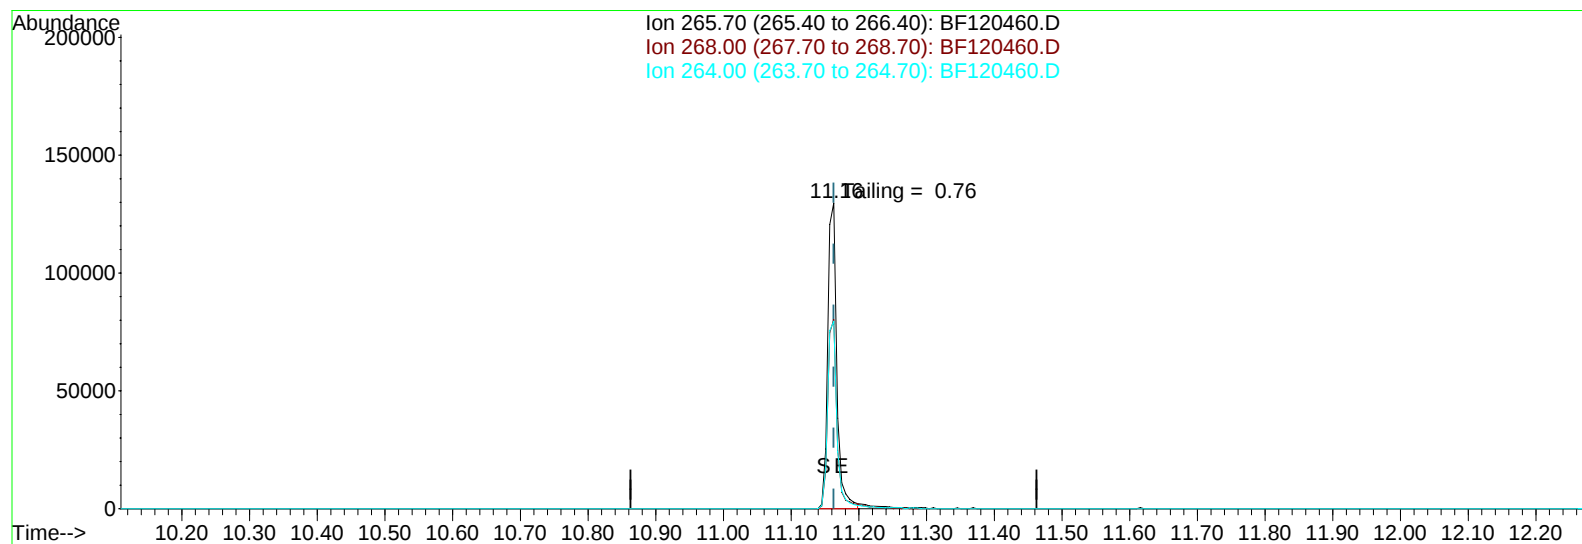

(70) Pentachlorophenol (C)




11.163min (+0.000) 36191.58ng

response 125119

Ion	Exp%	Act%
265.70	100	100
268.00	64.40	61.86
264.00	61.40	61.33
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF060120\
 Data File : BF120460.D
 Acq On : 1 Jun 2020 9:49
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 01 17:05:18 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF052820.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri May 29 12:39:43 2020
 Response via : Initial Calibration

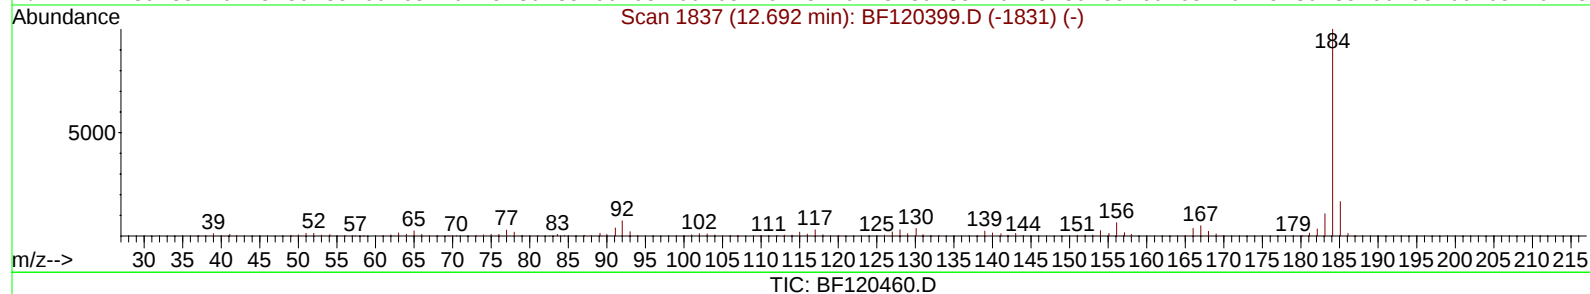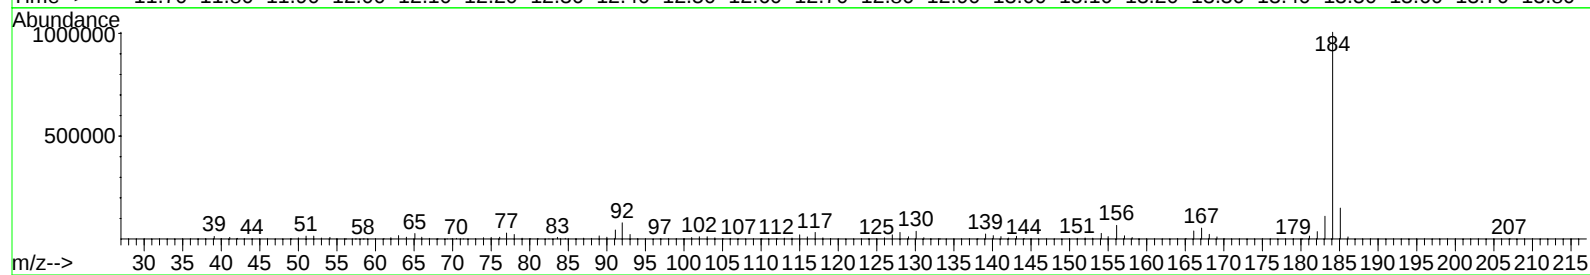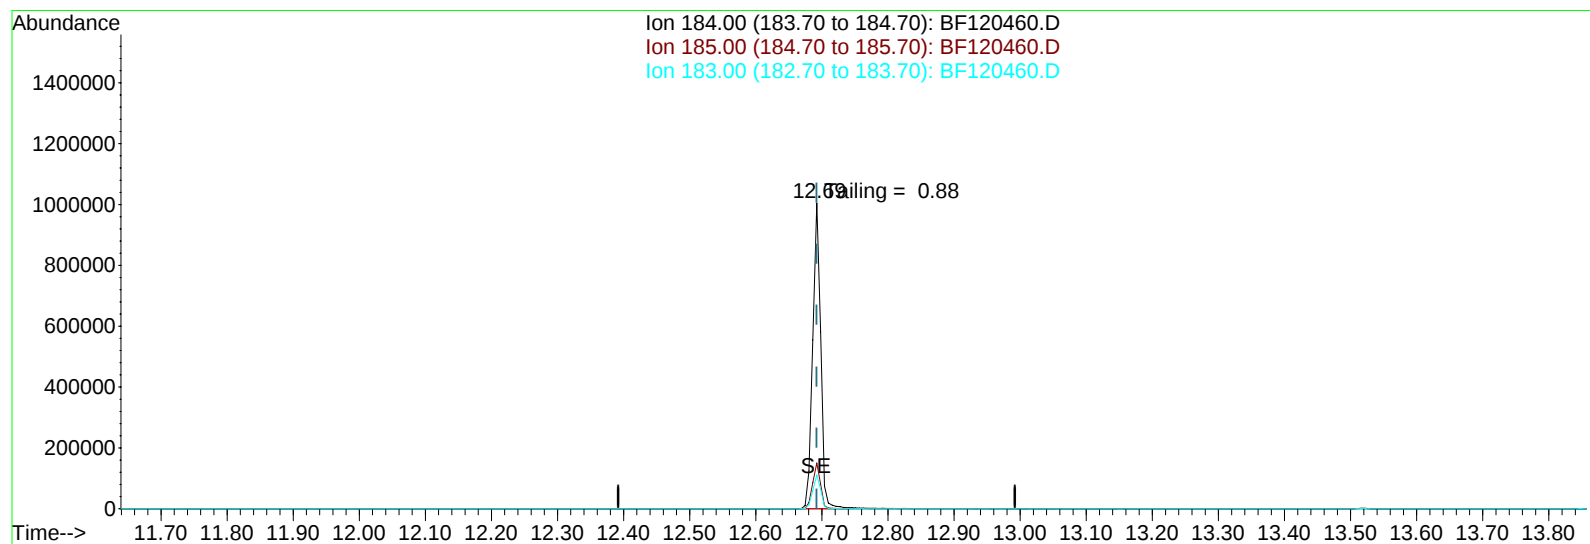

(77) Benzidine

12.692min (+0.000) 0.00ng

response 858164

Ion	Exp%	Act%
184.00	100	100
185.00	16.70	14.97
183.00	10.70	11.06
0.00	0.00	0.00