


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF060120\
 Data File : BF120460.D
 Acq On : 1 Jun 2020 9:49
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF052820.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Jun 02 11:37:51 2020

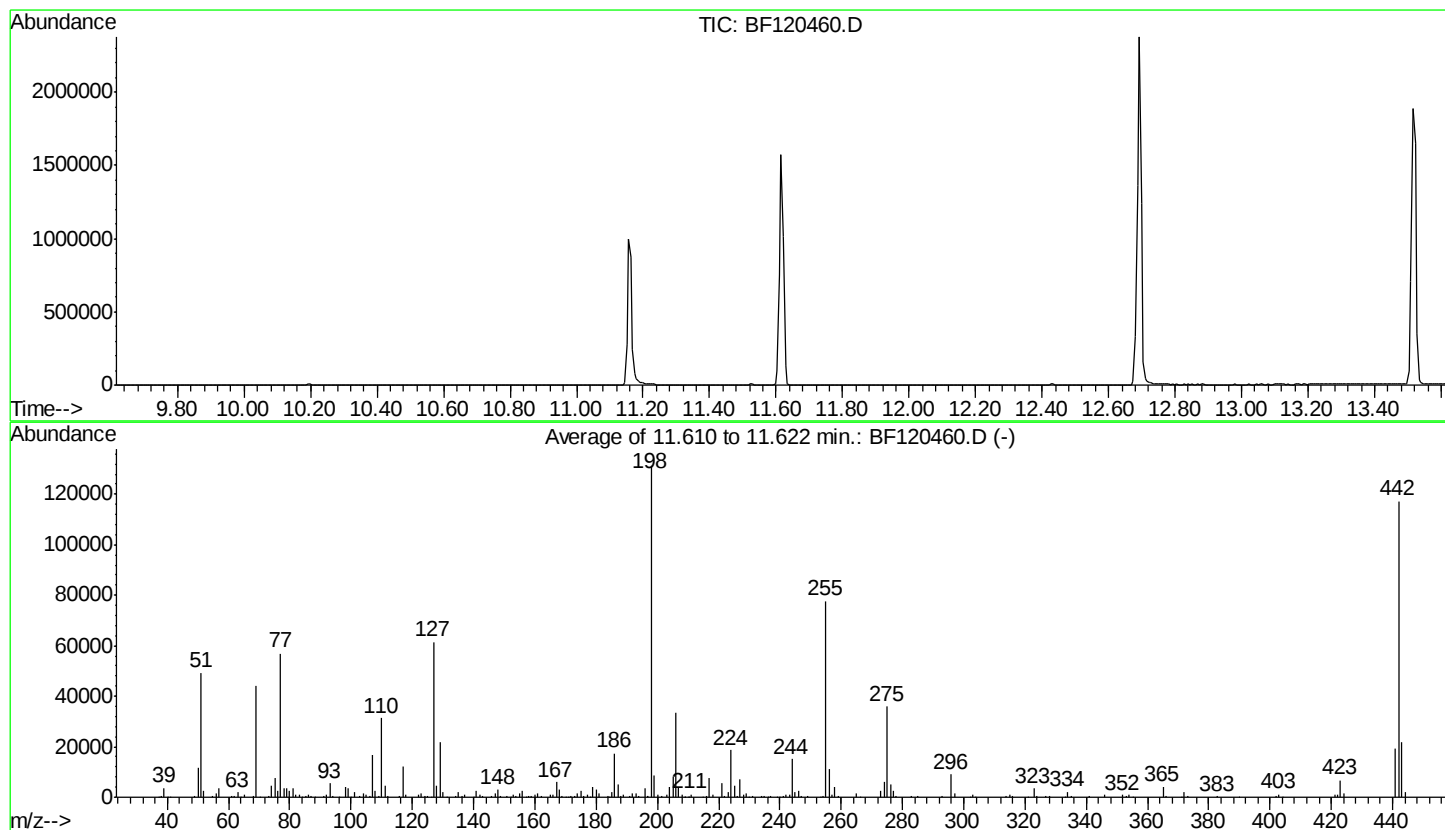

AutoFind: Scans 1653, 1654, 1655; Background Corrected with Scan 1648

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.6	49338	PASS
68	69	0.00	2	1.7	743	PASS
69	198	0.00	100	33.7	44288	PASS
70	69	0.00	2	0.3	140	PASS
127	198	10	80	46.8	61448	PASS
197	198	0.00	2	0.5	613	PASS
198	198	100	100	100.0	131338	PASS
199	198	5	9	6.6	8680	PASS
275	198	10	60	27.3	35802	PASS
365	198	1	100	3.3	4311	PASS
441	198	0.01	100	14.5	19042	PASS
442	198	50	100	89.3	117298	PASS
443	442	15	24	18.4	21620	PASS