

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF060122\
 Data File : BF128621.D
 Acq On : 01 Jun 2022 13:21
 Operator : CG\JU
 Sample : N2987-11
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 RB-220516

Quant Time: Jun 02 04:36:05 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052622.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri May 27 01:51:59 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	6.834	152	102587	20.000	ng	0.00
21) Naphthalene-d8	8.116	136	359026	20.000	ng	#-0.01
39) Acenaphthene-d10	9.869	164	205070	20.000	ng	-0.01
64) Phenanthrene-d10	11.357	188	406331	20.000	ng	#-0.01
76) Chrysene-d12	13.998	240	282075	20.000	ng	#-0.01
86) Perylene-d12	15.463	264	192646	20.000	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.493	112	400520	64.669	ng	0.04
7) Phenol-d6	6.516	99	319637	40.477	ng	0.05
23) Nitrobenzene-d5	7.398	82	712910	114.550	ng	-0.01
42) 2,4,6-Tribromophenol	10.669	330	336924	172.612	ng	0.00
45) 2-Fluorobiphenyl	9.192	172	1381323	109.434	ng	-0.01
79) Terphenyl-d14	12.951	244	1782204	122.065	ng	0.00
Target Compounds						
36) 4-Chloro-3-methylphenol	8.704	107	22223	4.089	ng	Qvalue 96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF060122\
Data File : BF128621.D
Acq On : 01 Jun 2022 13:21
Operator : CG\JU
Sample : N2987-11
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
RB-220516

Quant Time: Jun 02 04:36:05 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri May 27 01:51:59 2022
Response via : Initial Calibration




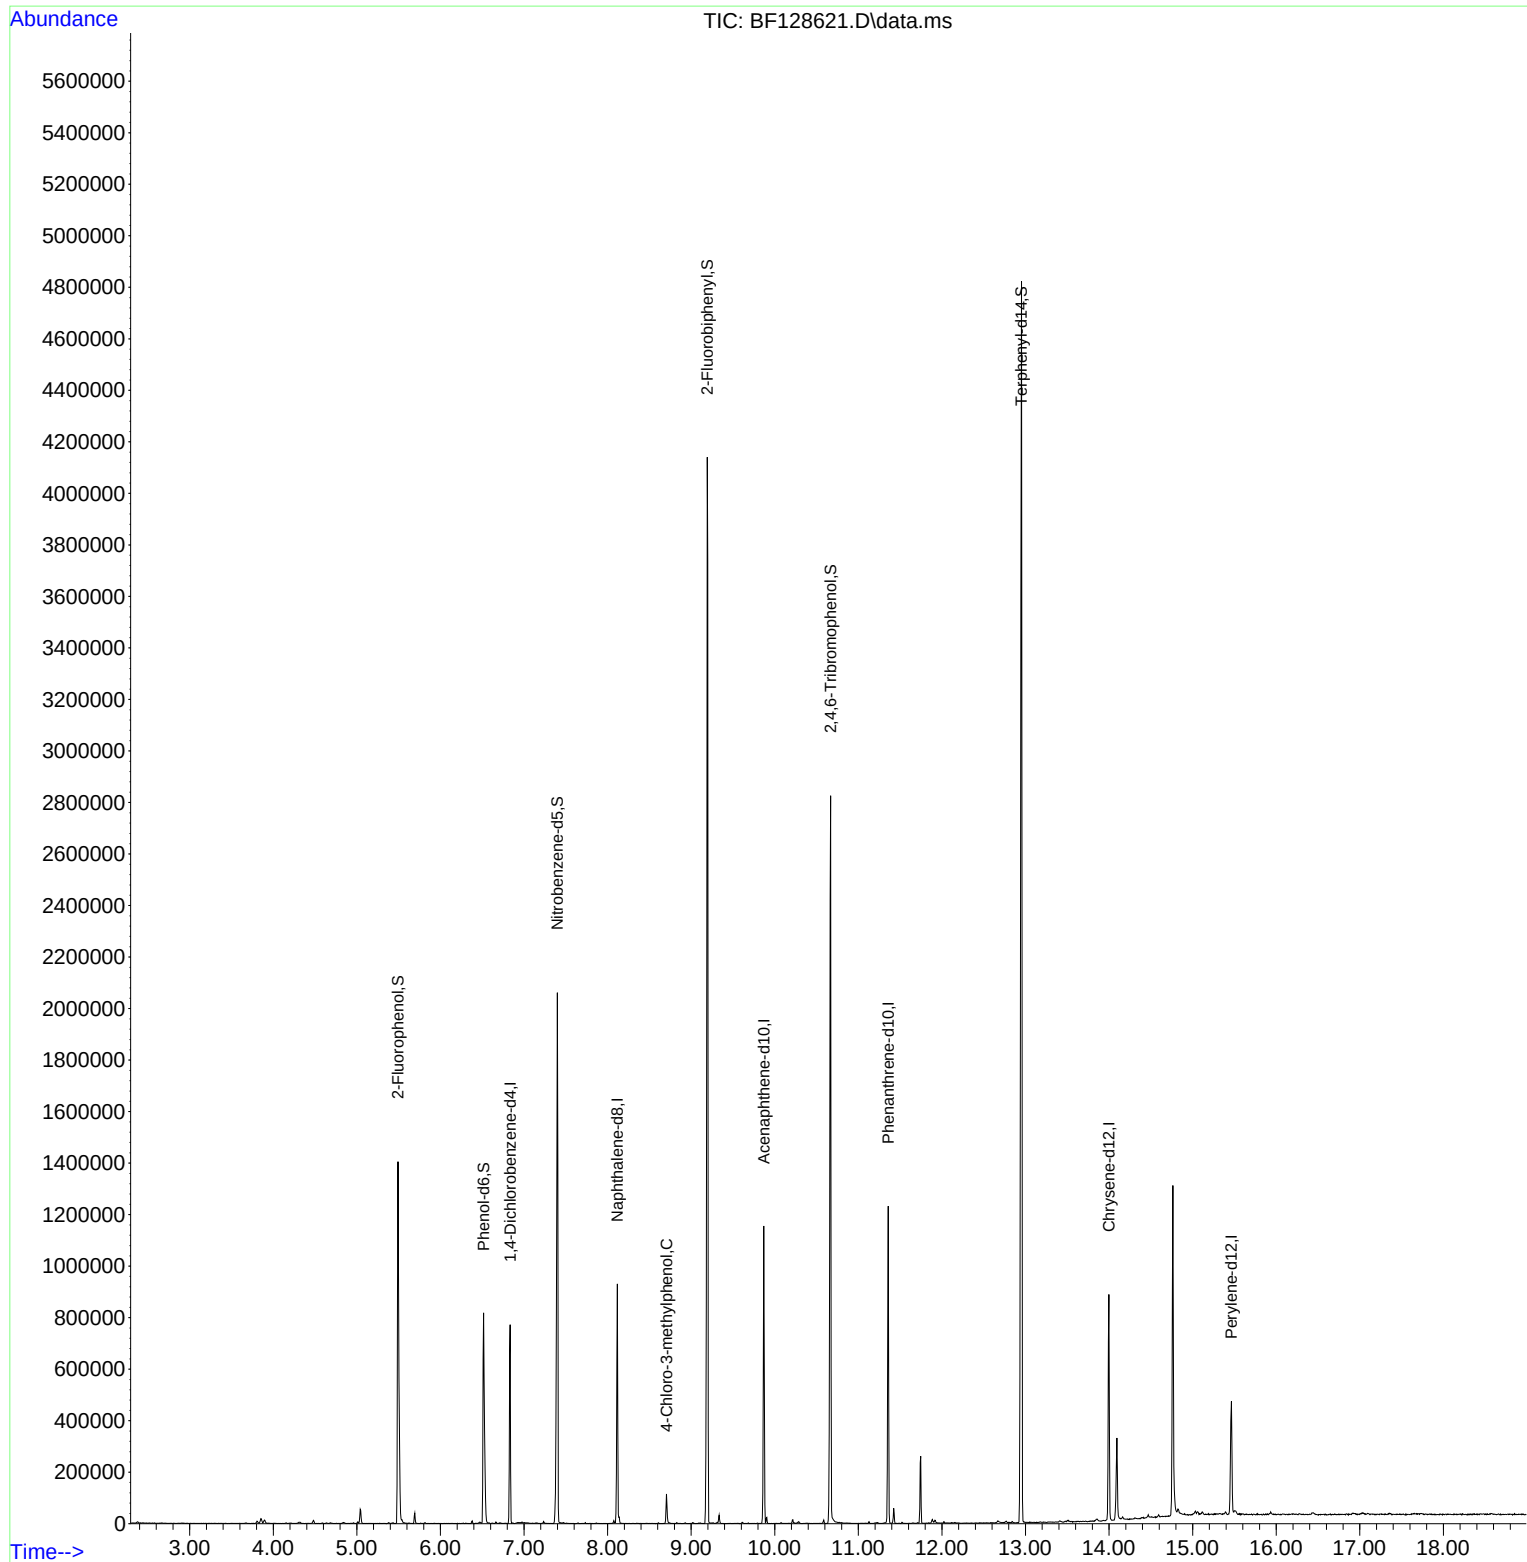


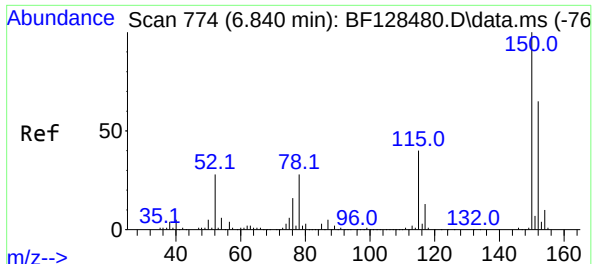

#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.834 min Scan# 71
Delta R.T. -0.006 min
Lab File: BF128621.D
Acq: 01 Jun 2022 13:21




Instrument :
BNA_F
ClientSampleId :
RB-220516


Tgt Ion:152 Resp: 102587
Ion Ratio Lower Upper
152 100
150 156.4 123.7 185.5
115 66.5 49.9 74.9

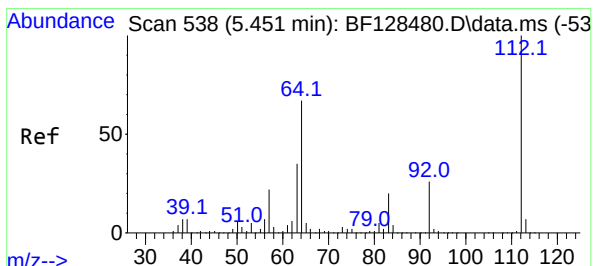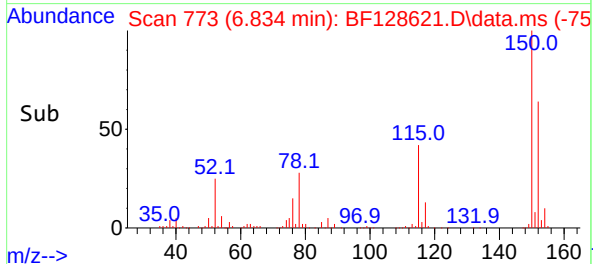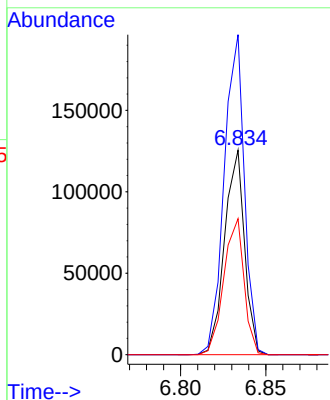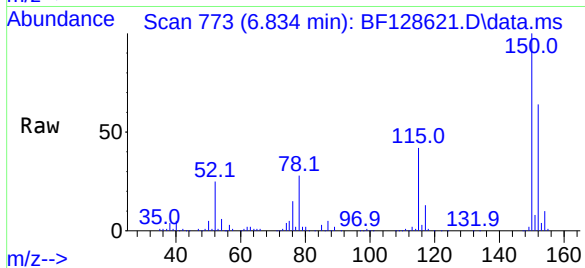

#5
2-Fluorophenol
Concen: 64.669 ng
RT: 5.493 min Scan# 545
Delta R.T. 0.041 min
Lab File: BF128621.D
Acq: 01 Jun 2022 13:21

Tgt Ion:112 Resp: 400520
Ion Ratio Lower Upper
112 100
64 67.7 53.3 79.9
63 39.2 28.0 42.0


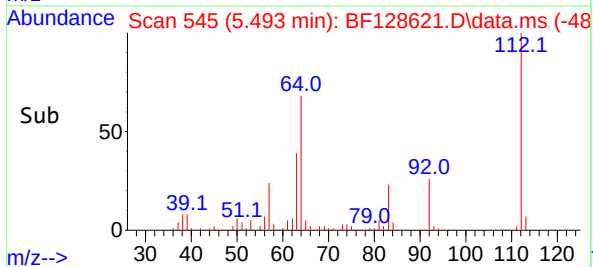
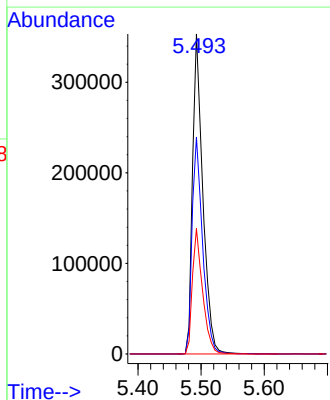
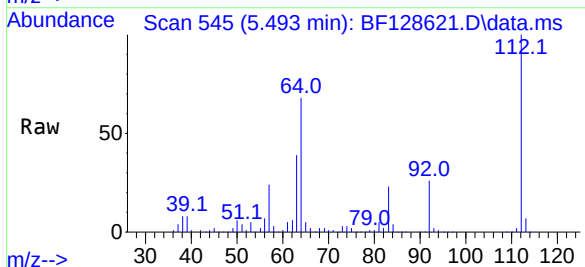


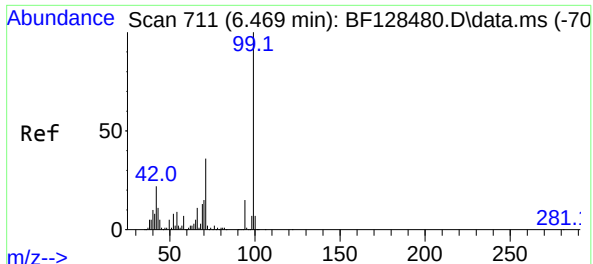

#7
Phenol-d6
Concen: 40.477 ng
RT: 6.516 min Scan# 711
Delta R.T. 0.047 min
Lab File: BF128621.D
Acq: 01 Jun 2022 13:21




Instrument :
BNA_F
ClientSampleId :
RB-220516


Tgt Ion: 99 Resp: 319637
Ion Ratio Lower Upper
99 100
42 23.6 17.3 25.9
71 42.0 28.9 43.3

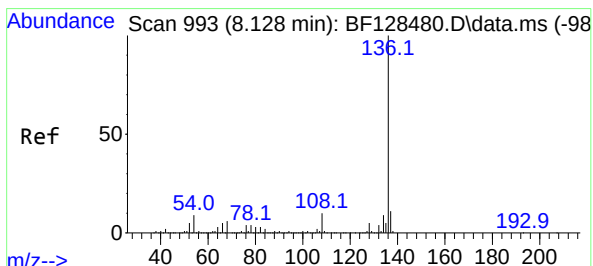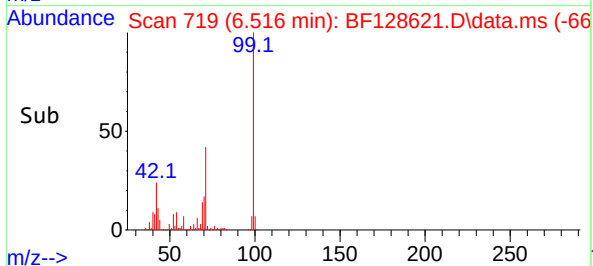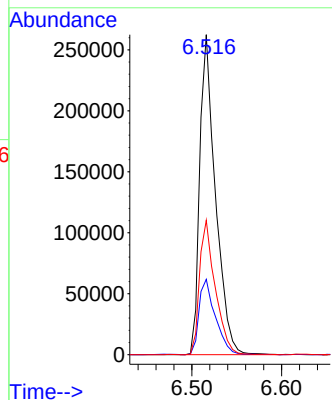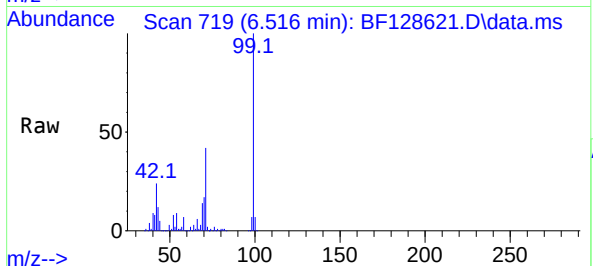

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 8.116 min Scan# 991
Delta R.T. -0.012 min
Lab File: BF128621.D
Acq: 01 Jun 2022 13:21

Tgt Ion: 136 Resp: 359026
Ion Ratio Lower Upper
136 100
137 11.2 8.8 13.2
54 8.7 7.5 11.3
68 4.5 4.7 7.1#

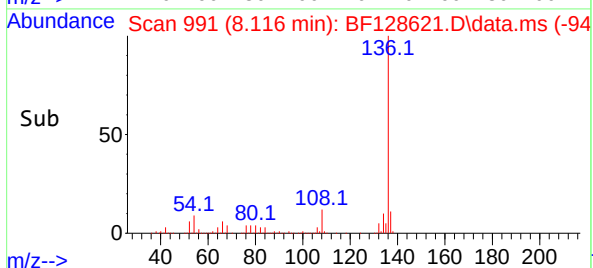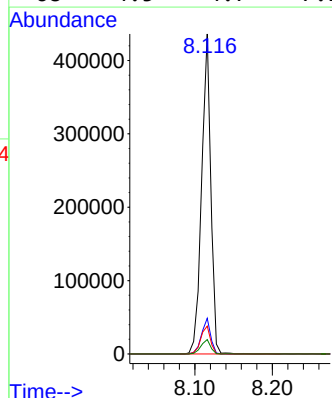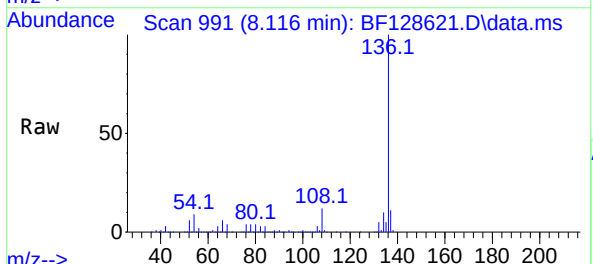

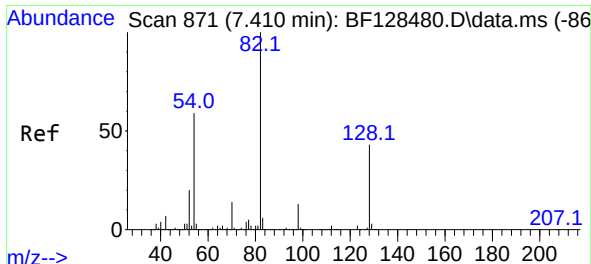

#23

Nitrobenzene-d5

Concen: 114.550 ng

RT: 7.398 min Scan# 8

Delta R.T. -0.012 min

Lab File: BF128621.D

Acq: 01 Jun 2022 13:21

Instrument :

BNA_F

ClientSampleId :

RB-220516





Tgt Ion: 82 Resp: 712910

Ion Ratio Lower Upper

82 100

128 40.0 34.0 51.0

54 60.3 46.9 70.3

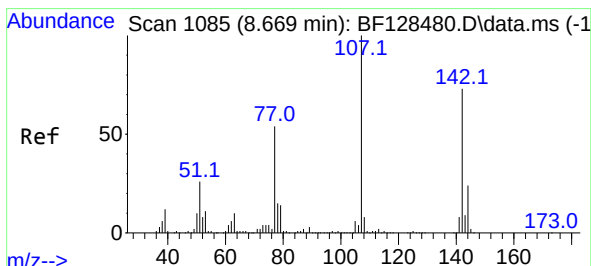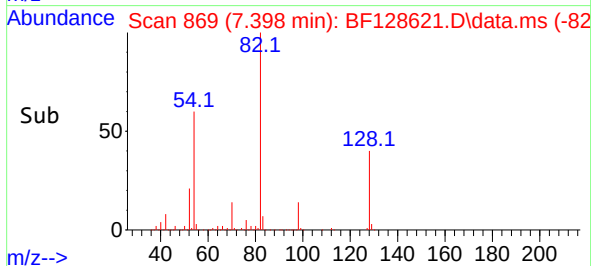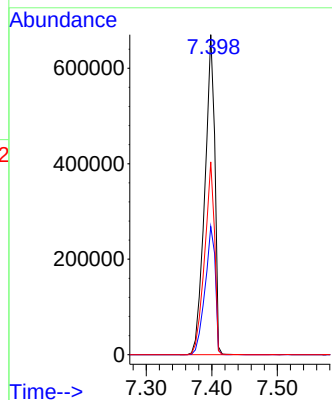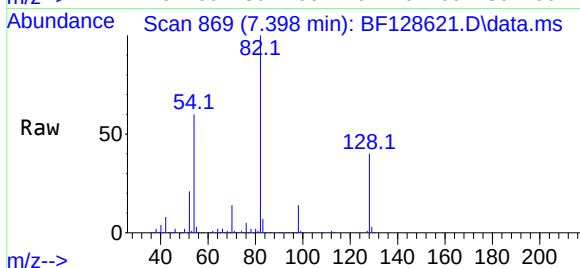

#36

4-Chloro-3-methylphenol

Concen: 4.089 ng

RT: 8.704 min Scan# 1091

Delta R.T. 0.035 min

Lab File: BF128621.D

Acq: 01 Jun 2022 13:21




Tgt Ion: 107 Resp: 22223


Ion Ratio Lower Upper

107 100

144 23.0 19.5 29.3

142 69.0 58.2 87.4

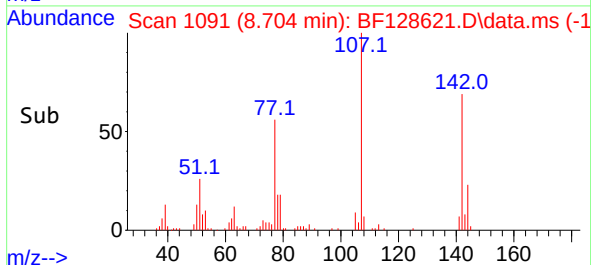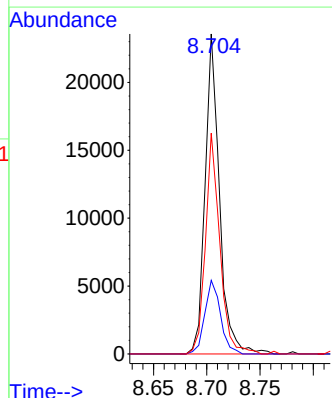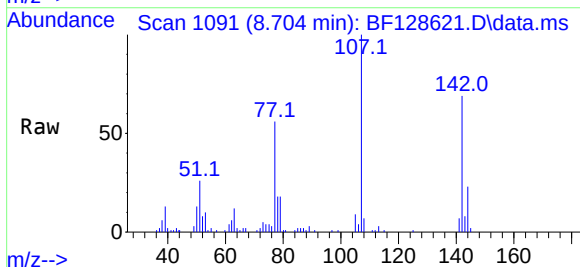

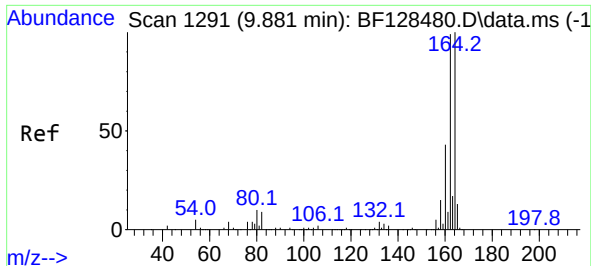

#39

Acenaphthene-d10

Concen: 20.000 ng

RT: 9.869 min Scan# 1

Delta R.T. -0.012 min

Lab File: BF128621.D

Acq: 01 Jun 2022 13:21

Instrument :

BNA_F

ClientSampleId :

RB-220516





Tgt Ion:164 Resp: 205070

Ion Ratio Lower Upper

164 100

162 102.1 79.5 119.3

160 46.2 34.2 51.4

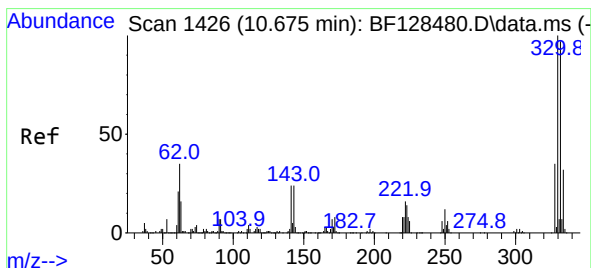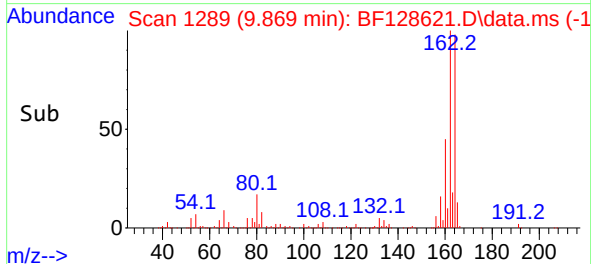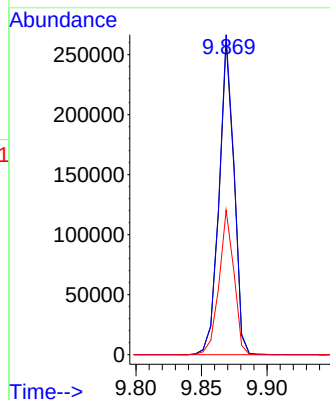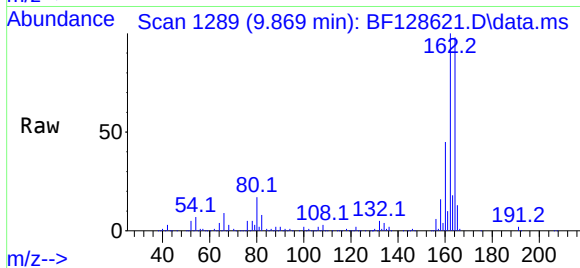

#42

2,4,6-Tribromophenol

Concen: 172.612 ng

RT: 10.669 min Scan# 1425

Delta R.T. -0.006 min

Lab File: BF128621.D

Acq: 01 Jun 2022 13:21




Tgt Ion:330 Resp: 336924


Ion Ratio Lower Upper

330 100

332 95.7 76.8 115.2

141 34.7 28.0 42.0

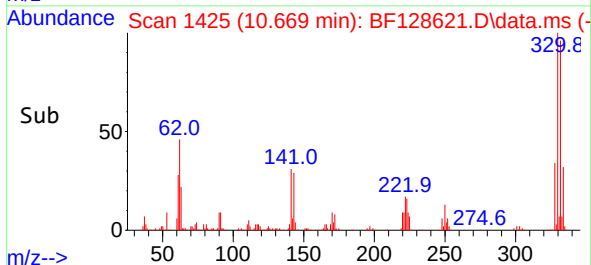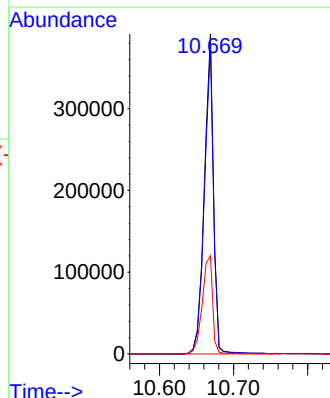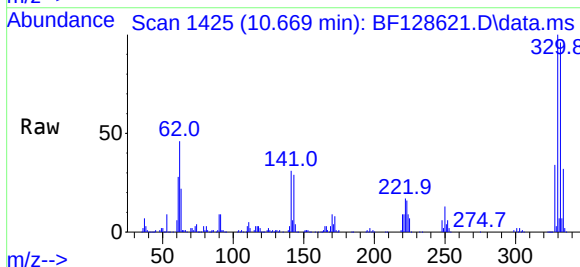

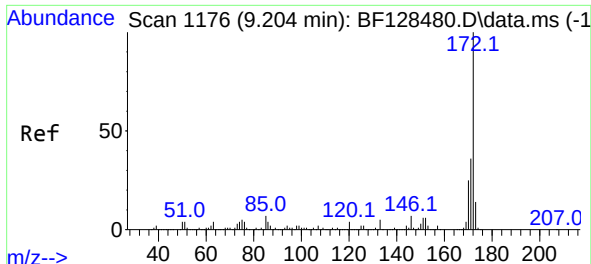

#45

2-Fluorobiphenyl

Concen: 109.434 ng

RT: 9.192 min Scan# 1174

Delta R.T. -0.012 min

Lab File: BF128621.D

Acq: 01 Jun 2022 13:21

Instrument :

BNA_F

ClientSampleId :

RB-220516





Tgt Ion:172 Resp: 1381323

Ion Ratio Lower Upper

172 100

171 35.7 28.8 43.2

170 23.5 19.8 29.8

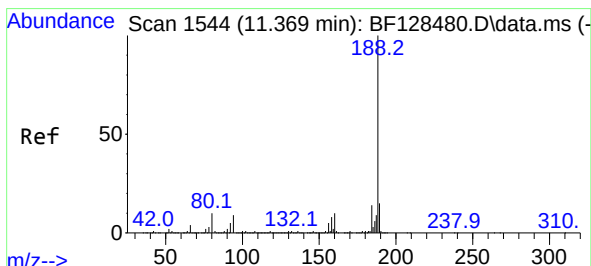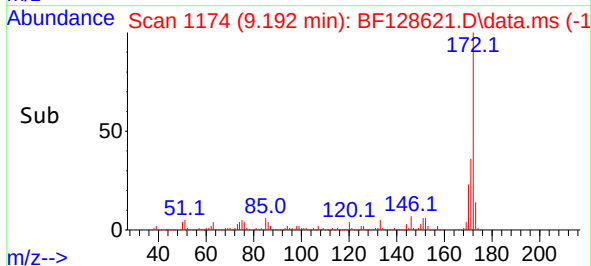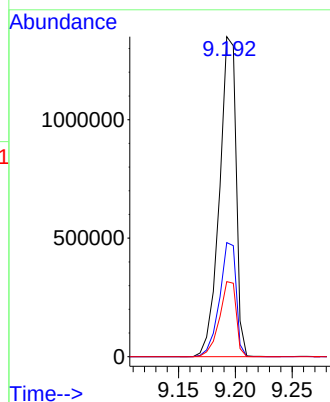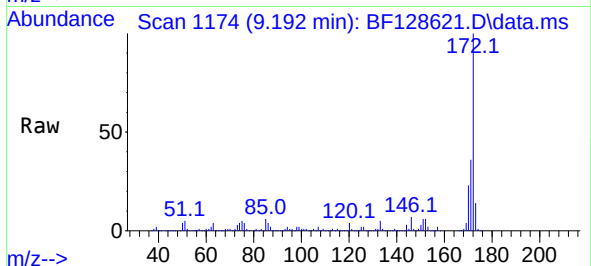

#64

Phenanthrene-d10

Concen: 20.000 ng

RT: 11.357 min Scan# 1542

Delta R.T. -0.012 min

Lab File: BF128621.D

Acq: 01 Jun 2022 13:21




Tgt Ion:188 Resp: 406331


Ion Ratio Lower Upper

188 100

94 7.0 7.0 10.6#

80 7.4 7.6 11.4#


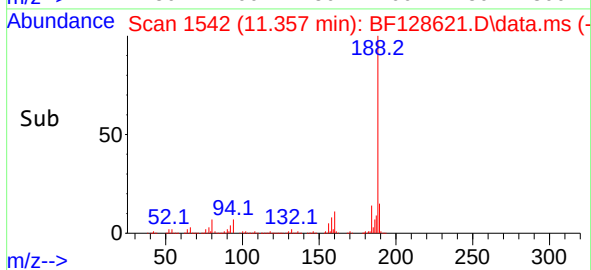
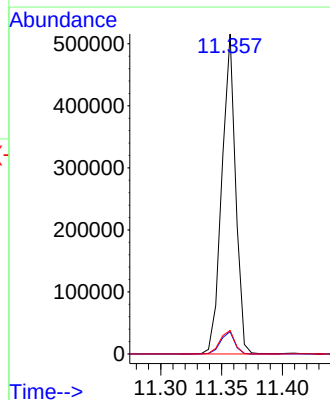
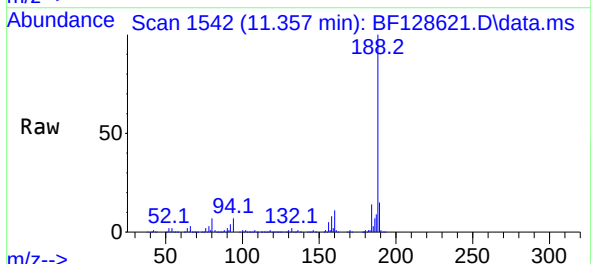


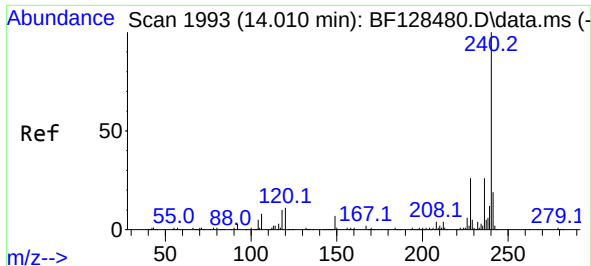

#76
Chrysene-d12
Concen: 20.000 ng
RT: 13.998 min Scan# 1991
Delta R.T. -0.012 min
Lab File: BF128621.D
Acq: 01 Jun 2022 13:21




Instrument :
BNA_F
ClientSampleId :
RB-220516


Tgt Ion:240 Resp: 282075
Ion Ratio Lower Upper
240 100
120 7.2 8.9 13.3#
236 25.9 20.8 31.2

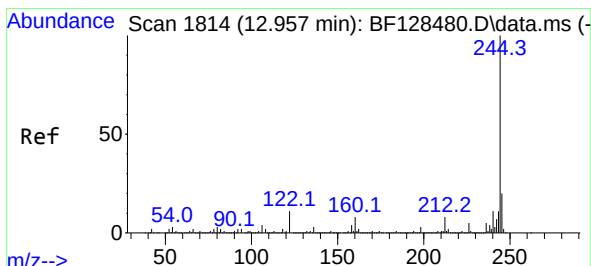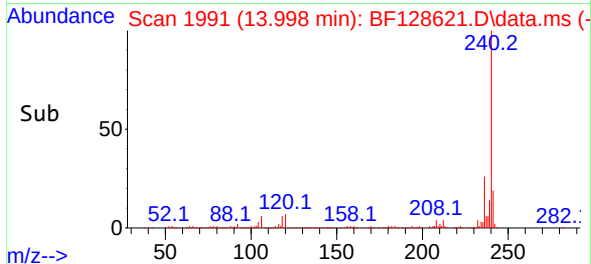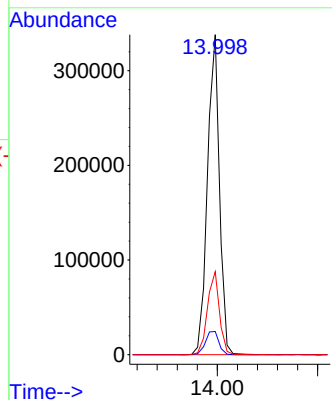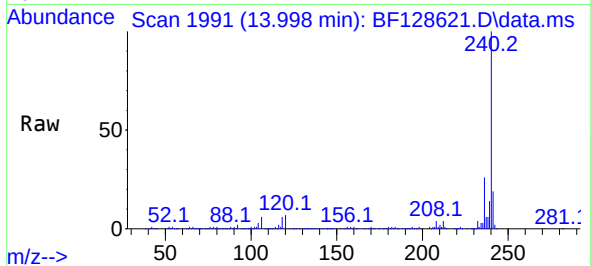

#79
Terphenyl-d14
Concen: 122.065 ng
RT: 12.951 min Scan# 1813
Delta R.T. -0.006 min
Lab File: BF128621.D
Acq: 01 Jun 2022 13:21


Tgt Ion:244 Resp: 1782204
Ion Ratio Lower Upper
244 100
212 7.5 6.1 9.1
122 10.4 8.8 13.2

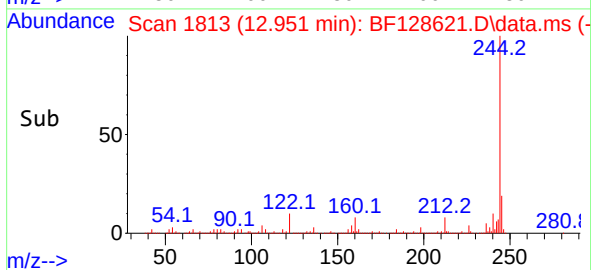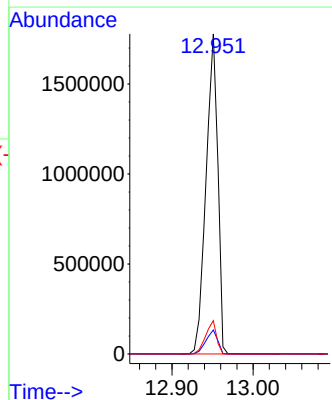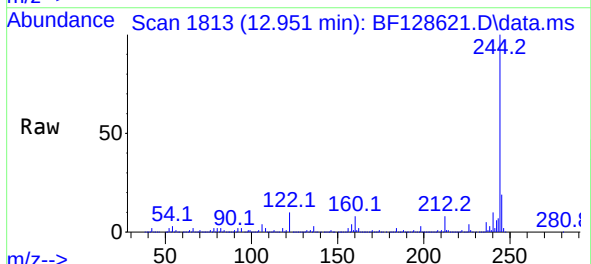

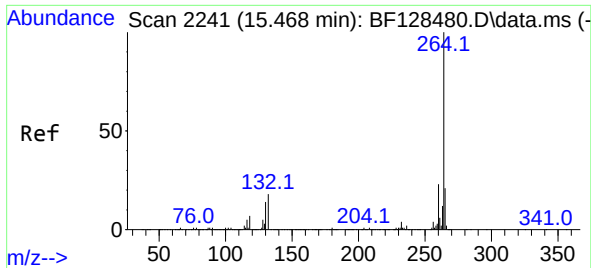

#86
Perylene-d12
Concen: 20.000 ng
RT: 15.463 min Scan# 21
Delta R.T. -0.006 min
Lab File: BF128621.D
Acq: 01 Jun 2022 13:21

Instrument :
BNA_F
ClientSampleId :
RB-220516

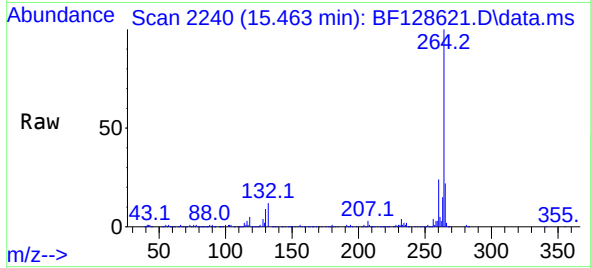

Tgt Ion:264 Resp: 192646

Ion	Ratio	Lower	Upper
264	100		
260	24.1	18.4	27.6
265	21.7	17.2	25.8

