

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF060122\
 Data File : BF128622.D
 Acq On : 01 Jun 2022 13:50
 Operator : CG\JU
 Sample : N3099-01
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 20220417-COMPOSITE-F

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052622.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF128622.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.075	470	474	482	rVB	31121	36892	1.03%	0.164%
2	5.499	542	546	561	rBV	2732763	3147445	88.13%	14.019%
3	6.510	714	718	728	rBV	3001012	3097240	86.73%	13.795%
4	6.834	769	773	776	rVB	769394	647127	18.12%	2.882%
5	7.398	863	869	872	rBV	1916874	1941221	54.36%	8.646%
6	8.116	986	991	994	rBV	811020	747788	20.94%	3.331%
7	9.192	1168	1174	1177	rBV	3861405	3386998	94.84%	15.086%
8	9.869	1284	1289	1292	rBV	1070971	885577	24.80%	3.944%
9	10.663	1418	1424	1427	rBV	2564451	2387062	66.84%	10.632%
10	11.357	1537	1542	1545	rBV	1179948	958636	26.84%	4.270%
11	11.886	1629	1632	1635	rBV2	39904	40610	1.14%	0.181%
12	12.945	1807	1812	1815	rBV	3668420	3571318	100.00%	15.907%
13	13.922	1971	1978	1985	rBV8	25758	63073	1.77%	0.281%
14	13.998	1985	1991	1994	rBV	814665	760045	21.28%	3.385%
15	14.092	2001	2007	2012	rBV	246452	275136	7.70%	1.225%
16	15.463	2234	2240	2244	rBV	409226	505374	14.15%	2.251%




Sum of corrected areas: 22451542

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF060122\
Data File : BF128622.D
Acq On : 01 Jun 2022 13:50
Operator : CG\JU
Sample : N3099-01
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
20220417-COMPOSITE-F

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

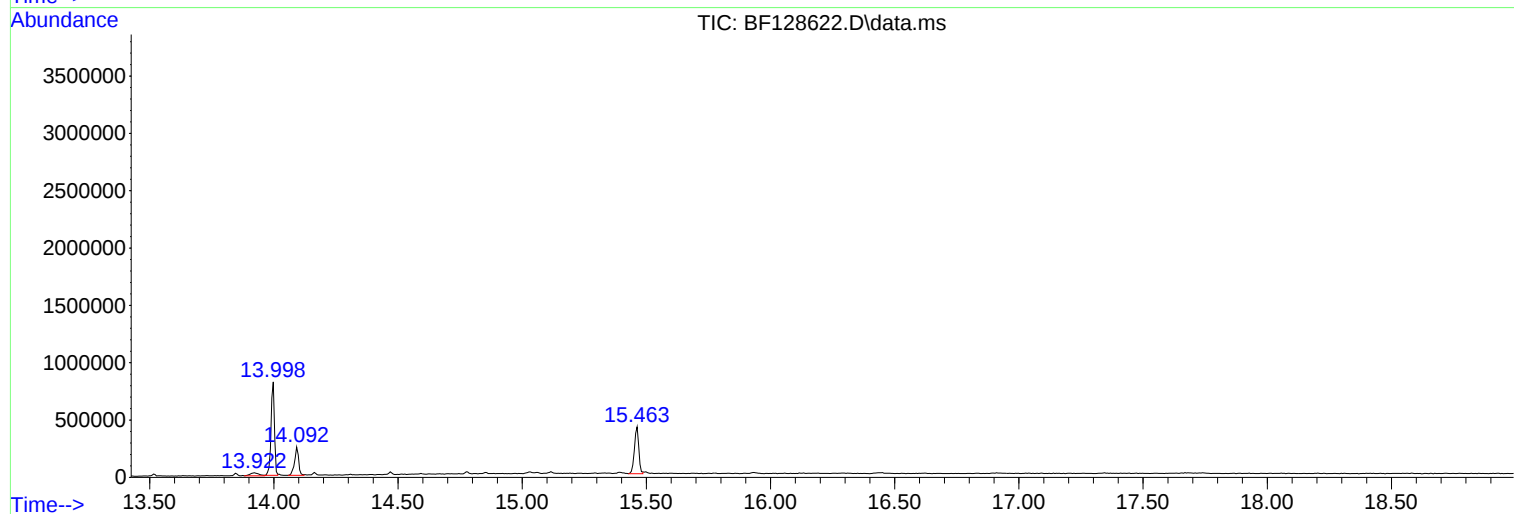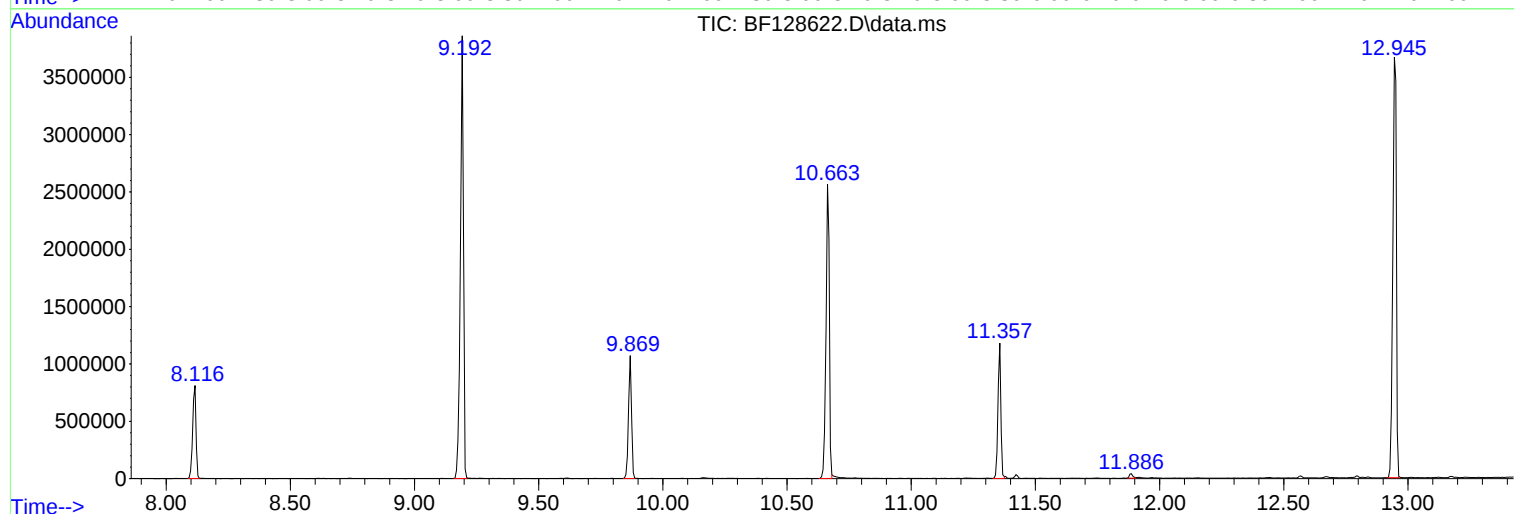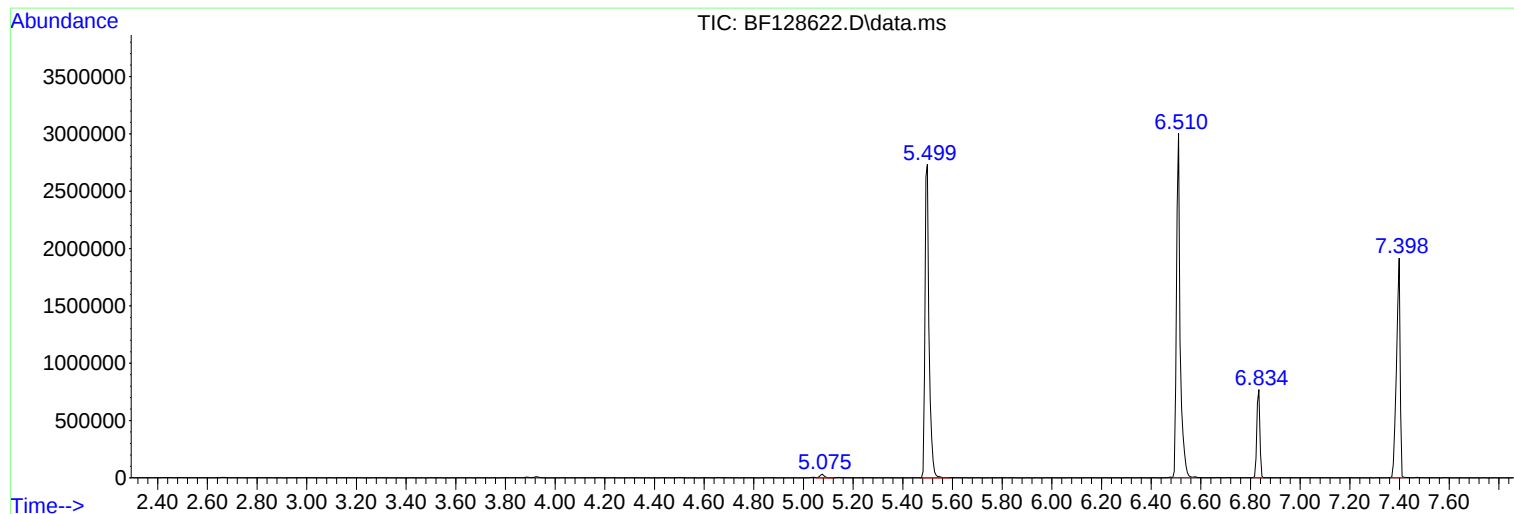

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF060122\
Data File : BF128622.D
Acq On : 01 Jun 2022 13:50
Operator : CG\JU
Sample : N3099-01
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
20220417-COMPOSITE-F










Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Triphenylphosphine oxide Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
14.092	7.24 ng	275136	Chrysene-d12	13.998

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Triphenylphosphine oxide	278	C18H15OP	000791-28-6	98
2			(E)-7-Benzylidene-1-azabicyclo[3...]	293	C15H19NO3S	1000483-83-4	70
3			3-(3,4-Dichlorophenyl)-2-thioxo-...	277	C9H5Cl2NOS2	017046-34-3	38
4			Butylaldehyde, 4-benzyloxy-4-[2,...	278	C16H22O4	149180-87-0	37
5			Formaldehyde, (triphenylphosphor...	304	C19H17N2P	015990-54-2	37

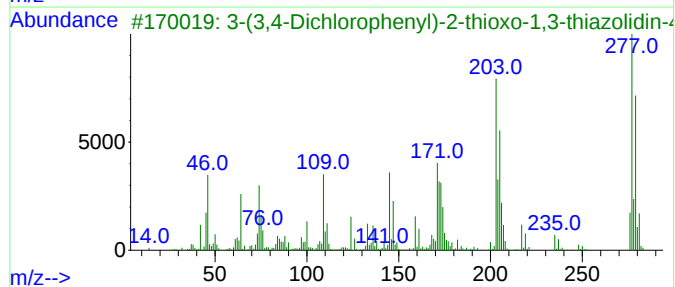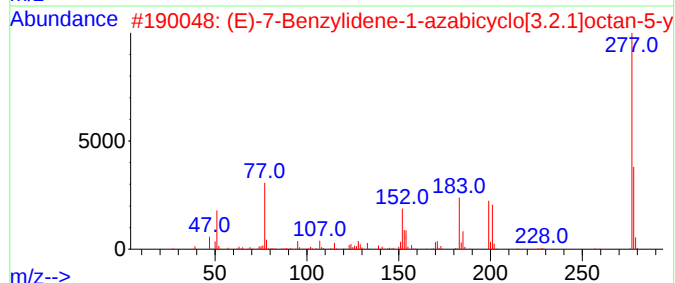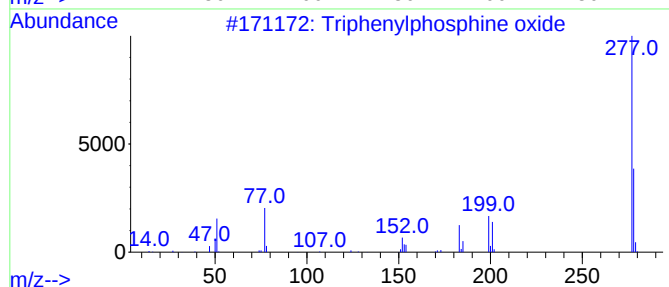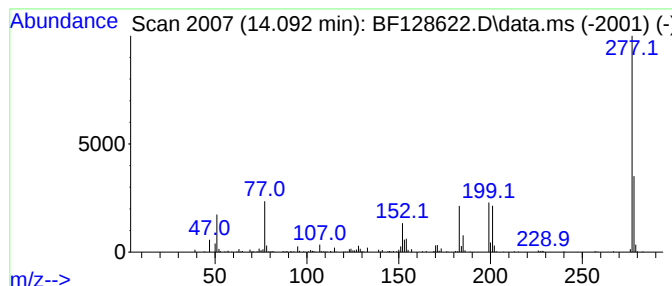

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF060122\
Data File : BF128622.D
Acq On : 01 Jun 2022 13:50
Operator : CG\JU
Sample : N3099-01
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
20220417-COMPOSITE-F

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Triphenylphosph...	14.092	7.2	ng	275136	5	13.998	760045	20.0