

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF060122\
 Data File : BF128627.D
 Acq On : 01 Jun 2022 17:25
 Operator : CG\JU
 Sample : N2953-02
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 P043-SS001-1824-01

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052622.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF128627.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.375	182	185	200	rBV	21153	44937	1.92%	0.291%
2	5.493	541	545	560	rBV	1842383	2133481	91.01%	13.800%
3	6.504	714	717	727	rBV	1884678	2145066	91.50%	13.875%
4	6.575	727	729	732	rVB	62886	49444	2.11%	0.320%
5	6.834	769	773	776	rBV	807424	635841	27.12%	4.113%
6	7.398	863	869	872	rBV	1499851	1527811	65.17%	9.882%
7	8.116	987	991	994	rBV	939021	774490	33.04%	5.010%
8	9.192	1169	1174	1177	rBV	2894844	2344344	100.00%	15.164%
9	9.869	1285	1289	1292	rBV	1005608	774515	33.04%	5.010%
10	10.663	1419	1424	1427	rBV	1380202	1267013	54.05%	8.195%
11	11.351	1538	1541	1545	rBV	743704	636654	27.16%	4.118%
12	11.745	1605	1608	1611	rBV	50484	45000	1.92%	0.291%
13	11.880	1627	1631	1640	rBV2	46124	56438	2.41%	0.365%
14	12.939	1807	1811	1815	rBV	1776433	1611576	68.74%	10.424%
15	13.916	1971	1977	1986	rBV5	29089	81539	3.48%	0.527%
16	13.992	1986	1990	1994	rVB	636791	547537	23.36%	3.542%
17	14.092	2000	2007	2012	rBV	192224	210503	8.98%	1.362%
18	15.457	2234	2239	2244	rBV	474574	573771	24.47%	3.711%




Sum of corrected areas: 15459960

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF060122\
Data File : BF128627.D
Acq On : 01 Jun 2022 17:25
Operator : CG\JU
Sample : N2953-02
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
P043-SS001-1824-01

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

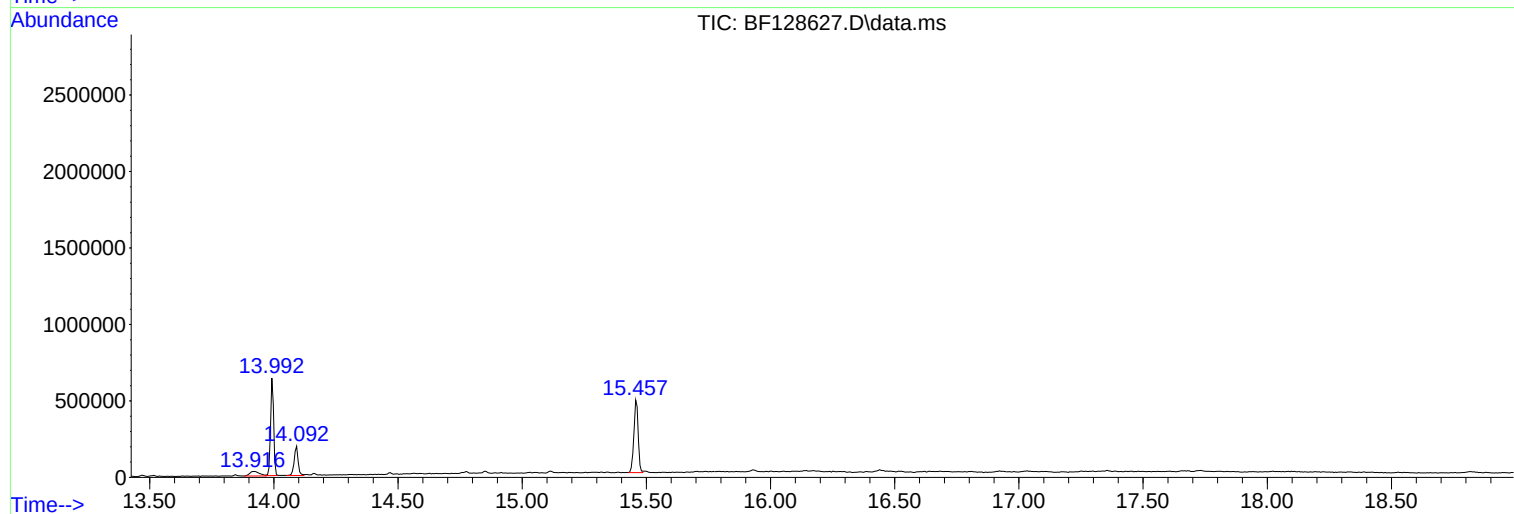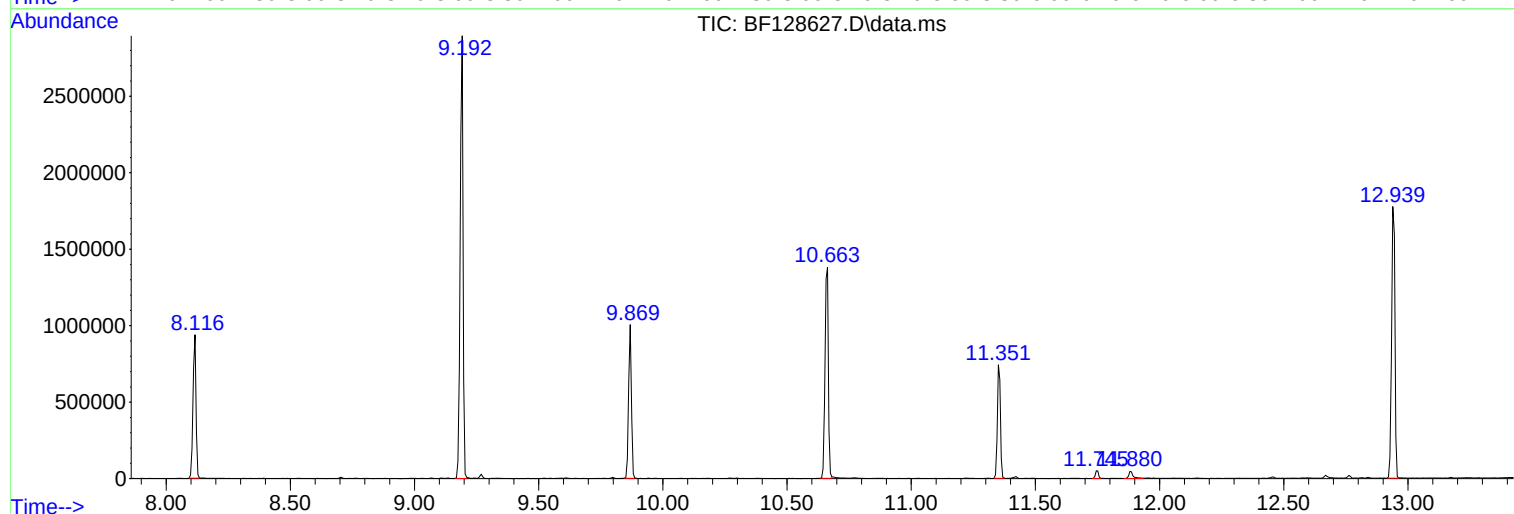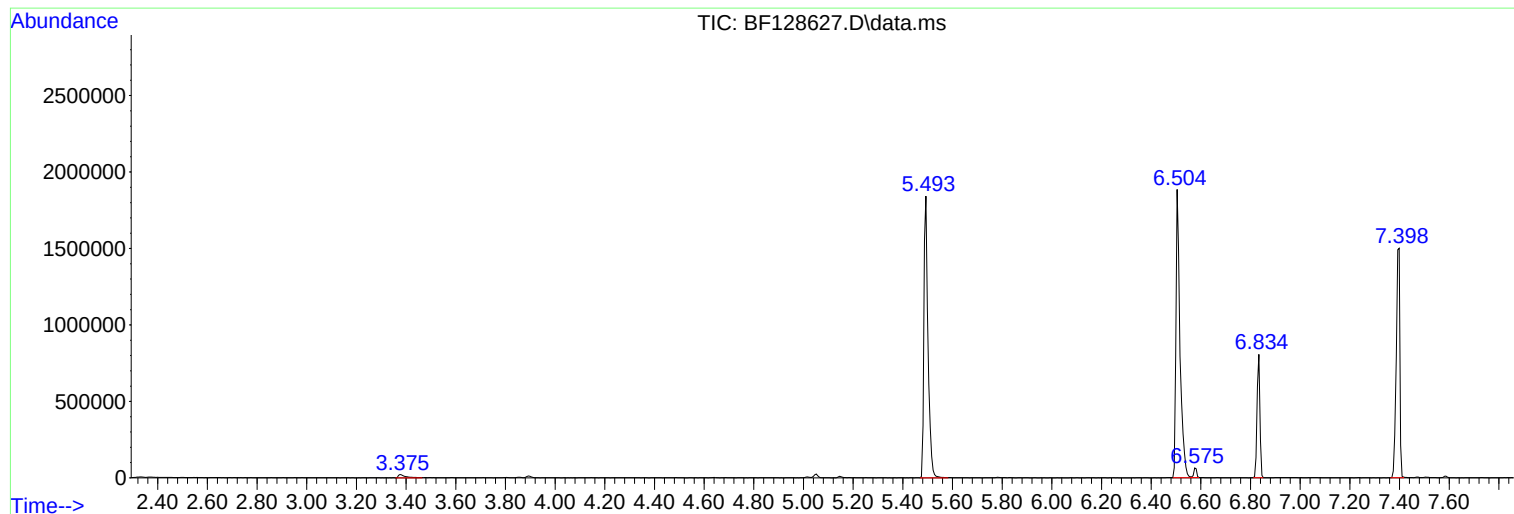

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF060122\
Data File : BF128627.D
Acq On : 01 Jun 2022 17:25
Operator : CG\JU
Sample : N2953-02
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
P043-SS001-1824-01










Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 1-Octadecanol Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
13.916	2.98 ng	81539	Chrysene-d12	13.992

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			1-Octadecanol	270	C18H38O	000112-92-5	76
2			Eicosyl methyl ether	312	C21H44O	1000406-29-4	76
3			Behenic alcohol	326	C22H46O	000661-19-8	74
4			Trifluoroacetoxy hexadecane	338	C18H33F3O2	006222-03-3	70
5			Heptafluorobutyric acid, hexadec...	438	C20H33F7O2	006385-15-5	70

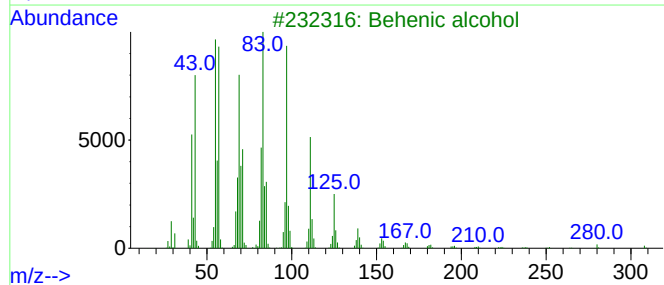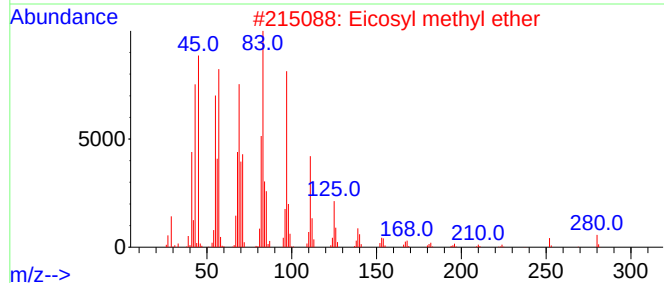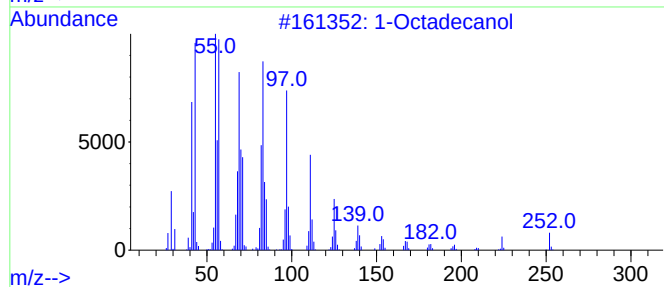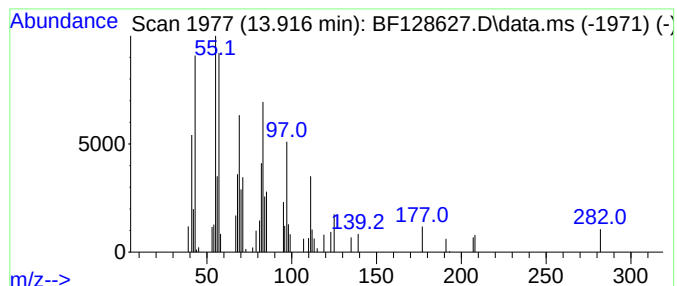

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF060122\
Data File : BF128627.D
Acq On : 01 Jun 2022 17:25
Operator : CG\JU
Sample : N2953-02
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
P043-SS001-1824-01










Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 Triphenylphosphine oxide Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
14.092	7.69 ng	210503	Chrysene-d12	13.992

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Triphenylphosphine oxide	278	C18H15OP	000791-28-6	97
2			(E)-7-Benzylidene-1-azabicyclo[3...	293	C15H19NO3S	1000483-83-4	91
3			Formaldehyde, (triphenylphosphor...	304	C19H17N2P	015990-54-2	45
4			3-(3,4-Dichlorophenyl)-2-thioxo...	277	C9H5Cl2NOS2	017046-34-3	43
5			Cobalt,(.eta.<5>-2,4-cyclopentad...	277	C16H15BCo	036682-12-9	38

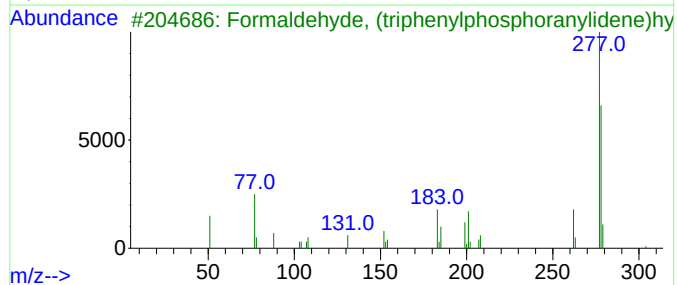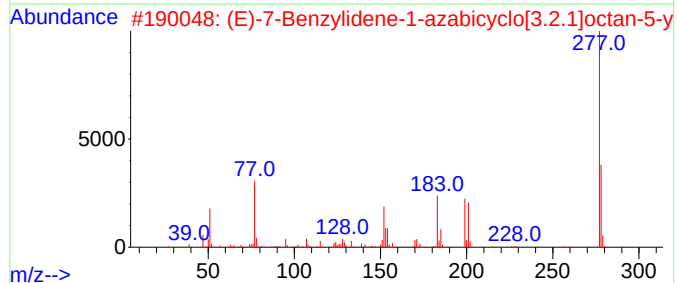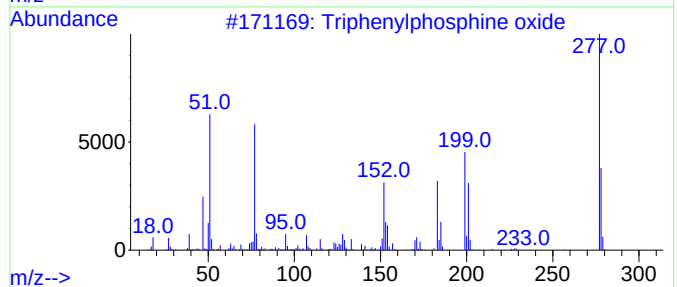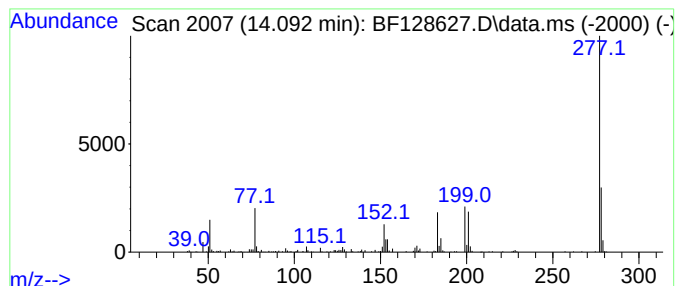

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF060122\
Data File : BF128627.D
Acq On : 01 Jun 2022 17:25
Operator : CG\JU
Sample : N2953-02
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
P043-SS001-1824-01

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
1-Octadecanol	13.916	3.0	ng	81539	5	13.992	547537	20.0
Triphenylphosph...	14.092	7.7	ng	210503	5	13.992	547537	20.0