
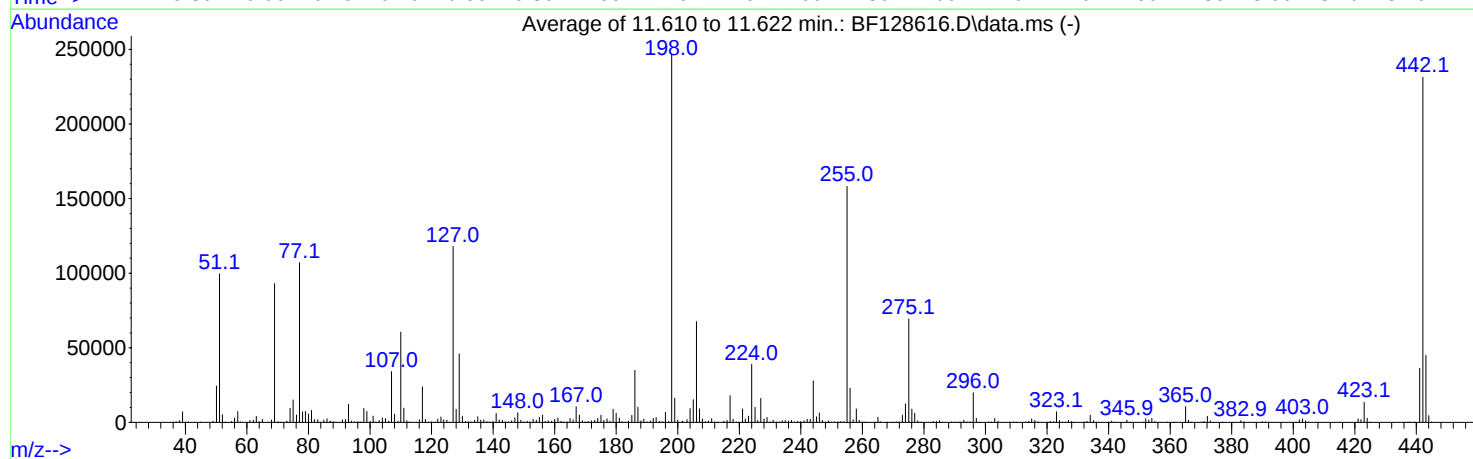


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF060122\
 Data File : BF128616.D
 Acq On : 01 Jun 2022 10:50
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052622.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri May 27 01:51:59 2022

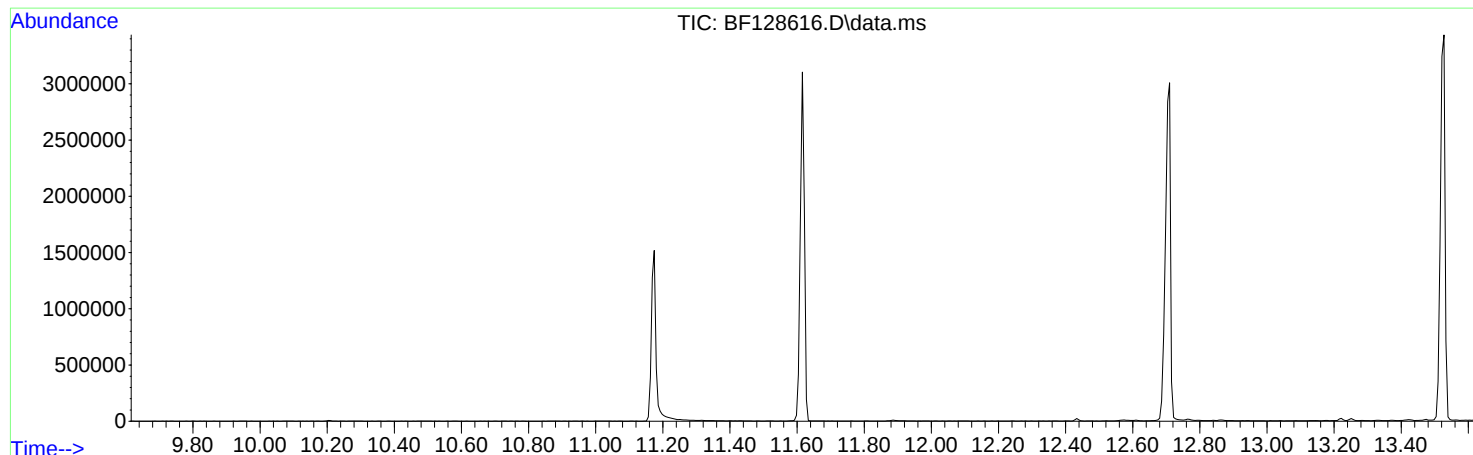




AutoFind: Scans 1585, 1586, 1587; Background Corrected with Scan 1579

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	40.4	99536	PASS
68	69	0.00	2	1.7	1618	PASS
69	198	0.00	100	37.7	92976	PASS
70	69	0.00	2	0.6	566	PASS
127	198	10	80	47.8	117819	PASS
197	198	0.00	2	0.3	680	PASS
198	198	100	100	100.0	246549	PASS
199	198	5	9	6.6	16151	PASS
275	198	10	60	28.1	69288	PASS
365	198	1	100	4.2	10465	PASS
441	198	0.01	100	14.7	36295	PASS
442	442	50	100	100.0	231371	PASS
443	442	15	24	19.4	44960	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF060122\
Data File : BF128616.D
Acq On : 01 Jun 2022 10:50
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jun 02 06:12:38 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri May 27 01:51:59 2022
Response via : Initial Calibration

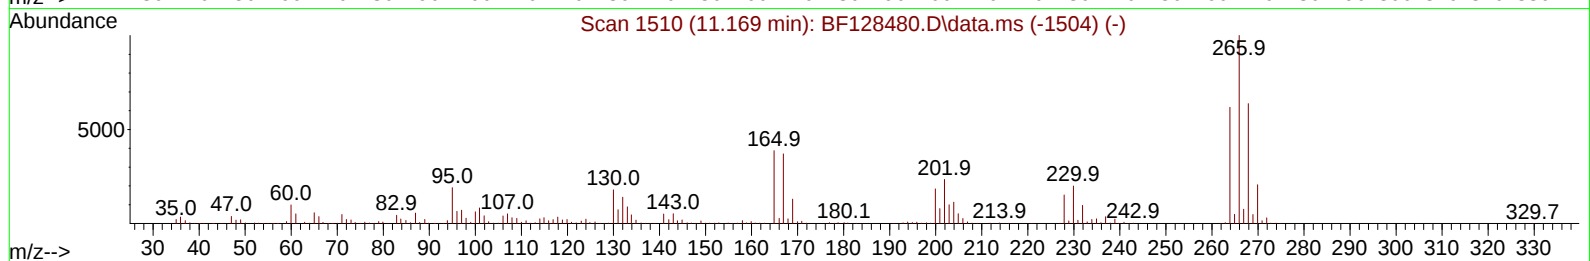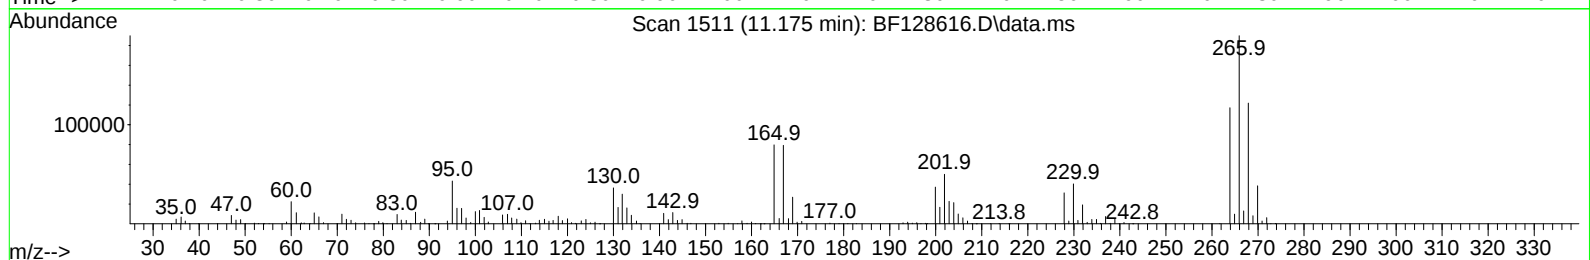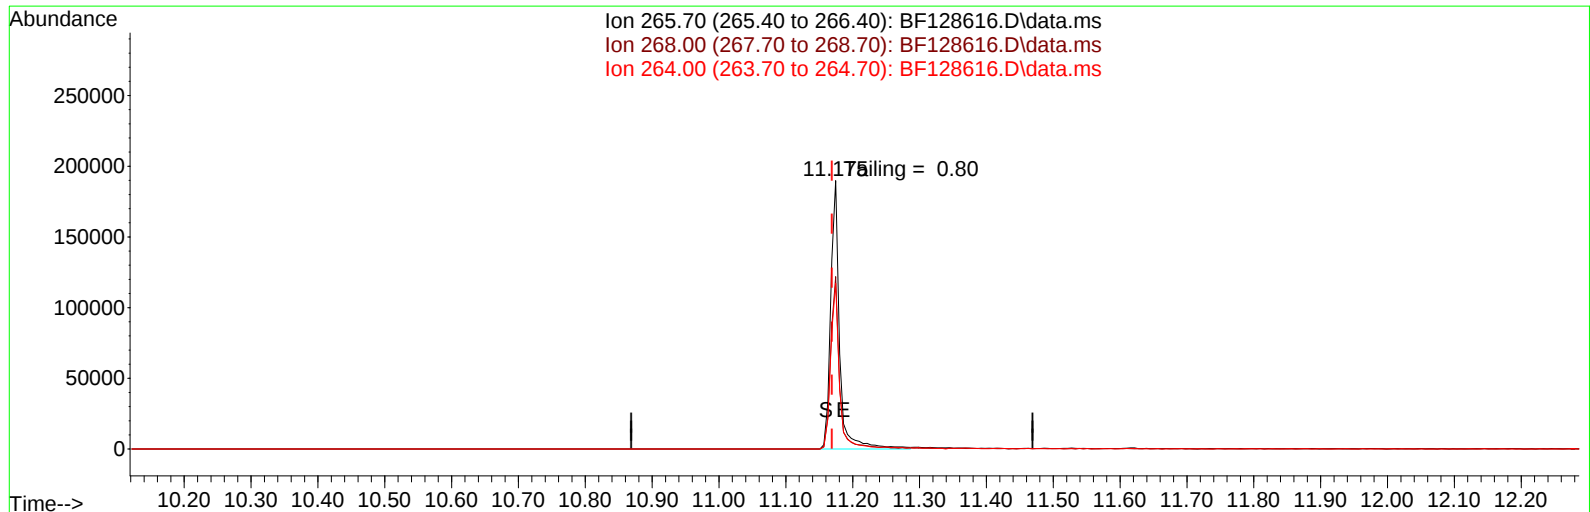

TIC: BF128616.D\data.ms

(70) Pentachlorophenol (C)

11.175min (+ 0.006) 22175.57 ng




response 177309

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.70	64.23
264.00	61.80	61.76
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF060122\
Data File : BF128616.D
Acq On : 01 Jun 2022 10:50
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jun 02 06:12:38 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri May 27 01:51:59 2022
Response via : Initial Calibration

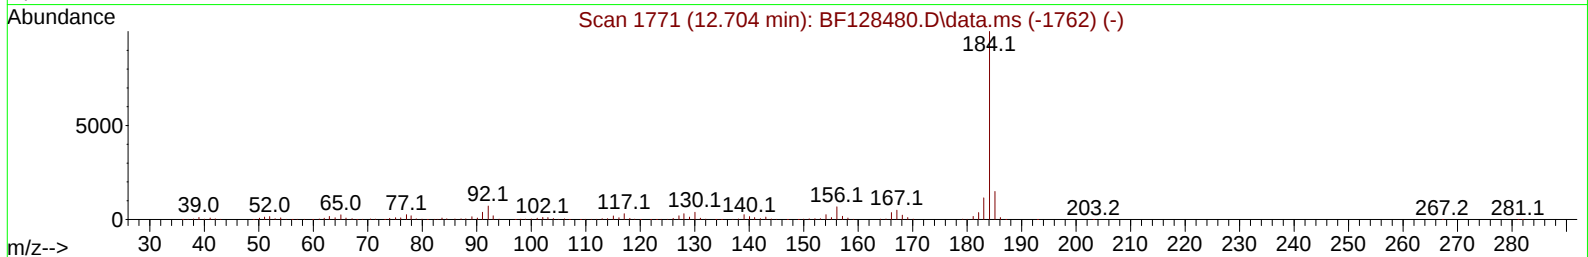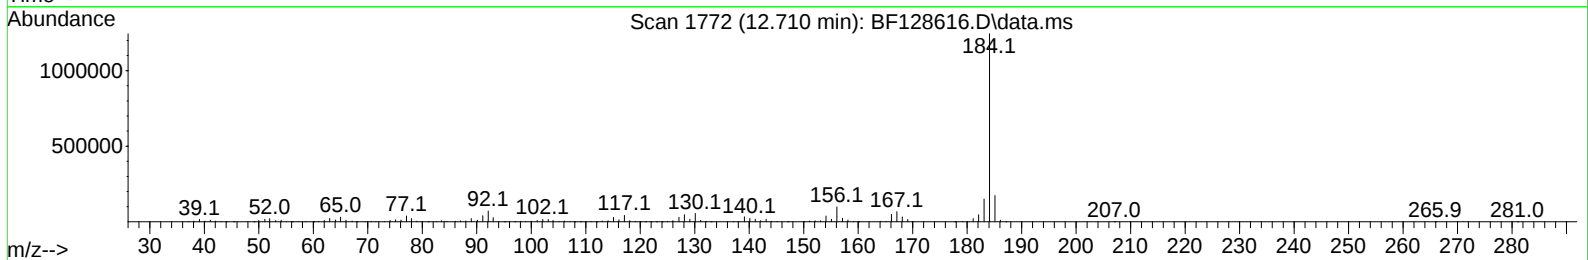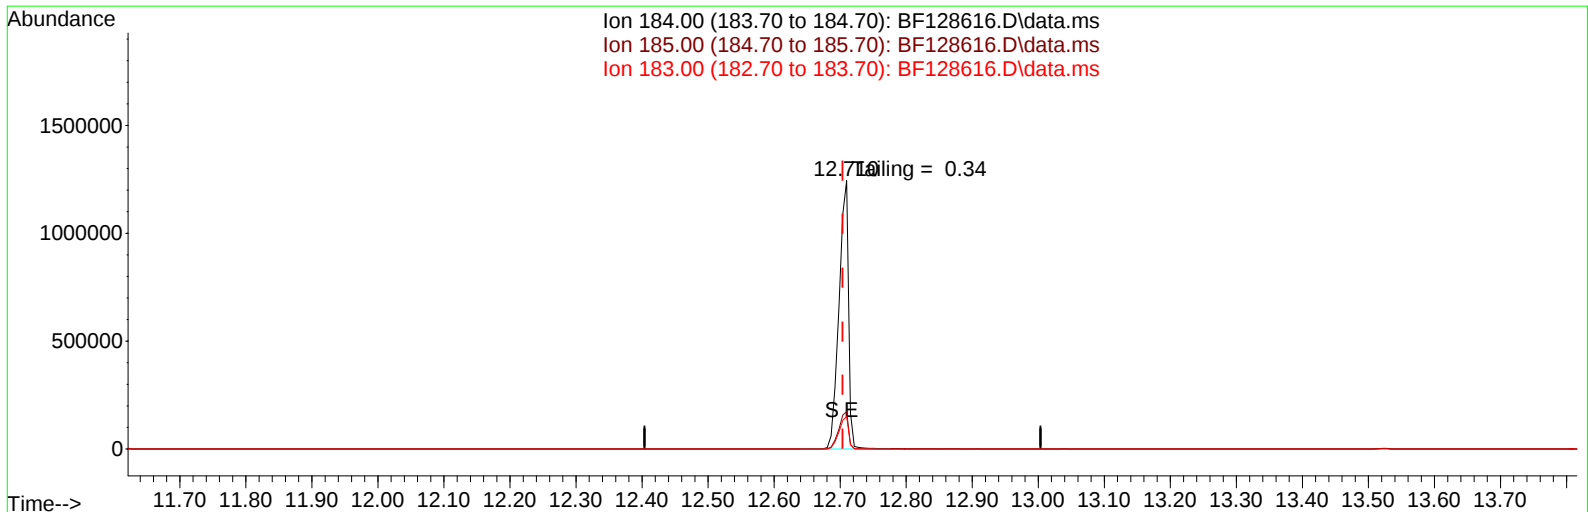

TIC: BF128616.D\data.ms

(77) Benzidine

12.710min (+ 0.006) 0.00 ng

response 1257659

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.90	13.95
183.00	11.60	12.10
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
6/1/2022	BNA_F	<u>BF128616.D</u>
Compound Name	Response	Retention Time
DDT	625769	13.527
DDD	6579	13.221
DDE	340	12.88
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
6919	632688	1.09

Instrument :
BNA_F
ClientSampleId :
DFTPP