
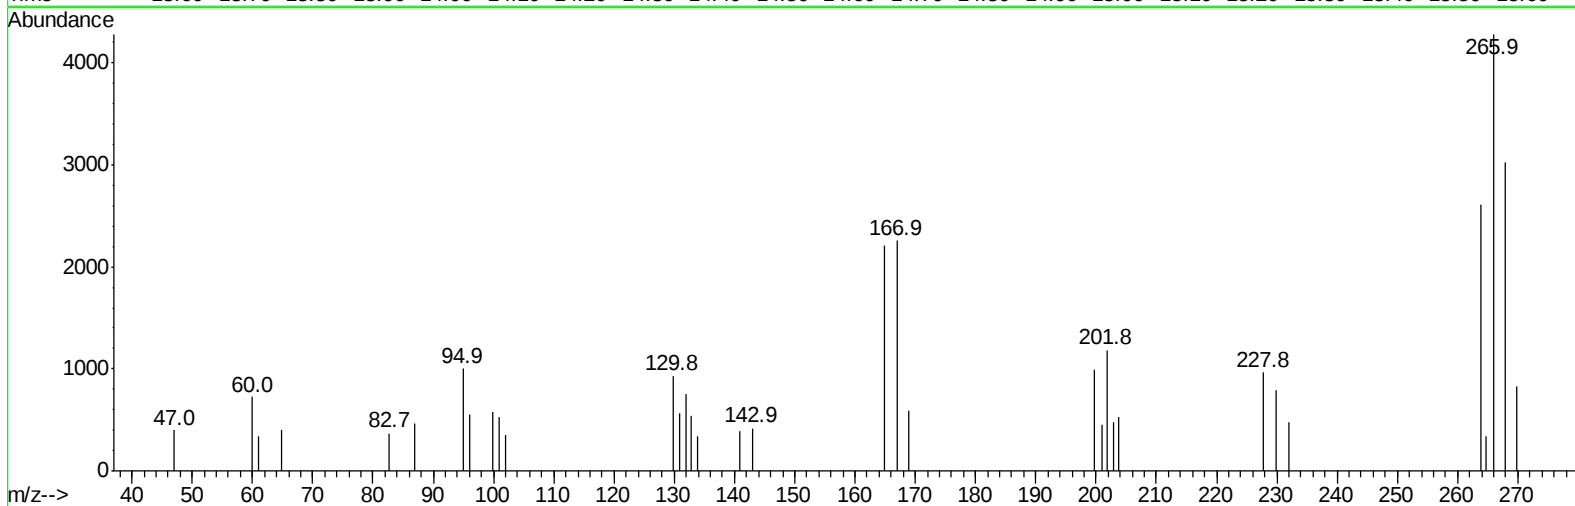


Data Path : Z:\HPCHEM1\BNA F\DATA\BF060217\
Data File : BF095654.D
Acq On : 3 Jun 2017 2:45
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 05 08:24:20 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF050217.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 01 18:51:16 2017
Response via : Initial Calibration

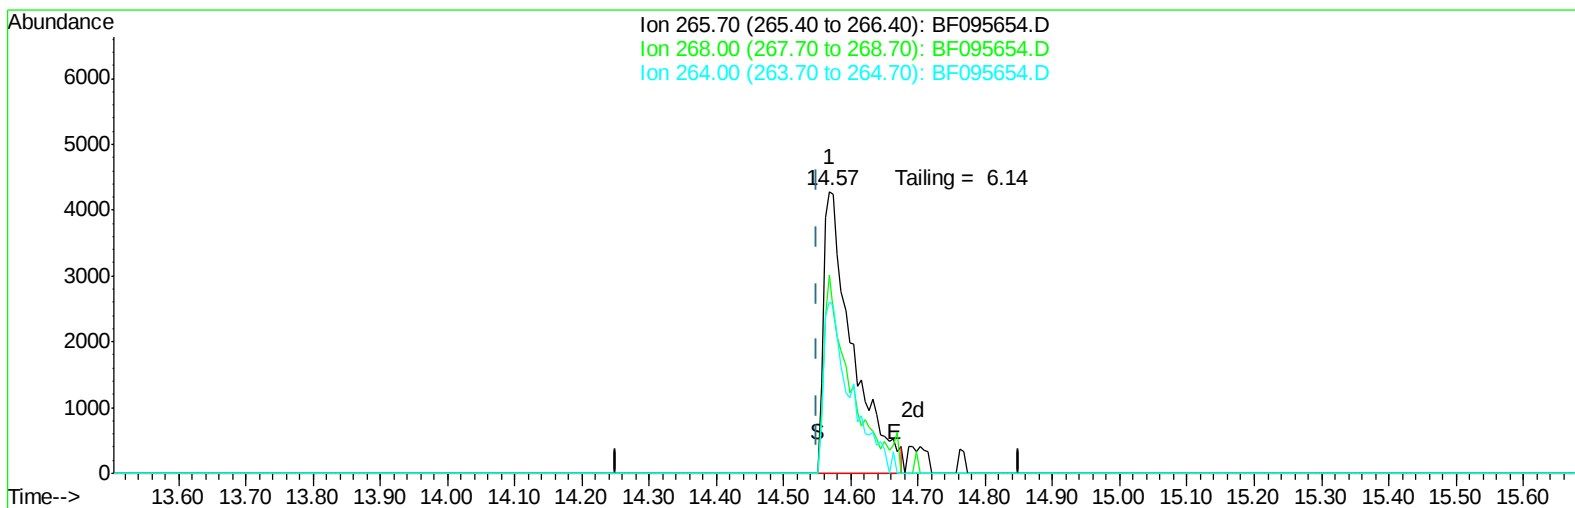

TIC: BF095654.D

(69) Pentachlorophenol (C)



14.568min (+0.017) 0.00ng

response 12697

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	70.62
264.00	64.60	61.07
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\DATA\BF060217\
Data File : BF095654.D
Acq On : 3 Jun 2017 2:45
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 05 08:24:20 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF050217.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 01 18:51:16 2017
Response via : Initial Calibration

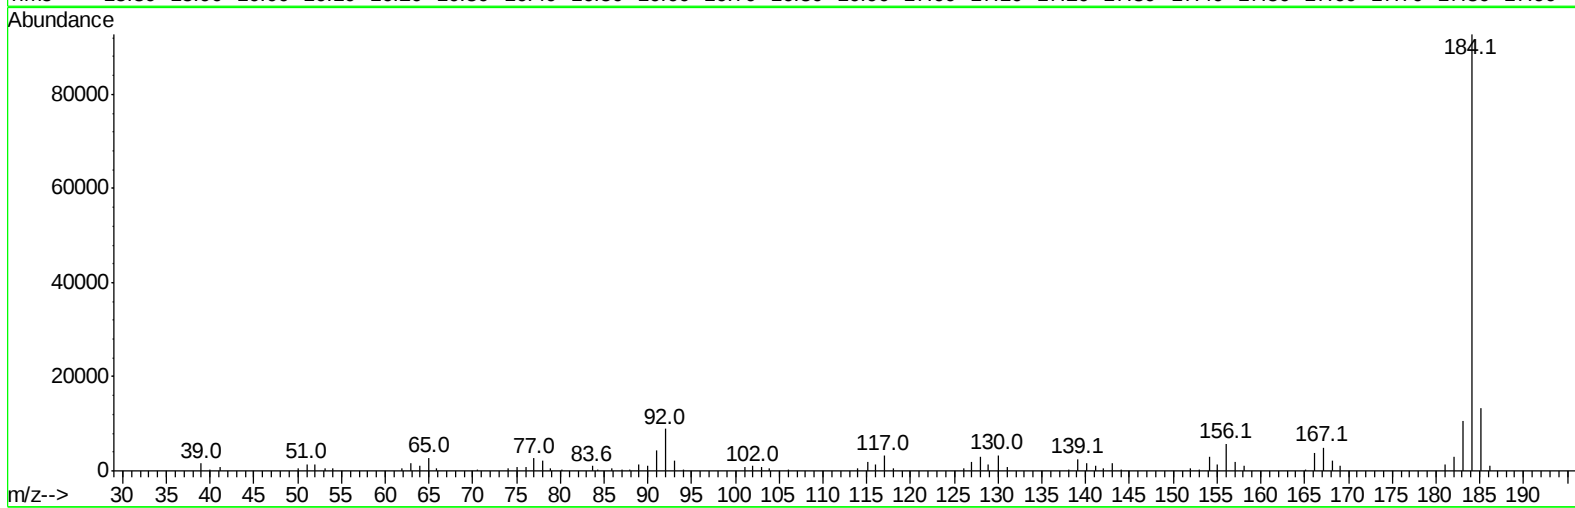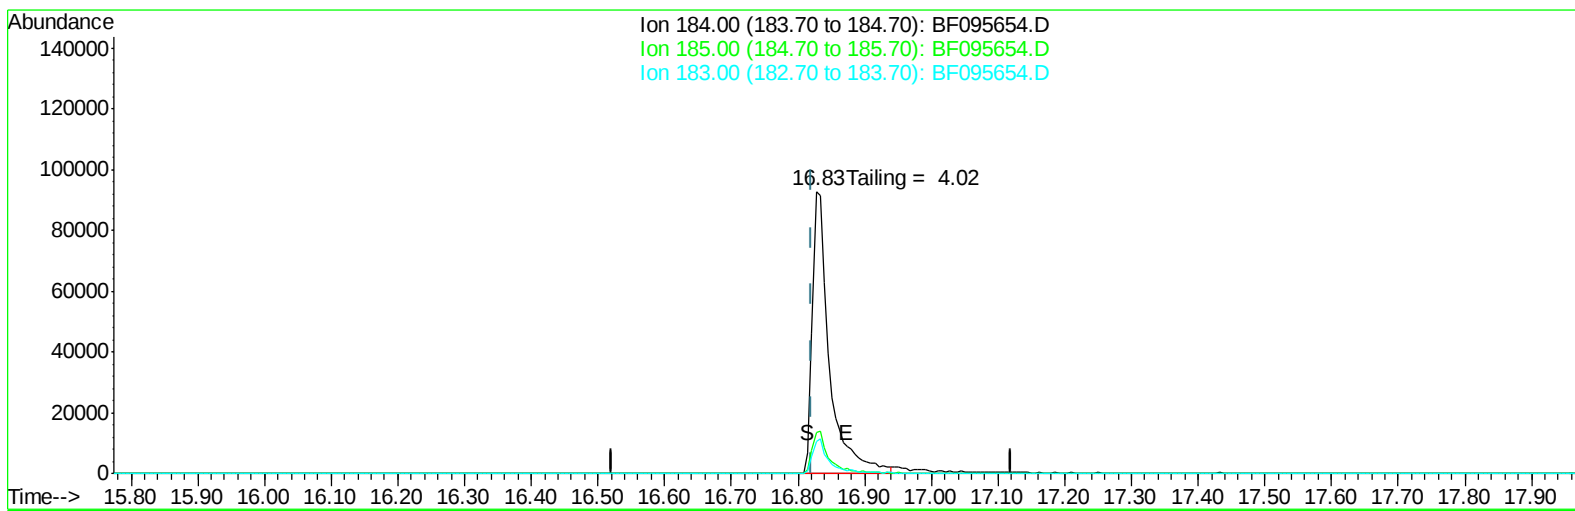

TIC: BF095654.D

(76) Benzidine

16.827min (+0.006) 0.00ng

response 165182

Ion	Exp%	Act%
184.00	100	100
185.00	19.40	14.38#
183.00	12.20	11.46
0.00	0.00	0.00