


Data Path : Z:\HPCHEM1\BNA F\Data\BF060217\
 Data File : BF095631.D
 Acq On : 2 Jun 2017 13:32
 Operator : SJ/MA
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF050217.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Jun 01 18:51:16 2017

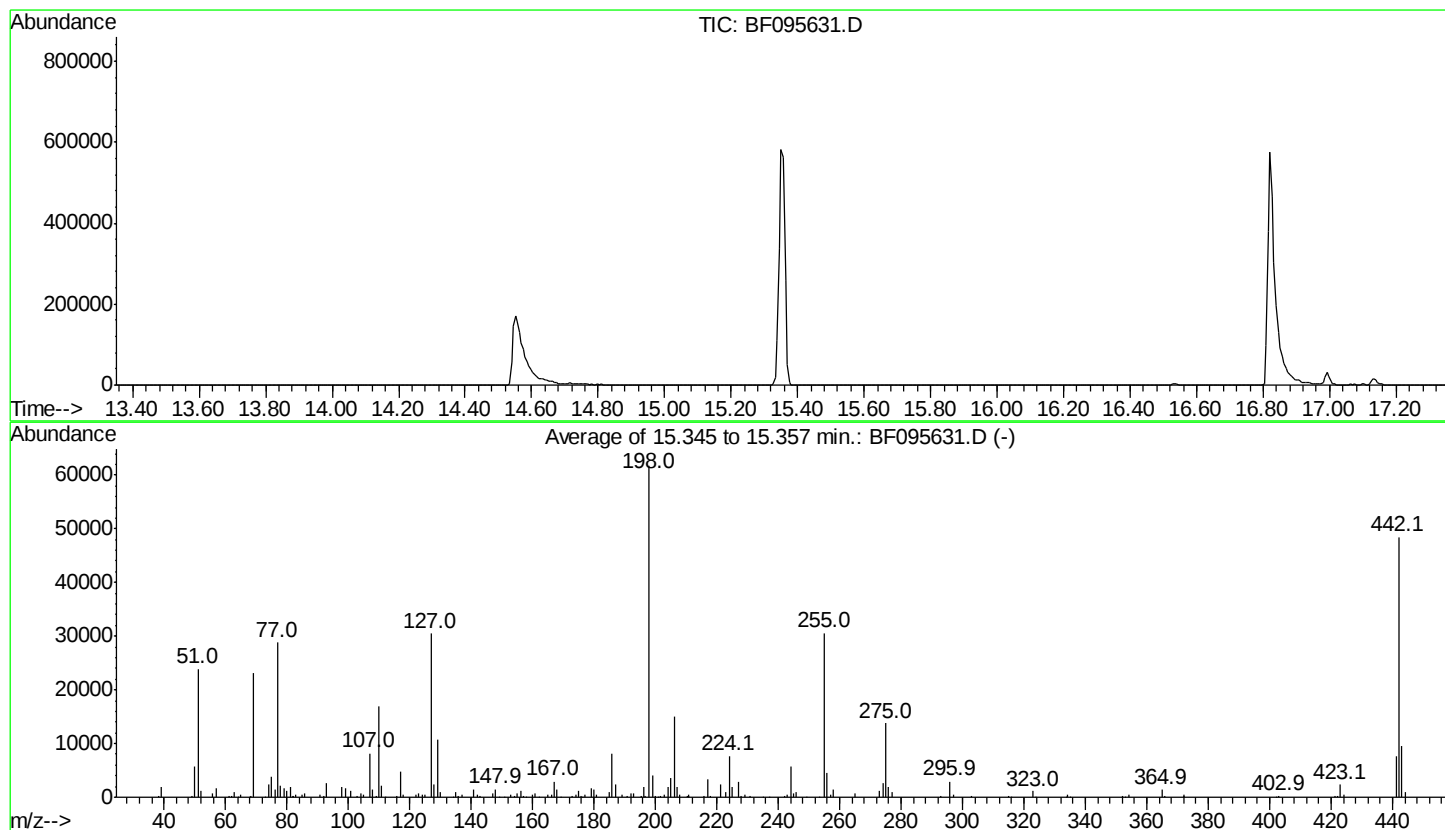

AutoFind: Scans 2322, 2323, 2324; Background Corrected with Scan 2316

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.7	23880	PASS
68	69	0.00	2	1.5	355	PASS
69	198	0.00	100	37.4	23101	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	49.4	30485	PASS
197	198	0.00	2	0.3	200	PASS
198	198	100	100	100.0	61760	PASS
199	198	5	9	6.6	4046	PASS
275	198	10	60	22.3	13761	PASS
365	198	1	100	2.2	1330	PASS
441	442	0.01	24	15.6	7581	PASS
442	198	50	100	78.6	48517	PASS
443	442	15	24	19.7	9544	PASS