
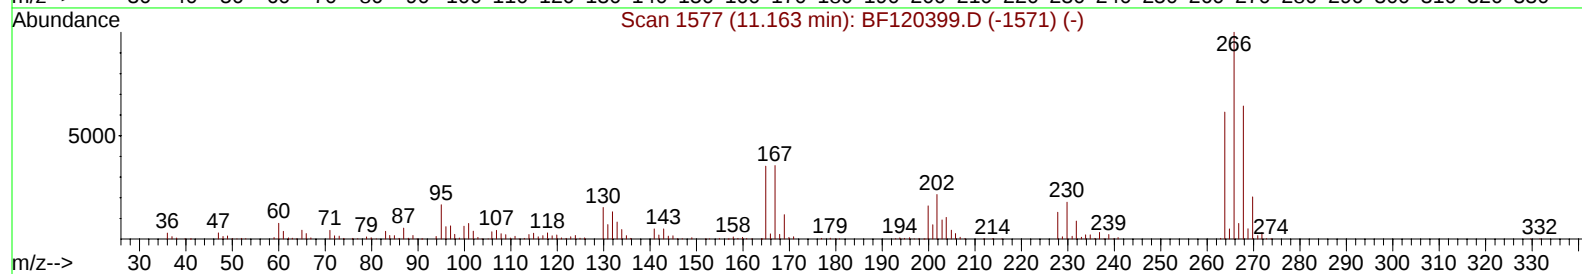
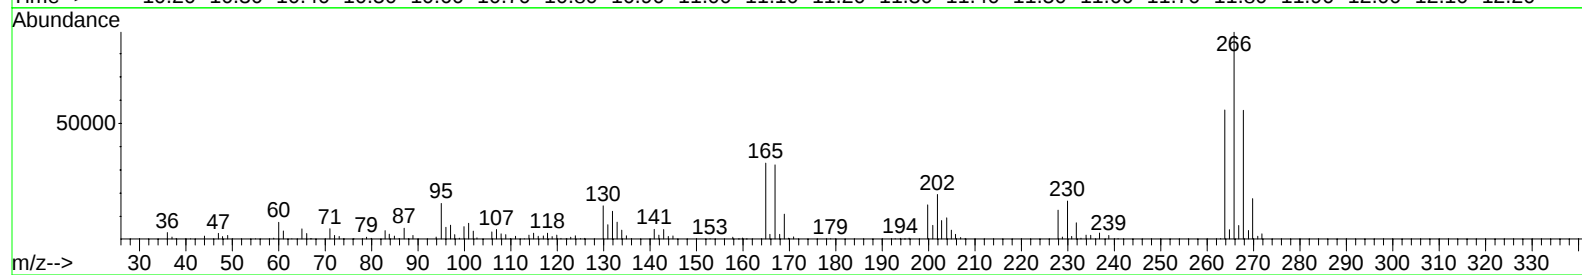


Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF060220\
 Data File : BF120484.D
 Acq On : 2 Jun 2020 10:12
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 02 11:57:49 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF052820.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jun 02 11:37:51 2020
 Response via : Initial Calibration

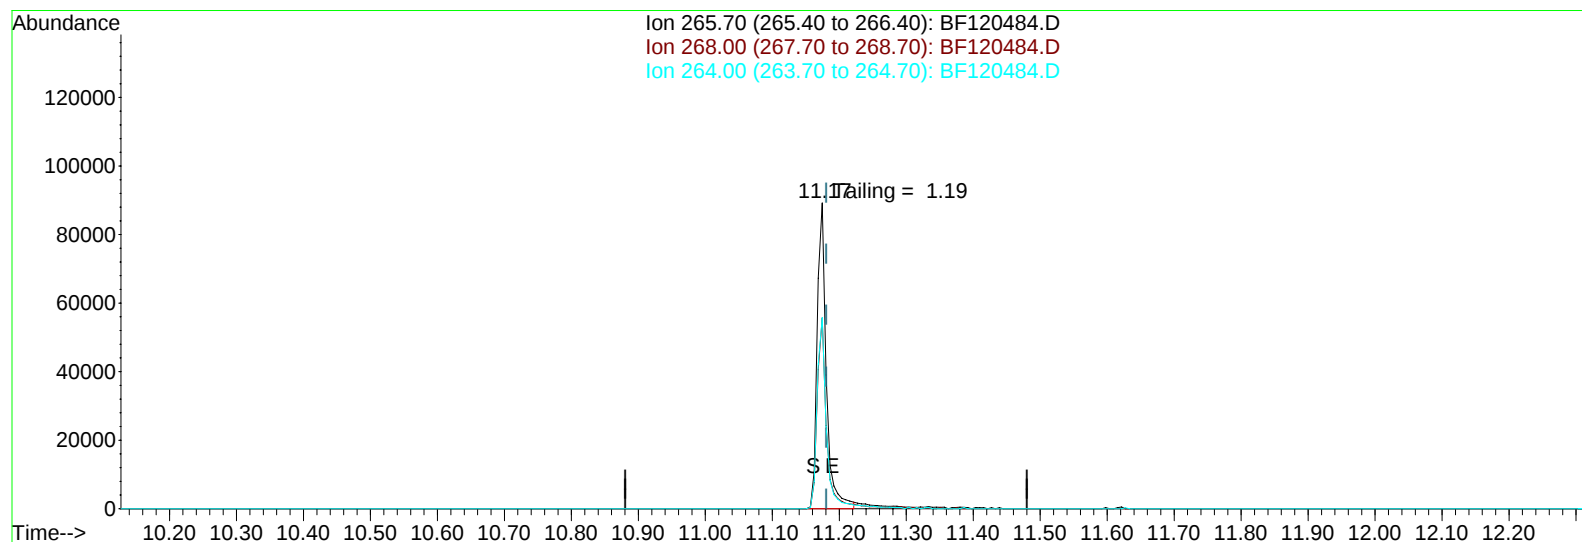

TIC: BF120484.D

(70) Pentachlorophenol (C)




11.174min (-0.006) 25600.19ng

response 89681

Ion	Exp%	Act%
265.70	100	100
268.00	64.70	62.37
264.00	63.50	62.49
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF060220\
 Data File : BF120484.D
 Acq On : 2 Jun 2020 10:12
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 02 11:57:49 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF052820.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jun 02 11:37:51 2020
 Response via : Initial Calibration

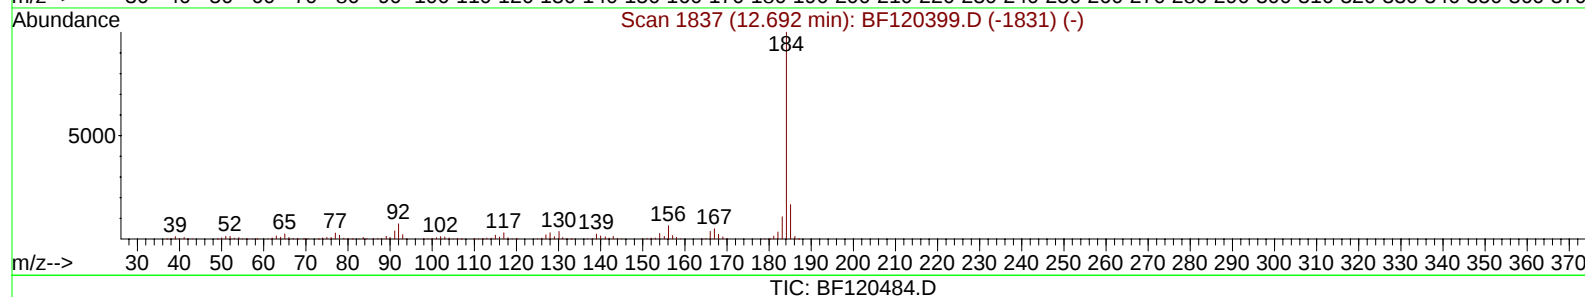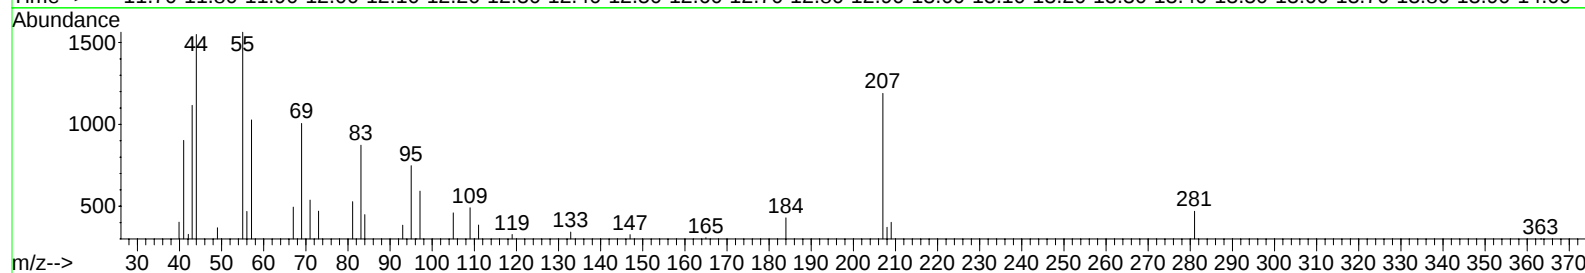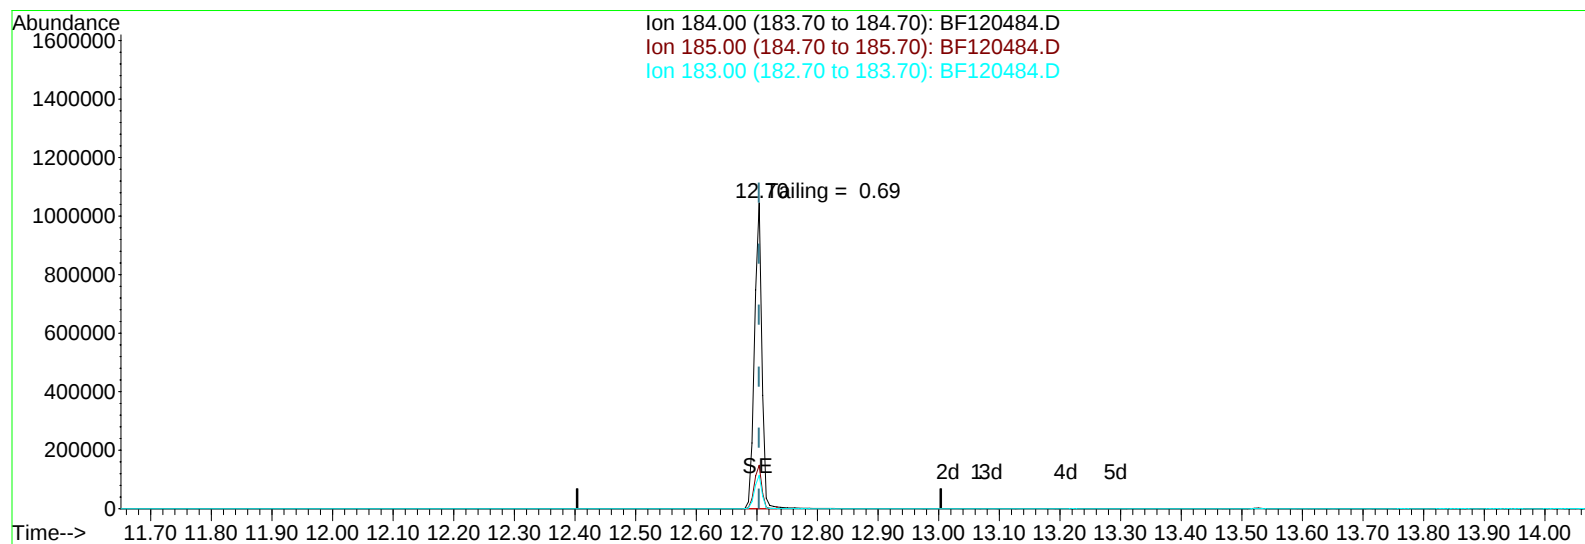

(77) Benzidine

13.063min (+0.359) 173.08ng

response 573

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	0.00#
183.00	11.20	0.00#
0.00	0.00	0.00